

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022202.D
 Acq On : 17 Sep 2021 22:18
 Operator : SY/MD
 Sample : M3676-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022202.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rBV	102201	103965	10.09%	1.195%
2	1.565	156	163	178	rVB	103211	116693	11.33%	1.341%
3	2.105	321	331	354	rBV2	231882	359189	34.88%	4.128%
4	2.706	515	518	520	rVB2	370	183	0.02%	0.002%
5	2.957	594	596	598	rVV	349	159	0.02%	0.002%
6	2.982	602	604	607	rVB2	387	193	0.02%	0.002%
7	3.121	645	647	650	rBV	250	154	0.01%	0.002%
8	3.137	650	652	660	rVB3	386	417	0.04%	0.005%
9	3.188	660	668	671	rBV4	915	1224	0.12%	0.014%
10	3.240	681	684	687	rBV	193	142	0.01%	0.002%
11	3.445	744	748	750	rBV	223	198	0.02%	0.002%
12	3.555	780	782	786	rVB	262	125	0.01%	0.001%
13	3.642	805	809	813	rBV2	305	263	0.03%	0.003%
14	3.908	880	892	922	rBV	79359	285083	27.68%	3.276%
15	4.349	1014	1029	1059	rBV	163553	410661	39.87%	4.720%
16	4.603	1098	1108	1111	rBV3	4738	6458	0.63%	0.074%
17	4.687	1131	1134	1135	rBV	372	171	0.02%	0.002%
18	4.716	1141	1143	1145	rBV	417	223	0.02%	0.003%
19	4.780	1159	1163	1165	rBV2	297	256	0.02%	0.003%
20	4.834	1178	1180	1184	rBV2	388	216	0.02%	0.002%
21	4.857	1184	1187	1189	rBV	209	130	0.01%	0.001%
22	4.921	1202	1207	1211	rVB2	372	335	0.03%	0.004%
23	4.944	1211	1214	1217	rBV2	289	223	0.02%	0.003%
24	4.992	1227	1229	1230	rBV	275	127	0.01%	0.001%
25	5.047	1230	1246	1282	rVV2	410207	1029929	100.00%	11.837%
26	5.291	1321	1322	1326	rVB2	472	241	0.02%	0.003%
27	5.349	1337	1340	1346	rVB2	618	549	0.05%	0.006%
28	5.375	1346	1348	1351	rBV2	501	284	0.03%	0.003%
29	5.461	1372	1375	1378	rBV2	349	290	0.03%	0.003%
30	5.497	1384	1386	1389	rVB2	406	208	0.02%	0.002%
31	5.516	1390	1392	1395	rVB	410	204	0.02%	0.002%
32	5.542	1398	1400	1403	rBV	223	165	0.02%	0.002%
33	5.558	1403	1405	1410	rVB2	341	212	0.02%	0.002%
34	5.619	1410	1424	1449	rBV	328004	668758	64.93%	7.686%
35	5.915	1501	1516	1551	rBV2	422536	854446	82.96%	9.820%
36	6.072	1553	1565	1585	rBV	231004	464538	45.10%	5.339%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022202.D
 Acq On : 17 Sep 2021 22:18
 Operator : SY/MD
 Sample : M3676-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.269	1624	1626	1628	rBV2	448	205	0.02%	0.002%
38	6.314	1635	1640	1647	rVB5	410	497	0.05%	0.006%
39	6.400	1665	1667	1673	rVB4	478	370	0.04%	0.004%
40	6.426	1673	1675	1676	rBV4	266	138	0.01%	0.002%
41	6.513	1699	1702	1707	rVB2	340	248	0.02%	0.003%
42	6.539	1707	1710	1711	rBV2	272	172	0.02%	0.002%
43	6.738	1769	1772	1778	rBV2	328	227	0.02%	0.003%
44	6.767	1778	1781	1786	rVV2	314	289	0.03%	0.003%
45	6.789	1786	1788	1791	rVB2	390	223	0.02%	0.003%
46	6.841	1798	1804	1808	rBV3	345	329	0.03%	0.004%
47	6.896	1818	1821	1824	rBV	179	134	0.01%	0.002%
48	6.989	1839	1850	1870	rBV	111770	206085	20.01%	2.368%
49	7.121	1889	1891	1893	rBV2	482	167	0.02%	0.002%
50	7.320	1938	1953	1971	rBV	463626	810398	78.68%	9.314%
51	7.625	2039	2048	2068	rBV	75888	132758	12.89%	1.526%
52	7.805	2102	2104	2108	rBV3	328	185	0.02%	0.002%
53	7.850	2114	2118	2119	rBV2	471	282	0.03%	0.003%
54	7.889	2128	2130	2135	rBV2	327	181	0.02%	0.002%
55	7.937	2140	2145	2152	rBV3	758	976	0.09%	0.011%
56	8.095	2184	2194	2231	rBV2	258406	521591	50.64%	5.995%
57	8.532	2327	2330	2337	rVB3	425	426	0.04%	0.005%
58	8.587	2345	2347	2349	rBV2	242	138	0.01%	0.002%
59	8.686	2376	2378	2384	rBV2	407	342	0.03%	0.004%
60	8.715	2384	2387	2390	rVV3	320	234	0.02%	0.003%
61	8.738	2392	2394	2397	rVV	336	180	0.02%	0.002%
62	8.757	2398	2400	2403	rVB2	413	254	0.02%	0.003%
63	8.854	2416	2430	2453	rBV	493758	802036	77.87%	9.218%
64	9.072	2496	2498	2502	rVB4	468	287	0.03%	0.003%
65	9.114	2509	2511	2514	rBV2	308	169	0.02%	0.002%
66	9.149	2514	2522	2526	rBV5	1163	1475	0.14%	0.017%
67	9.236	2544	2549	2555	rVB3	415	490	0.05%	0.006%
68	9.262	2555	2557	2561	rVB3	274	128	0.01%	0.001%
69	9.288	2561	2565	2570	rBV2	444	412	0.04%	0.005%
70	9.551	2642	2647	2649	rBV2	612	552	0.05%	0.006%
71	9.641	2672	2675	2677	rBV2	270	185	0.02%	0.002%
72	9.690	2687	2690	2693	rBV	299	198	0.02%	0.002%
73	9.828	2730	2733	2737	rBV3	376	285	0.03%	0.003%
74	10.130	2815	2827	2836	rBV4	1444	2702	0.26%	0.031%
75	10.217	2842	2854	2875	rBV	305617	483552	46.95%	5.557%
76	10.336	2890	2891	2896	rBV2	252	168	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022202.D
 Acq On : 17 Sep 2021 22:18
 Operator : SY/MD
 Sample : M3676-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.410	2912	2914	2919	rBV2	243	134	0.01%	0.002%
78	10.445	2924	2925	2928	rVB3	392	171	0.02%	0.002%
79	10.474	2931	2934	2938	rBV2	310	249	0.02%	0.003%
80	10.545	2951	2956	2960	rBV4	418	459	0.04%	0.005%
81	10.580	2965	2967	2969	rBV	437	221	0.02%	0.003%
82	10.651	2987	2989	2993	rBV2	207	181	0.02%	0.002%
83	10.764	3023	3024	3029	rVB	239	150	0.01%	0.002%
84	10.924	3066	3074	3078	rBV5	1650	2003	0.19%	0.023%
85	11.088	3122	3125	3129	rBV2	223	170	0.02%	0.002%
86	11.143	3138	3142	3152	rVB7	829	1220	0.12%	0.014%
87	11.252	3165	3176	3194	rBV	452978	708572	68.80%	8.143%
88	11.526	3258	3261	3262	rBV	268	148	0.01%	0.002%
89	11.625	3280	3292	3315	rBV	447406	708926	68.83%	8.147%
90	11.841	3356	3359	3360	rBV2	322	191	0.02%	0.002%
91	11.899	3373	3377	3379	rBV2	262	255	0.02%	0.003%
92	12.268	3488	3492	3495	rBV	244	161	0.02%	0.002%
93	12.480	3556	3558	3561	rBV	263	135	0.01%	0.002%
94	12.918	3691	3694	3698	rBV2	349	337	0.03%	0.004%
95	13.152	3766	3767	3770	rBV	340	155	0.02%	0.002%
96	13.474	3864	3867	3869	rBV2	397	238	0.02%	0.003%
97	13.519	3879	3881	3884	rBV2	481	230	0.02%	0.003%
98	13.699	3933	3937	3939	rBV	232	170	0.02%	0.002%
99	13.779	3960	3962	3966	rVB2	371	159	0.02%	0.002%
100	14.603	4214	4218	4219	rBV2	422	239	0.02%	0.003%




Sum of corrected areas: 8701154

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022202.D
Acq On : 17 Sep 2021 22:18
Operator : SY/MD
Sample : M3676-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

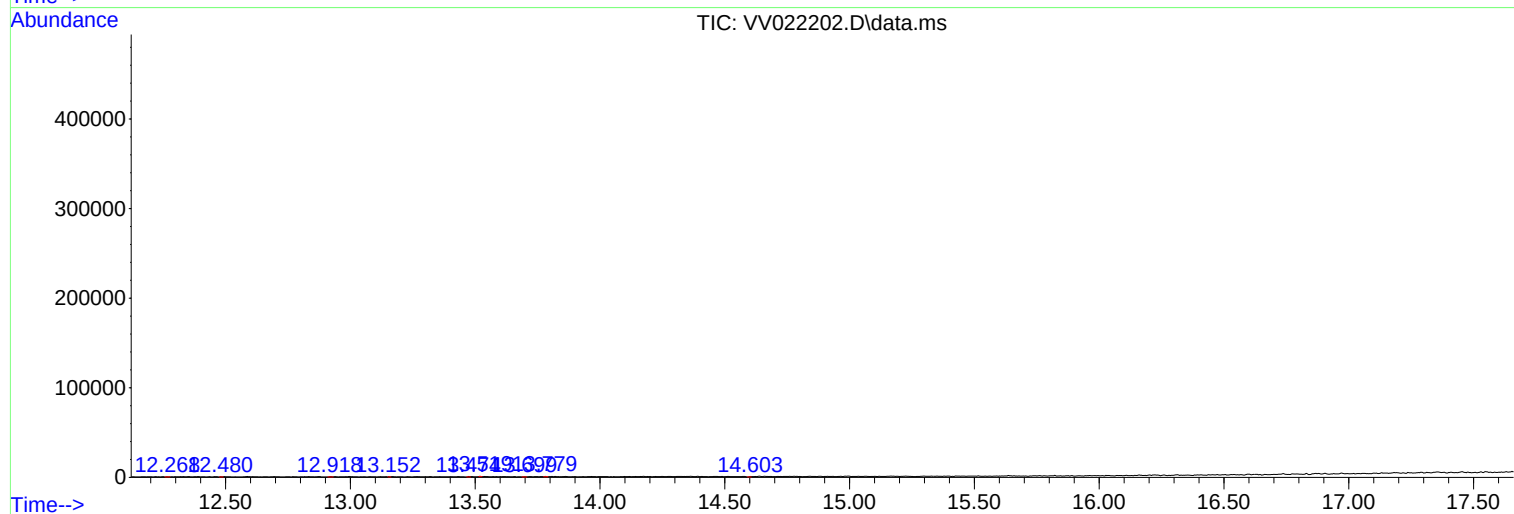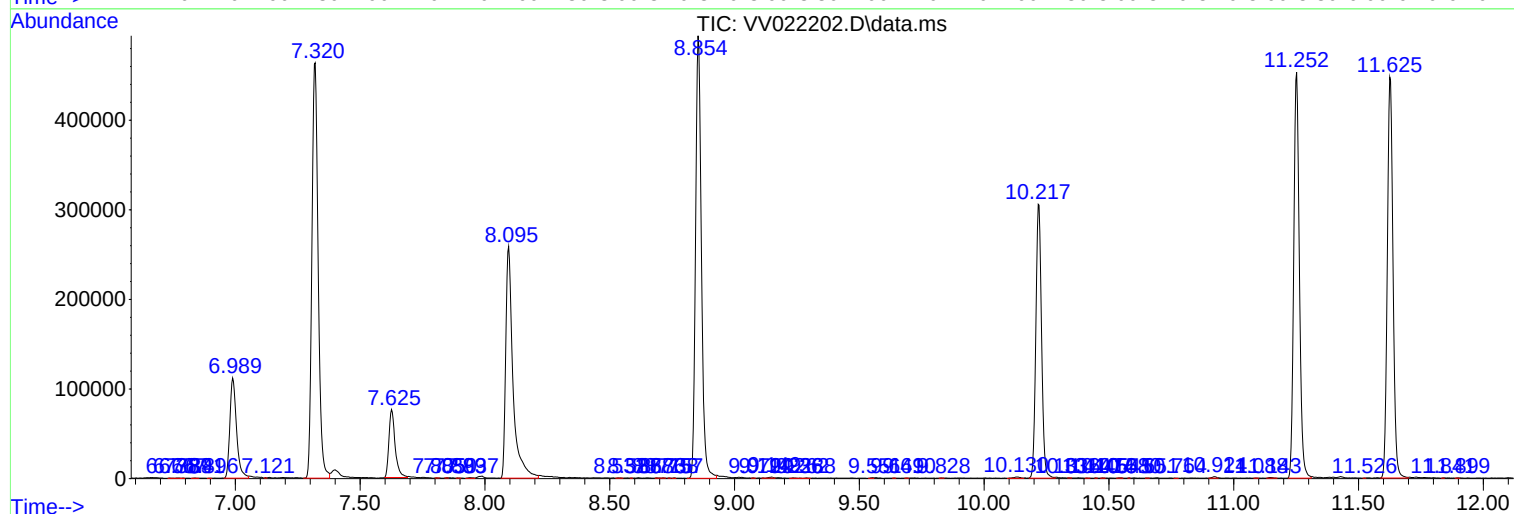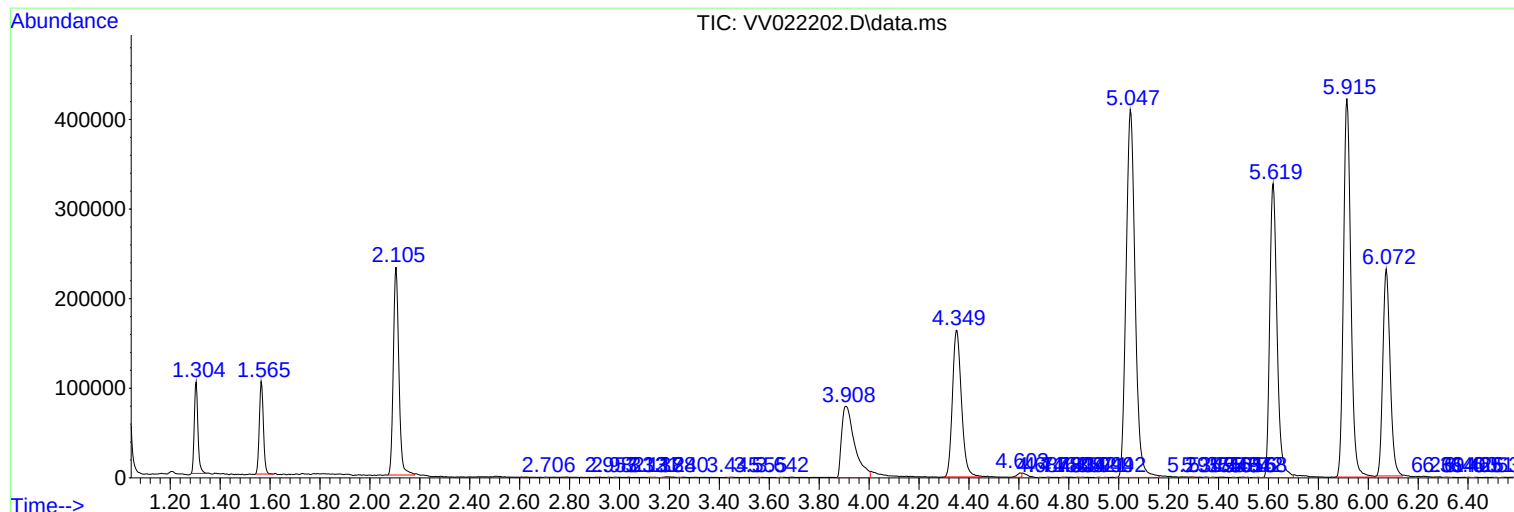

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022202.D
Acq On : 17 Sep 2021 22:18
Operator : SY/MD
Sample : M3676-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022202.D
Acq On : 17 Sep 2021 22:18
Operator : SY/MD
Sample : M3676-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------