

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022205.D
 Acq On : 17 Sep 2021 23:30
 Operator : SY/MD
 Sample : M3787-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022205.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rBV	174494	184449	15.42%	2.085%
2	1.568	156	164	180	rVB	143817	165383	13.83%	1.870%
3	2.105	321	331	345	rBV	305285	439227	36.72%	4.966%
4	2.860	564	566	573	rVB2	348	193	0.02%	0.002%
5	2.889	573	575	580	rBV2	372	253	0.02%	0.003%
6	3.310	700	706	710	rBV	278	324	0.03%	0.004%
7	3.391	727	731	734	rVB2	210	125	0.01%	0.001%
8	3.410	734	737	739	rBV	214	156	0.01%	0.002%
9	3.458	750	752	758	rBV4	229	165	0.01%	0.002%
10	3.487	758	761	764	rVB2	325	181	0.02%	0.002%
11	3.632	804	806	811	rVB3	362	234	0.02%	0.003%
12	3.789	852	855	858	rBV2	155	131	0.01%	0.001%
13	3.844	869	872	876	rVB	274	133	0.01%	0.002%
14	3.902	876	890	932	rBV	77705	275548	23.04%	3.115%
15	4.352	1012	1030	1063	rBV	186520	464417	38.83%	5.250%
16	4.558	1091	1094	1102	rVB4	658	824	0.07%	0.009%
17	4.625	1113	1115	1119	rVB4	442	260	0.02%	0.003%
18	4.651	1119	1123	1125	rBV3	559	374	0.03%	0.004%
19	4.680	1130	1132	1133	rBV3	407	140	0.01%	0.002%
20	4.709	1138	1141	1142	rBV2	253	157	0.01%	0.002%
21	4.748	1152	1153	1158	rVB2	477	191	0.02%	0.002%
22	4.793	1164	1167	1169	rBV2	240	162	0.01%	0.002%
23	4.821	1174	1176	1179	rVB2	343	157	0.01%	0.002%
24	4.841	1179	1182	1183	rBV	354	127	0.01%	0.001%
25	4.940	1211	1213	1216	rVB	266	174	0.01%	0.002%
26	5.047	1230	1246	1293	rBV2	473128	1196162	100.00%	13.523%
27	5.268	1311	1315	1320	rVB2	635	638	0.05%	0.007%
28	5.336	1334	1336	1337	rBV2	375	148	0.01%	0.002%
29	5.394	1350	1354	1357	rBV3	307	140	0.01%	0.002%
30	5.410	1357	1359	1360	rBV	314	153	0.01%	0.002%
31	5.503	1386	1388	1391	rVB	259	136	0.01%	0.002%
32	5.526	1393	1395	1398	rBV2	386	209	0.02%	0.002%
33	5.619	1412	1424	1454	rBV	351334	710439	59.39%	8.032%
34	5.847	1493	1495	1498	rBV2	564	314	0.03%	0.004%
35	5.908	1503	1514	1536	rVB5	27741	62639	5.24%	0.708%
36	6.072	1548	1565	1594	rBV	260313	534657	44.70%	6.045%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022205.D
 Acq On : 17 Sep 2021 23:30
 Operator : SY/MD
 Sample : M3787-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.272	1624	1627	1629	rBV2	660	362	0.03%	0.004%
38	6.403	1664	1668	1669	rBV2	233	153	0.01%	0.002%
39	6.513	1698	1702	1708	rBV3	259	241	0.02%	0.003%
40	6.538	1708	1710	1713	rBV2	316	231	0.02%	0.003%
41	6.577	1718	1722	1724	rBV3	272	154	0.01%	0.002%
42	6.609	1729	1732	1734	rBV2	350	219	0.02%	0.002%
43	6.645	1740	1743	1747	rVB2	195	168	0.01%	0.002%
44	6.712	1762	1764	1767	rVB2	288	134	0.01%	0.002%
45	6.741	1771	1773	1775	rBV	300	134	0.01%	0.002%
46	6.989	1838	1850	1881	rBV	126959	240733	20.13%	2.722%
47	7.214	1918	1920	1924	rVB3	499	227	0.02%	0.003%
48	7.272	1935	1938	1940	rBV2	221	141	0.01%	0.002%
49	7.317	1940	1952	1971	rBV	536453	944229	78.94%	10.675%
50	7.625	2037	2048	2080	rBV	86912	159146	13.30%	1.799%
51	7.915	2133	2138	2139	rBV	362	291	0.02%	0.003%
52	7.985	2152	2160	2166	rVB7	1495	2205	0.18%	0.025%
53	8.095	2183	2194	2230	rBV2	285987	567828	47.47%	6.420%
54	8.461	2306	2308	2311	rVB2	480	259	0.02%	0.003%
55	8.567	2338	2341	2343	rBV2	374	258	0.02%	0.003%
56	8.677	2373	2375	2379	rBV2	307	170	0.01%	0.002%
57	8.696	2379	2381	2388	rVB2	214	143	0.01%	0.002%
58	8.760	2399	2401	2405	rVB	440	229	0.02%	0.003%
59	8.853	2419	2430	2458	rBV	517389	849649	71.03%	9.606%
60	9.149	2517	2522	2531	rBV4	653	907	0.08%	0.010%
61	9.197	2534	2537	2540	rBV	251	200	0.02%	0.002%
62	9.288	2559	2565	2574	rBV3	363	553	0.05%	0.006%
63	9.371	2588	2591	2597	rVB2	303	264	0.02%	0.003%
64	9.426	2606	2608	2613	rBV2	257	128	0.01%	0.001%
65	9.545	2641	2645	2646	rVV2	231	152	0.01%	0.002%
66	9.660	2679	2681	2687	rVB3	326	257	0.02%	0.003%
67	9.898	2753	2755	2759	rVB	295	142	0.01%	0.002%
68	9.934	2759	2766	2770	rBV2	294	286	0.02%	0.003%
69	10.056	2801	2804	2808	rBV2	202	158	0.01%	0.002%
70	10.133	2817	2828	2839	rVB5	2045	3436	0.29%	0.039%
71	10.220	2840	2855	2876	rBV	324109	512345	42.83%	5.792%
72	10.387	2904	2907	2910	rBV2	598	304	0.03%	0.003%
73	10.455	2926	2928	2932	rBV2	438	338	0.03%	0.004%
74	10.574	2961	2965	2971	rBV4	551	543	0.05%	0.006%
75	10.615	2976	2978	2981	rVV3	394	215	0.02%	0.002%
76	10.660	2990	2992	2998	rVB3	485	361	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022205.D
 Acq On : 17 Sep 2021 23:30
 Operator : SY/MD
 Sample : M3787-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.689	2998	3001	3003	rBV	261	179	0.01%	0.002%
78	10.818	3038	3041	3043	rBV	200	130	0.01%	0.001%
79	10.911	3066	3070	3071	rBV2	1175	713	0.06%	0.008%
80	10.985	3090	3093	3097	rBV	408	222	0.02%	0.003%
81	11.037	3107	3109	3110	rBV2	452	231	0.02%	0.003%
82	11.123	3133	3136	3137	rBV	217	130	0.01%	0.001%
83	11.252	3164	3176	3198	rBV	481929	735945	61.53%	8.320%
84	11.468	3240	3243	3245	rBV3	348	248	0.02%	0.003%
85	11.551	3266	3269	3271	rVB	263	145	0.01%	0.002%
86	11.625	3279	3292	3313	rBV	494746	777096	64.97%	8.785%
87	11.799	3344	3346	3348	rVB2	504	200	0.02%	0.002%
88	11.860	3361	3365	3369	rBV4	519	531	0.04%	0.006%
89	12.033	3417	3419	3421	rBV2	255	125	0.01%	0.001%
90	12.046	3421	3423	3428	rVB	418	310	0.03%	0.004%
91	12.098	3435	3439	3440	rBV3	350	251	0.02%	0.003%
92	12.185	3464	3466	3469	rVB2	356	180	0.02%	0.002%
93	12.484	3557	3559	3561	rBV	321	173	0.01%	0.002%
94	12.529	3571	3573	3576	rBV2	231	126	0.01%	0.001%
95	12.853	3672	3674	3677	rBV2	316	194	0.02%	0.002%
96	13.159	3765	3769	3770	rBV	330	220	0.02%	0.002%
97	13.226	3788	3790	3793	rBV	433	176	0.01%	0.002%
98	13.895	3995	3998	4000	rBV2	298	205	0.02%	0.002%
99	13.950	4014	4015	4018	rVB2	381	149	0.01%	0.002%
100	14.352	4137	4140	4143	rBV2	558	407	0.03%	0.005%




Sum of corrected areas: 8845299

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022205.D
Acq On : 17 Sep 2021 23:30
Operator : SY/MD
Sample : M3787-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

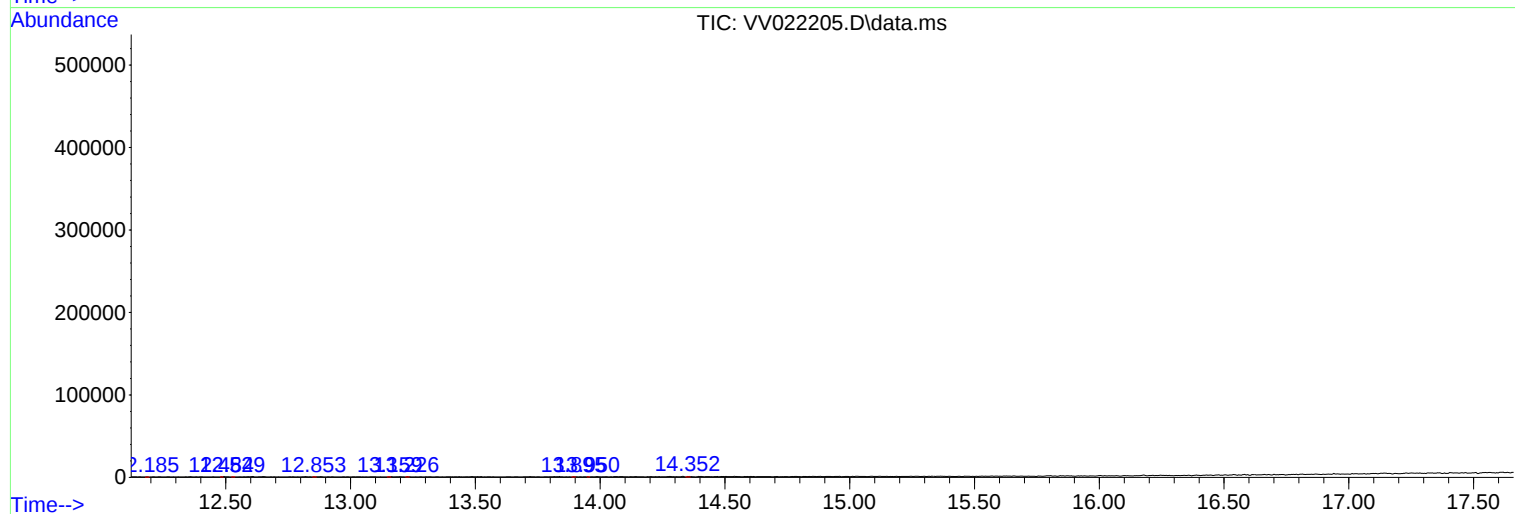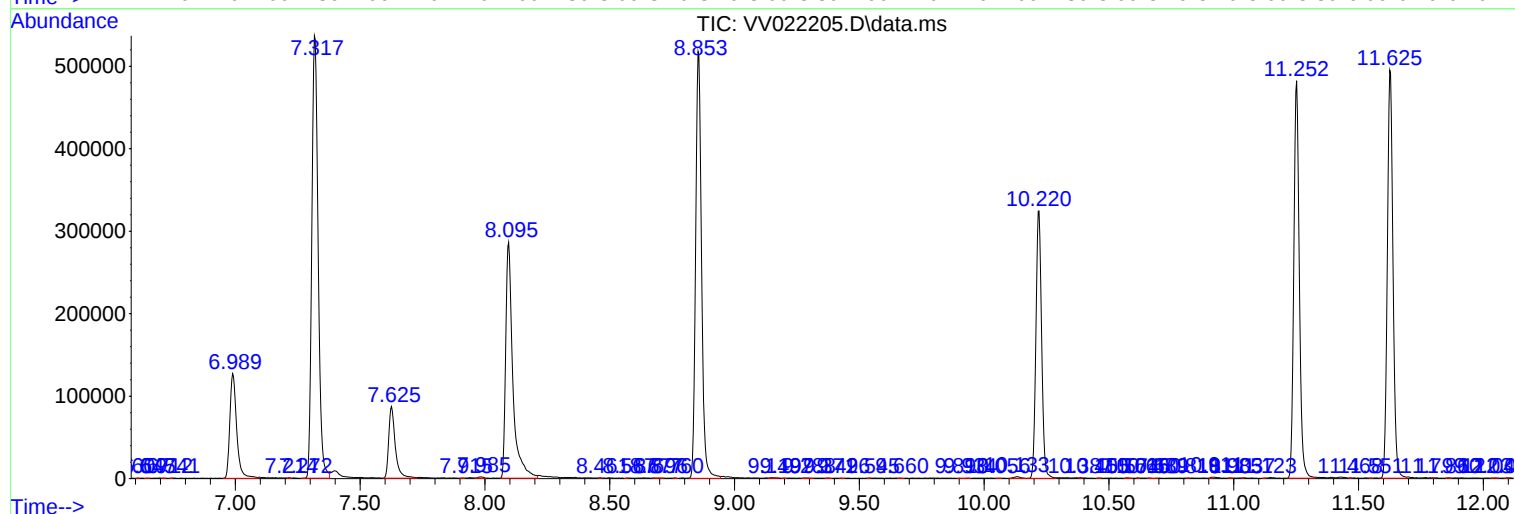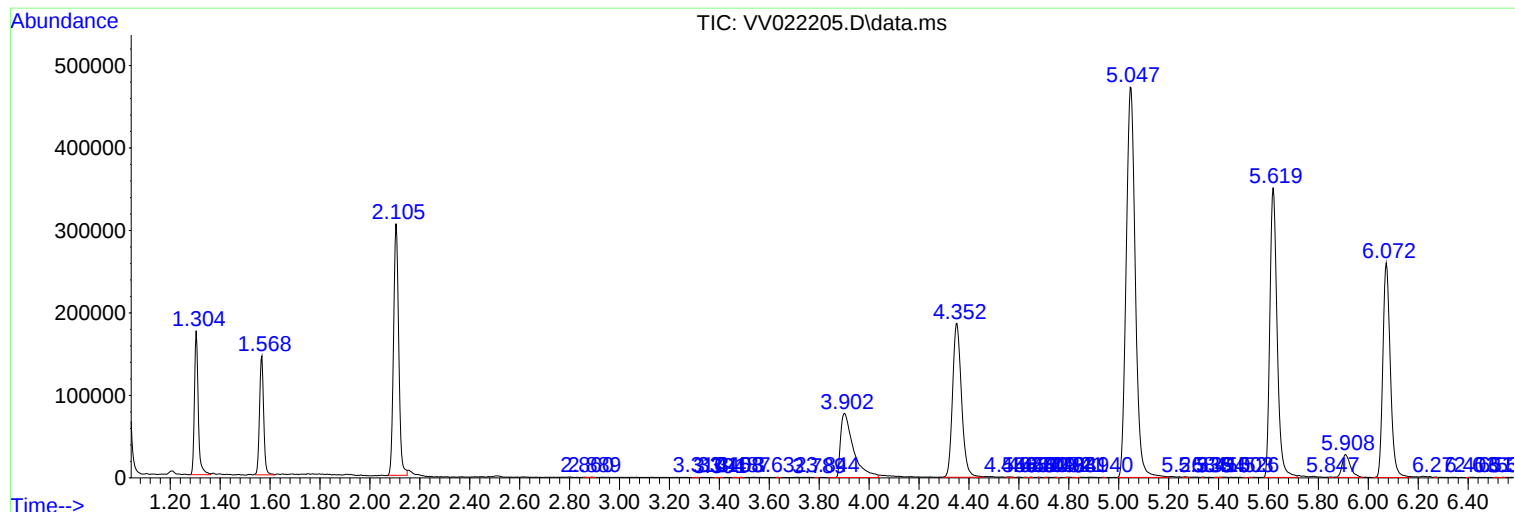

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022205.D
Acq On : 17 Sep 2021 23:30
Operator : SY/MD
Sample : M3787-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022205.D
Acq On : 17 Sep 2021 23:30
Operator : SY/MD
Sample : M3787-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
