

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022206.D
 Acq On : 17 Sep 2021 23:54
 Operator : SY/MD
 Sample : M3787-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022206.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rBV	175148	183435	15.52%	1.973%
2	1.564	156	163	178	rBV	138684	161936	13.70%	1.742%
3	2.105	321	331	347	rBV2	311900	464089	39.27%	4.992%
4	2.336	400	403	407	rBV4	761	682	0.06%	0.007%
5	2.732	522	526	530	rBV3	423	369	0.03%	0.004%
6	2.783	539	542	544	rBV2	240	171	0.01%	0.002%
7	2.912	579	582	584	rBV	248	145	0.01%	0.002%
8	2.989	604	606	610	rVB2	421	246	0.02%	0.003%
9	3.024	610	617	621	rBV2	520	586	0.05%	0.006%
10	3.124	646	648	654	rVB4	248	236	0.02%	0.003%
11	3.166	659	661	664	rBV	269	169	0.01%	0.002%
12	3.262	687	691	693	rVV	253	165	0.01%	0.002%
13	3.285	696	698	701	rVV2	297	194	0.02%	0.002%
14	3.301	701	703	707	rVB2	288	181	0.02%	0.002%
15	3.449	745	749	754	rBV2	290	300	0.03%	0.003%
16	3.487	758	761	765	rVB2	319	190	0.02%	0.002%
17	3.510	765	768	774	rVB	285	185	0.02%	0.002%
18	3.693	823	825	832	rVB3	400	269	0.02%	0.003%
19	3.831	862	868	869	rBV	259	162	0.01%	0.002%
20	3.908	879	892	933	rBV	86393	327278	27.70%	3.521%
21	4.352	1015	1030	1053	rBV	184532	455690	38.56%	4.902%
22	4.796	1164	1168	1170	rBV3	253	159	0.01%	0.002%
23	4.934	1208	1211	1214	rBV	329	220	0.02%	0.002%
24	4.950	1214	1216	1222	rBV3	365	284	0.02%	0.003%
25	5.050	1228	1247	1278	rBV2	466374	1181687	100.00%	12.712%
26	5.307	1324	1327	1330	rVB2	552	351	0.03%	0.004%
27	5.387	1349	1352	1356	rBV4	489	385	0.03%	0.004%
28	5.542	1398	1400	1403	rBV2	213	152	0.01%	0.002%
29	5.619	1411	1424	1451	rBV	341348	694065	58.74%	7.466%
30	5.915	1502	1516	1545	rBV3	261931	548183	46.39%	5.897%
31	6.072	1552	1565	1587	rBV2	254839	522924	44.25%	5.625%
32	6.249	1618	1620	1624	rBV3	703	416	0.04%	0.004%
33	6.339	1645	1648	1651	rVB2	248	159	0.01%	0.002%
34	6.362	1651	1655	1658	rBV	261	197	0.02%	0.002%
35	6.381	1658	1661	1665	rBV	239	200	0.02%	0.002%
36	6.558	1711	1716	1719	rBV3	512	404	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022206.D
 Acq On : 17 Sep 2021 23:54
 Operator : SY/MD
 Sample : M3787-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.670	1748	1751	1758	rVB3	659	516	0.04%	0.006%
38	6.780	1781	1785	1786	rBV	222	149	0.01%	0.002%
39	6.886	1816	1818	1821	rVB	344	160	0.01%	0.002%
40	6.921	1825	1829	1832	rBV2	311	165	0.01%	0.002%
41	6.989	1839	1850	1877	rBV	126714	238302	20.17%	2.564%
42	7.320	1941	1953	1971	rBV	542030	930936	78.78%	10.015%
43	7.526	2015	2017	2018	rBV	546	208	0.02%	0.002%
44	7.577	2030	2033	2037	rVB2	416	333	0.03%	0.004%
45	7.625	2037	2048	2070	rBV	87216	154605	13.08%	1.663%
46	7.834	2108	2113	2115	rBV6	339	321	0.03%	0.003%
47	8.095	2183	2194	2227	rBV3	282797	564222	47.75%	6.070%
48	8.381	2281	2283	2287	rBV2	370	262	0.02%	0.003%
49	8.400	2287	2289	2293	rVB3	495	380	0.03%	0.004%
50	8.423	2293	2296	2301	rBV4	366	252	0.02%	0.003%
51	8.516	2323	2325	2327	rBV2	427	273	0.02%	0.003%
52	8.574	2339	2343	2345	rBV	409	243	0.02%	0.003%
53	8.632	2356	2361	2368	rVB3	408	528	0.04%	0.006%
54	8.667	2369	2372	2377	rVV2	277	244	0.02%	0.003%
55	8.722	2386	2389	2394	rVB2	441	267	0.02%	0.003%
56	8.854	2419	2430	2455	rBV	507343	834048	70.58%	8.972%
57	9.114	2510	2511	2514	rVB	369	157	0.01%	0.002%
58	9.146	2515	2521	2524	rBV5	840	896	0.08%	0.010%
59	9.230	2542	2547	2551	rBV3	378	368	0.03%	0.004%
60	9.262	2553	2557	2558	rBV2	272	150	0.01%	0.002%
61	9.400	2596	2600	2602	rBV	195	183	0.02%	0.002%
62	9.461	2617	2619	2622	rVB	343	150	0.01%	0.002%
63	9.538	2637	2643	2646	rBV2	172	246	0.02%	0.003%
64	9.612	2662	2666	2667	rBV2	261	160	0.01%	0.002%
65	9.718	2696	2699	2702	rBV	232	157	0.01%	0.002%
66	9.934	2764	2766	2771	rVB3	213	149	0.01%	0.002%
67	9.976	2773	2779	2780	rBV2	168	187	0.02%	0.002%
68	10.066	2805	2807	2810	rBV2	242	158	0.01%	0.002%
69	10.130	2817	2827	2835	rBV4	1870	2869	0.24%	0.031%
70	10.220	2843	2855	2876	rBV	320967	507886	42.98%	5.464%
71	10.558	2956	2960	2963	rVV2	300	242	0.02%	0.003%
72	10.587	2967	2969	2972	rVB2	426	176	0.01%	0.002%
73	10.731	3010	3014	3018	rBV2	269	240	0.02%	0.003%
74	10.760	3021	3023	3025	rVV	452	201	0.02%	0.002%
75	10.780	3026	3029	3031	rVV2	416	194	0.02%	0.002%
76	10.818	3037	3041	3045	rVB	203	185	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022206.D
 Acq On : 17 Sep 2021 23:54
 Operator : SY/MD
 Sample : M3787-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.963	3082	3086	3088	rBV2	196	179	0.02%	0.002%
78	11.046	3110	3112	3113	rBV	478	151	0.01%	0.002%
79	11.149	3137	3144	3151	rBV4	891	937	0.08%	0.010%
80	11.252	3164	3176	3200	rBV	463493	728637	61.66%	7.838%
81	11.435	3229	3233	3234	rBV	861	466	0.04%	0.005%
82	11.468	3240	3243	3245	rBV2	336	175	0.01%	0.002%
83	11.564	3270	3273	3275	rVB3	405	201	0.02%	0.002%
84	11.625	3280	3292	3312	rBV	491650	773711	65.48%	8.323%
85	11.738	3326	3327	3330	rVB	514	205	0.02%	0.002%
86	11.808	3347	3349	3354	rBV3	251	222	0.02%	0.002%
87	11.898	3372	3377	3379	rBV2	427	372	0.03%	0.004%
88	11.937	3386	3389	3392	rBV2	451	381	0.03%	0.004%
89	12.349	3515	3517	3520	rBV	260	182	0.02%	0.002%
90	12.439	3542	3545	3546	rBV2	321	186	0.02%	0.002%
91	12.921	3691	3695	3698	rBV2	384	249	0.02%	0.003%
92	13.008	3719	3722	3726	rVB2	372	278	0.02%	0.003%
93	13.181	3773	3776	3777	rBV	430	206	0.02%	0.002%
94	13.246	3793	3796	3799	rBV	317	177	0.01%	0.002%
95	13.394	3840	3842	3845	rVB	418	254	0.02%	0.003%
96	13.516	3878	3880	3882	rVB2	456	162	0.01%	0.002%
97	13.532	3882	3885	3887	rBV	315	176	0.01%	0.002%
98	13.635	3915	3917	3924	rBV3	238	163	0.01%	0.002%
99	13.921	4002	4006	4008	rVB3	311	183	0.02%	0.002%
100	15.123	4378	4380	4382	rBV2	421	184	0.02%	0.002%




Sum of corrected areas: 9295869

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022206.D
Acq On : 17 Sep 2021 23:54
Operator : SY/MD
Sample : M3787-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

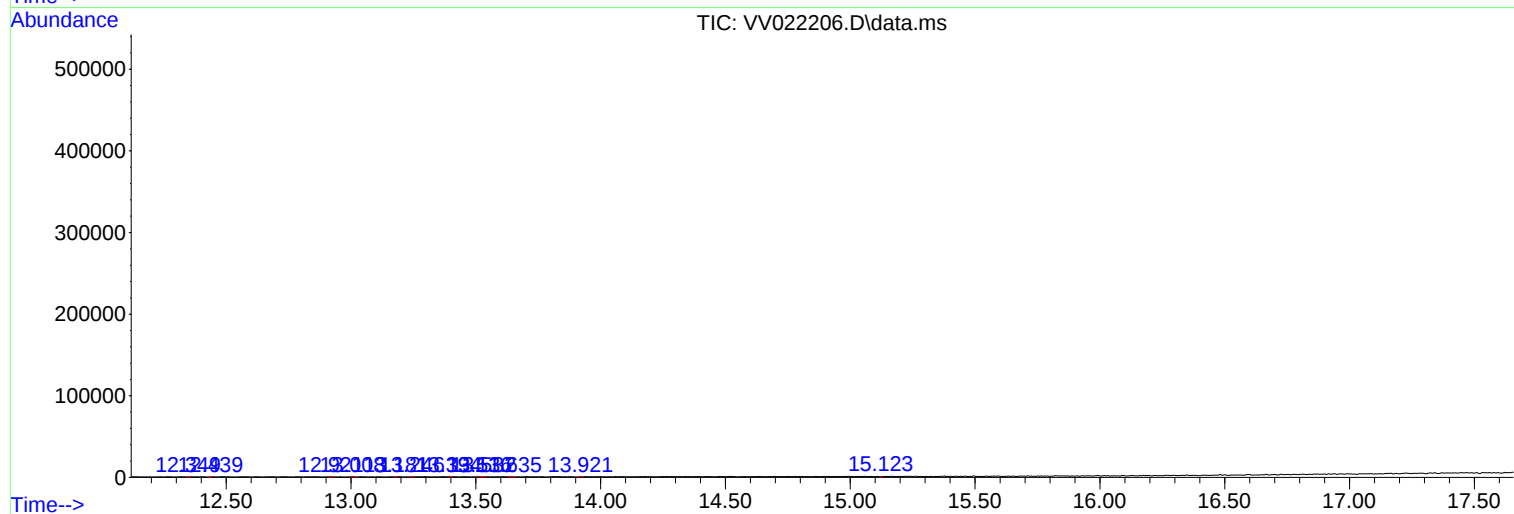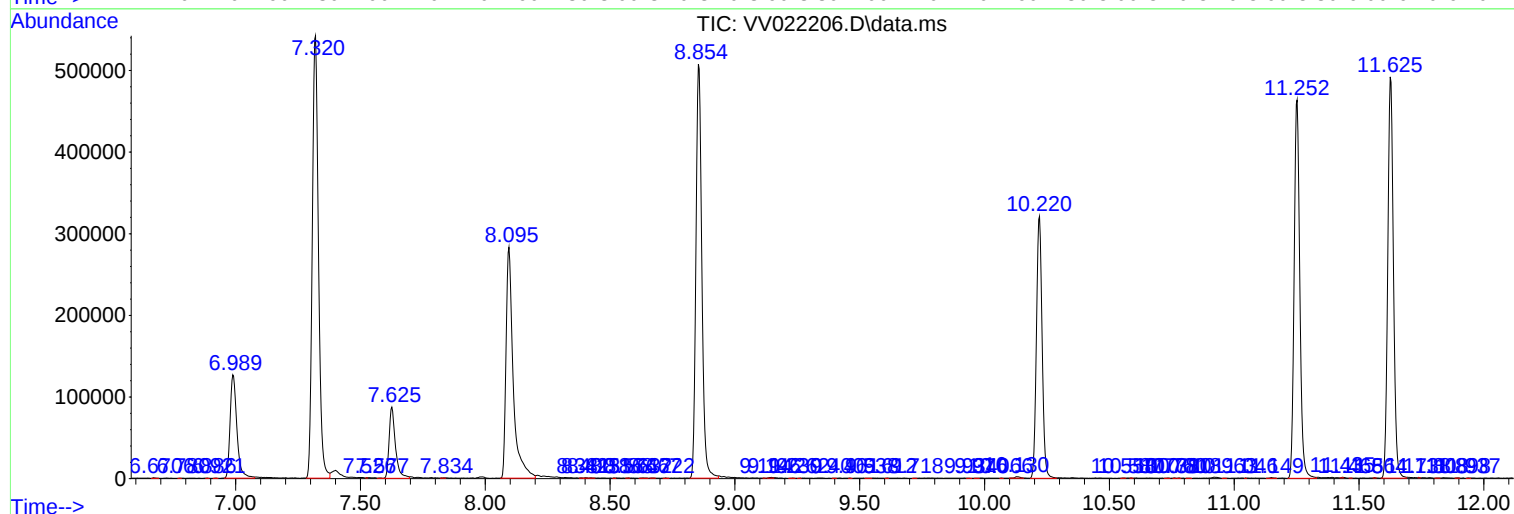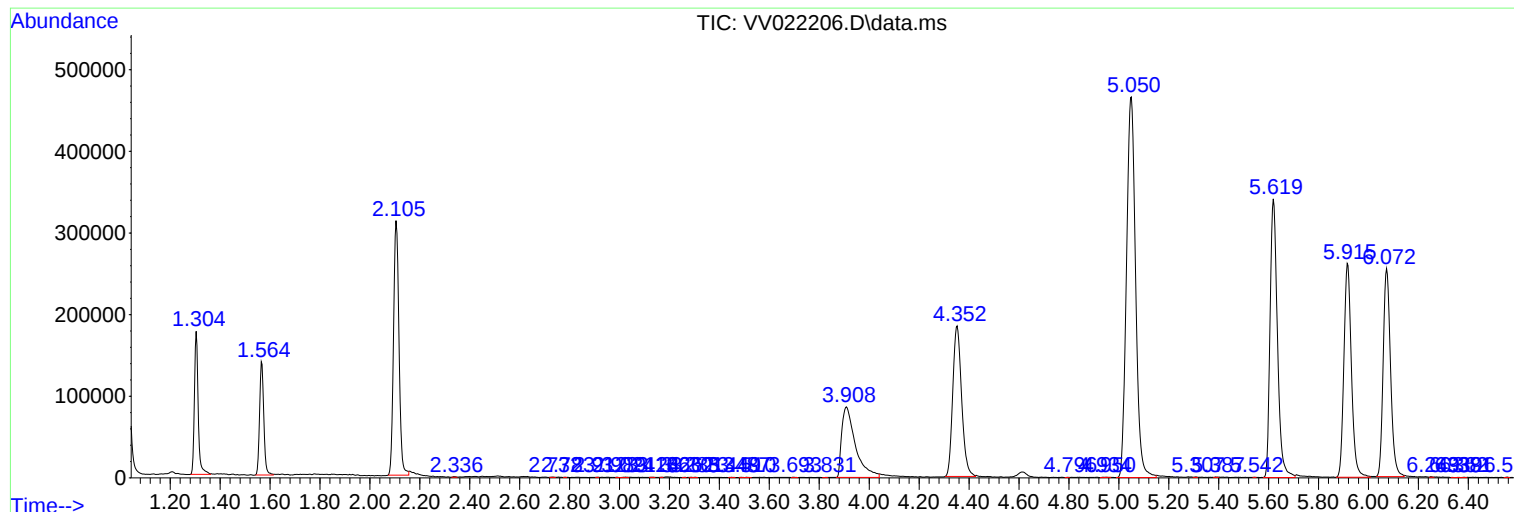

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022206.D
Acq On : 17 Sep 2021 23:54
Operator : SY/MD
Sample : M3787-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022206.D
Acq On : 17 Sep 2021 23:54
Operator : SY/MD
Sample : M3787-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
