

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022208.D
 Acq On : 18 Sep 2021 00:42
 Operator : SY/MD
 Sample : M3787-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CG5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022208.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rBV	173340	181110	15.69%	2.035%
2	1.564	156	163	178	rVB	137317	156292	13.54%	1.756%
3	2.104	321	331	348	rBV	299342	435249	37.72%	4.890%
4	2.564	471	474	475	rBV	369	187	0.02%	0.002%
5	2.629	492	494	498	rVB	395	261	0.02%	0.003%
6	2.648	498	500	502	rBV3	338	175	0.02%	0.002%
7	2.719	520	522	524	rBV	265	135	0.01%	0.002%
8	2.799	544	547	550	rBV2	339	267	0.02%	0.003%
9	2.892	572	576	579	rVB2	574	374	0.03%	0.004%
10	2.953	592	595	596	rBV2	303	140	0.01%	0.002%
11	3.059	623	628	630	rBV2	158	160	0.01%	0.002%
12	3.481	757	759	764	rVB	302	215	0.02%	0.002%
13	3.526	764	773	776	rBV	355	375	0.03%	0.004%
14	3.551	779	781	784	rVB3	331	146	0.01%	0.002%
15	3.567	784	786	790	rVB	202	139	0.01%	0.002%
16	3.587	790	792	794	rBV2	354	176	0.02%	0.002%
17	3.715	829	832	836	rVB3	438	323	0.03%	0.004%
18	3.905	880	891	930	rBV2	72667	273001	23.66%	3.067%
19	4.211	984	986	990	rBB3	573	306	0.03%	0.003%
20	4.349	1013	1029	1061	rBV	178000	451572	39.13%	5.074%
21	4.715	1139	1143	1144	rBV3	219	176	0.02%	0.002%
22	4.844	1181	1183	1187	rBV2	343	181	0.02%	0.002%
23	4.934	1207	1211	1215	rVB3	349	340	0.03%	0.004%
24	5.050	1227	1247	1275	rBV2	459246	1154007	100.00%	12.966%
25	5.255	1309	1311	1312	rBV3	445	143	0.01%	0.002%
26	5.284	1318	1320	1322	rBV	394	188	0.02%	0.002%
27	5.423	1360	1363	1364	rBV	297	207	0.02%	0.002%
28	5.452	1369	1372	1374	rBV2	284	134	0.01%	0.002%
29	5.490	1379	1384	1387	rVB2	370	219	0.02%	0.002%
30	5.513	1387	1391	1393	rBV2	344	215	0.02%	0.002%
31	5.529	1393	1396	1401	rVB2	481	379	0.03%	0.004%
32	5.558	1403	1405	1408	rVB	421	155	0.01%	0.002%
33	5.619	1412	1424	1454	rBV	336541	681206	59.03%	7.654%
34	5.915	1502	1516	1542	rBV3	186205	399435	34.61%	4.488%
35	6.072	1552	1565	1591	rBV	255243	514377	44.57%	5.779%
36	6.310	1636	1639	1643	rVB3	505	356	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022208.D
 Acq On : 18 Sep 2021 00:42
 Operator : SY/MD
 Sample : M3787-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CG5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.394	1663	1665	1668	rVV3	295	185	0.02%	0.002%
38	6.635	1735	1740	1742	rVV	293	220	0.02%	0.002%
39	6.667	1746	1750	1752	rBV	282	200	0.02%	0.002%
40	6.763	1775	1780	1782	rBV	267	224	0.02%	0.003%
41	6.828	1797	1800	1802	rBV2	322	222	0.02%	0.002%
42	6.902	1818	1823	1826	rBV2	161	163	0.01%	0.002%
43	6.989	1838	1850	1879	rBV	120430	230107	19.94%	2.585%
44	7.243	1925	1929	1932	rBV2	490	399	0.03%	0.004%
45	7.317	1941	1952	1970	rBV	524191	914405	79.24%	10.274%
46	7.625	2037	2048	2075	rBV	84938	152536	13.22%	1.714%
47	7.799	2099	2102	2105	rVV3	629	358	0.03%	0.004%
48	7.857	2115	2120	2121	rBV4	268	242	0.02%	0.003%
49	7.915	2135	2138	2140	rBV	380	238	0.02%	0.003%
50	8.095	2183	2194	2235	rBV2	272726	560467	48.57%	6.297%
51	8.361	2275	2277	2279	rVB2	438	202	0.02%	0.002%
52	8.452	2303	2305	2311	rVB3	578	566	0.05%	0.006%
53	8.538	2330	2332	2334	rVB3	372	148	0.01%	0.002%
54	8.558	2334	2338	2339	rBV	433	266	0.02%	0.003%
55	8.853	2416	2430	2454	rBV	496852	813914	70.53%	9.145%
56	9.037	2485	2487	2489	rBV	250	128	0.01%	0.001%
57	9.146	2514	2521	2525	rBV4	628	818	0.07%	0.009%
58	9.207	2537	2540	2543	rVB2	305	183	0.02%	0.002%
59	9.226	2543	2546	2549	rBV2	236	152	0.01%	0.002%
60	9.246	2549	2552	2555	rVB2	300	180	0.02%	0.002%
61	9.342	2576	2582	2584	rBV3	349	314	0.03%	0.004%
62	9.413	2600	2604	2606	rBV2	237	158	0.01%	0.002%
63	9.445	2611	2614	2618	rBV2	516	363	0.03%	0.004%
64	9.490	2624	2628	2633	rBV3	347	338	0.03%	0.004%
65	9.660	2678	2681	2683	rBV2	243	154	0.01%	0.002%
66	9.680	2683	2687	2688	rVV	224	136	0.01%	0.002%
67	9.760	2709	2712	2717	rVB2	355	340	0.03%	0.004%
68	9.799	2718	2724	2726	rBV	394	320	0.03%	0.004%
69	9.995	2783	2785	2788	rBV2	286	156	0.01%	0.002%
70	10.133	2817	2828	2835	rBV3	2049	3012	0.26%	0.034%
71	10.217	2842	2854	2878	rBV	305107	491667	42.61%	5.524%
72	10.352	2893	2896	2897	rBV	389	206	0.02%	0.002%
73	10.426	2917	2919	2923	rBV	575	367	0.03%	0.004%
74	10.468	2929	2932	2934	rBV2	553	313	0.03%	0.004%
75	10.525	2945	2950	2957	rBV2	260	269	0.02%	0.003%
76	10.564	2959	2962	2964	rBV2	396	274	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022208.D
 Acq On : 18 Sep 2021 00:42
 Operator : SY/MD
 Sample : M3787-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CG5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.709	3004	3007	3011	rVB3	421	264	0.02%	0.003%
78	10.741	3013	3017	3022	rBV2	275	278	0.02%	0.003%
79	10.853	3048	3052	3054	rBV2	351	291	0.03%	0.003%
80	10.914	3065	3071	3074	rBV3	1525	1619	0.14%	0.018%
81	10.992	3092	3095	3098	rBV2	251	183	0.02%	0.002%
82	11.030	3104	3107	3108	rBV	307	163	0.01%	0.002%
83	11.149	3138	3144	3147	rBV5	873	847	0.07%	0.010%
84	11.252	3164	3176	3194	rBV	457996	708195	61.37%	7.957%
85	11.545	3264	3267	3276	rBV4	515	501	0.04%	0.006%
86	11.625	3281	3292	3311	rBV	475681	756286	65.54%	8.498%
87	11.853	3361	3363	3368	rBV2	369	293	0.03%	0.003%
88	12.033	3418	3419	3424	rBV	273	255	0.02%	0.003%
89	12.297	3499	3501	3504	rVB	420	183	0.02%	0.002%
90	12.345	3513	3516	3517	rBV2	461	275	0.02%	0.003%
91	12.602	3593	3596	3598	rBV2	364	187	0.02%	0.002%
92	12.670	3613	3617	3622	rVB3	292	307	0.03%	0.003%
93	12.728	3632	3635	3641	rVB2	443	303	0.03%	0.003%
94	12.757	3641	3644	3646	rBV2	238	155	0.01%	0.002%
95	13.332	3820	3823	3826	rVB2	303	185	0.02%	0.002%
96	13.528	3879	3884	3890	rBV2	366	505	0.04%	0.006%
97	13.583	3899	3901	3905	rBV2	325	197	0.02%	0.002%
98	14.278	4113	4117	4122	rBV3	449	421	0.04%	0.005%
99	14.863	4297	4299	4304	rBV3	419	252	0.02%	0.003%
100	15.239	4414	4416	4425	rBV2	570	724	0.06%	0.008%


Sum of corrected areas: 8900100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022208.D
Acq On : 18 Sep 2021 00:42
Operator : SY/MD
Sample : M3787-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

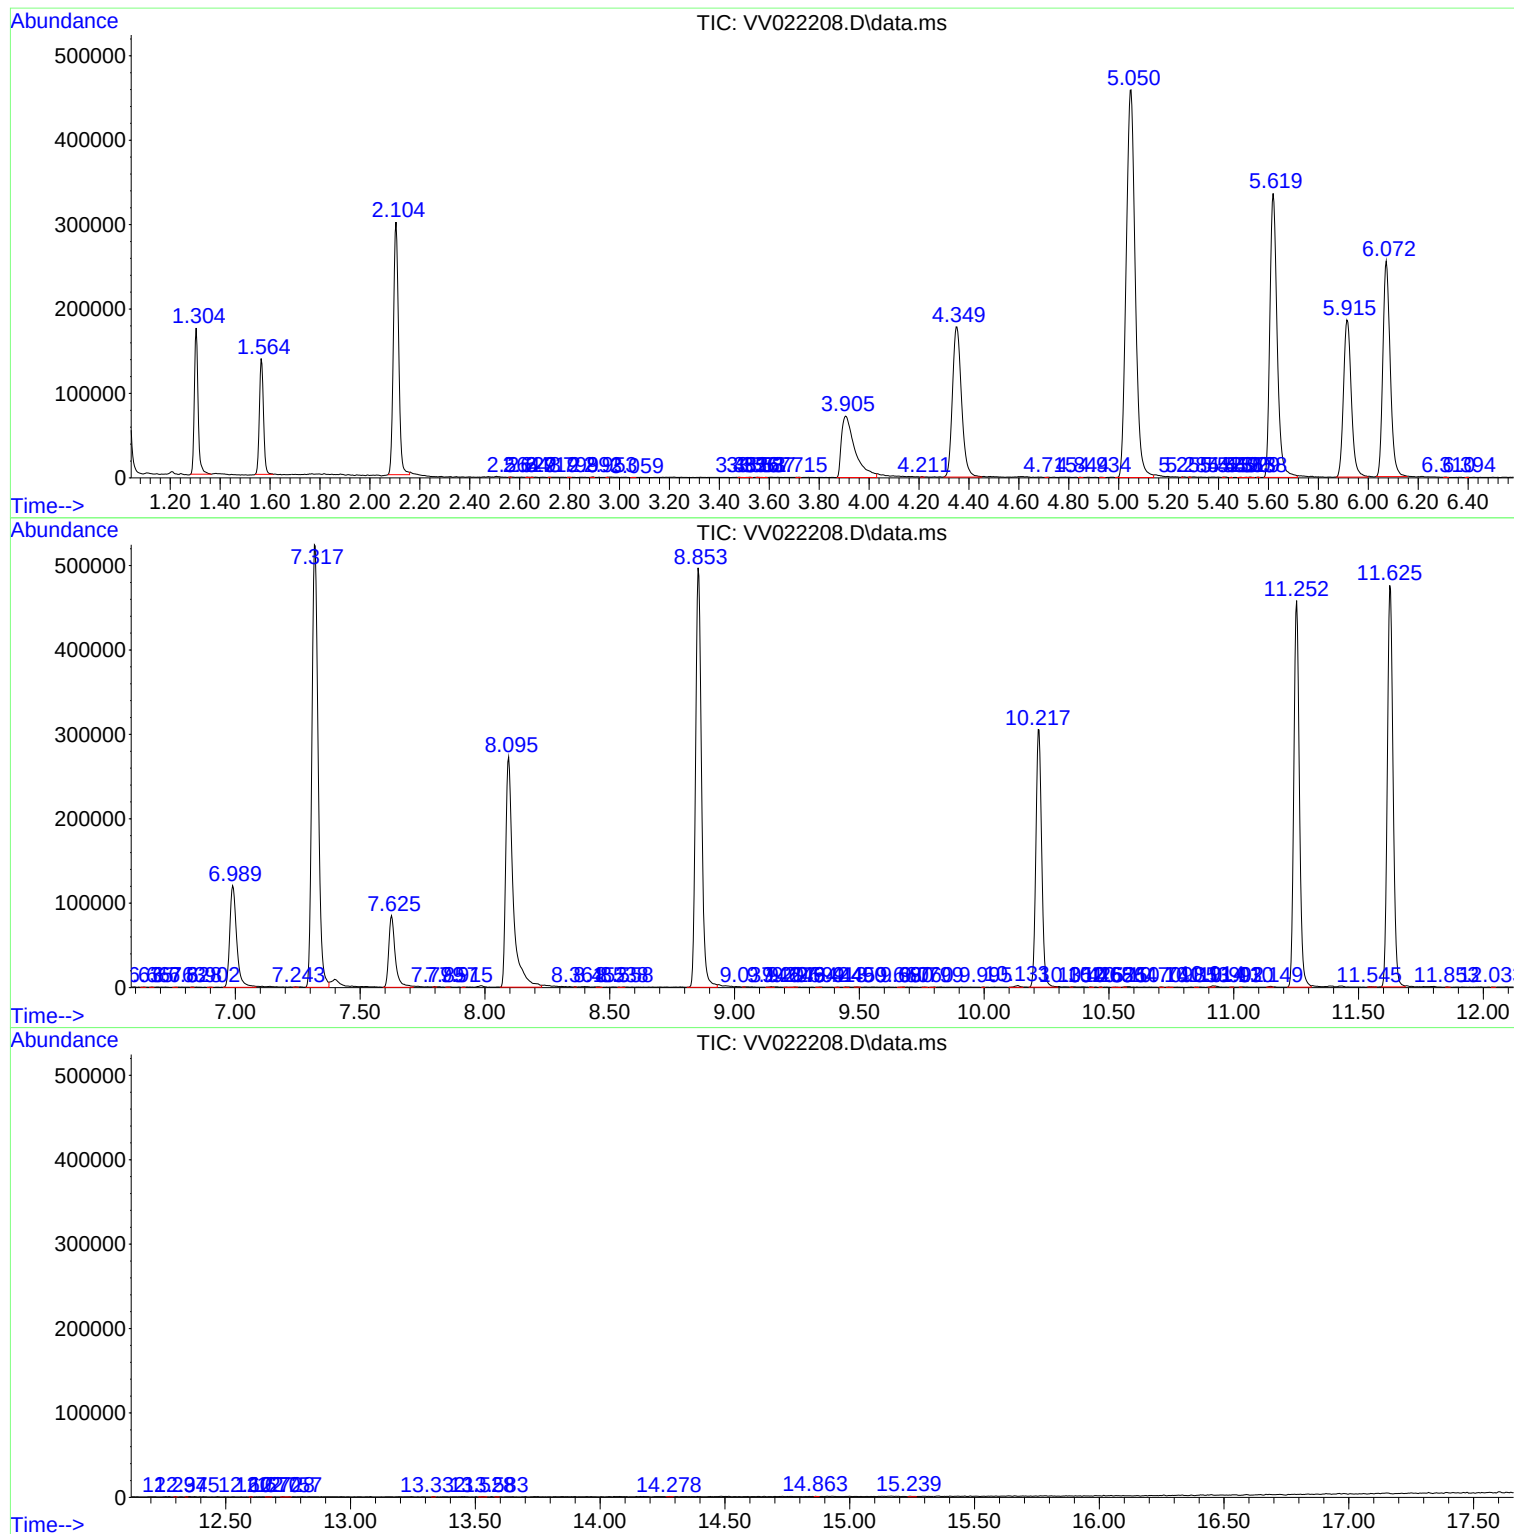

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022208.D
Acq On : 18 Sep 2021 00:42
Operator : SY/MD
Sample : M3787-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022208.D
Acq On : 18 Sep 2021 00:42
Operator : SY/MD
Sample : M3787-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
