

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022212.D
 Acq On : 18 Sep 2021 02:18
 Operator : SY/MD
 Sample : M3787-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022212.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rBV	174926	181633	6.61%	1.544%
2	1.564	156	163	180	rVB	141037	162613	5.92%	1.382%
3	2.105	322	331	367	rVB2	334515	531861	19.37%	4.521%
4	2.677	505	509	511	rBV	478	292	0.01%	0.002%
5	2.761	527	535	548	rBV3	6183	10958	0.40%	0.093%
6	3.008	608	612	613	rBV	322	193	0.01%	0.002%
7	3.031	617	619	623	rBV2	226	156	0.01%	0.001%
8	3.050	623	625	629	rVV3	380	220	0.01%	0.002%
9	3.085	631	636	639	rBV3	382	291	0.01%	0.002%
10	3.201	659	672	677	rBV4	2609	4395	0.16%	0.037%
11	3.487	759	761	767	rVB2	314	214	0.01%	0.002%
12	3.545	775	779	782	rBV3	321	239	0.01%	0.002%
13	3.661	812	815	818	rVB2	385	185	0.01%	0.002%
14	3.738	837	839	844	rBV2	252	206	0.01%	0.002%
15	3.780	848	852	854	rBV	240	183	0.01%	0.002%
16	3.908	879	892	922	rBV2	125856	407502	14.84%	3.464%
17	4.349	1014	1029	1066	rBV	188175	474789	17.29%	4.036%
18	4.561	1093	1095	1097	rBV	518	297	0.01%	0.003%
19	4.609	1097	1110	1132	rVB3	44424	112336	4.09%	0.955%
20	4.715	1141	1143	1146	rVB2	322	141	0.01%	0.001%
21	4.760	1154	1157	1159	rBV2	377	220	0.01%	0.002%
22	4.831	1176	1179	1182	rBV2	321	305	0.01%	0.003%
23	4.876	1192	1193	1196	rVB2	388	150	0.01%	0.001%
24	4.915	1202	1205	1208	rVV2	396	328	0.01%	0.003%
25	5.047	1229	1246	1276	rBV3	466967	1176699	42.85%	10.003%
26	5.368	1344	1346	1352	rBV4	332	307	0.01%	0.003%
27	5.436	1364	1367	1369	rBV	316	250	0.01%	0.002%
28	5.523	1390	1394	1396	rBV2	274	193	0.01%	0.002%
29	5.619	1411	1424	1452	rBV	337648	682394	24.85%	5.801%
30	5.915	1501	1516	1545	rBV	1404567	2745898	100.00%	23.343%
31	6.072	1553	1565	1592	rVB	259428	527849	19.22%	4.487%
32	6.301	1634	1636	1640	rBV2	413	287	0.01%	0.002%
33	6.394	1661	1665	1666	rBV2	311	233	0.01%	0.002%
34	6.522	1703	1705	1707	rBV	238	167	0.01%	0.001%
35	6.571	1716	1720	1724	rBV	443	458	0.02%	0.004%
36	6.641	1739	1742	1746	rBV3	509	443	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022212.D
 Acq On : 18 Sep 2021 02:18
 Operator : SY/MD
 Sample : M3787-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.664	1746	1749	1751	rBV	345	212	0.01%	0.002%
38	6.719	1763	1766	1768	rVB	315	148	0.01%	0.001%
39	6.818	1793	1797	1800	rVB	305	150	0.01%	0.001%
40	6.912	1821	1826	1828	rVB	265	162	0.01%	0.001%
41	6.928	1828	1831	1833	rBV	225	177	0.01%	0.002%
42	6.989	1838	1850	1872	rBV	127732	236877	8.63%	2.014%
43	7.204	1914	1917	1921	rBV3	462	409	0.01%	0.003%
44	7.317	1938	1952	1972	rBV	532416	937363	34.14%	7.969%
45	7.625	2037	2048	2074	rBV	86386	154165	5.61%	1.311%
46	7.857	2113	2120	2129	rVB8	1478	2214	0.08%	0.019%
47	7.934	2140	2144	2147	rVB	231	146	0.01%	0.001%
48	7.953	2147	2150	2152	rVB2	399	259	0.01%	0.002%
49	7.982	2152	2159	2163	rBV4	2001	2517	0.09%	0.021%
50	8.095	2183	2194	2229	rBV2	277177	570190	20.77%	4.847%
51	8.403	2287	2290	2292	rBV2	534	281	0.01%	0.002%
52	8.580	2340	2345	2348	rVB4	454	368	0.01%	0.003%
53	8.612	2351	2355	2360	rVB3	682	610	0.02%	0.005%
54	8.667	2370	2372	2374	rBV2	285	157	0.01%	0.001%
55	8.751	2394	2398	2400	rBV2	256	175	0.01%	0.001%
56	8.854	2414	2430	2450	rBV	506692	821086	29.90%	6.980%
57	9.153	2519	2523	2524	rBV3	534	317	0.01%	0.003%
58	9.236	2547	2549	2553	rBV2	315	225	0.01%	0.002%
59	9.622	2664	2669	2670	rBV2	273	220	0.01%	0.002%
60	9.770	2711	2715	2718	rBV2	274	212	0.01%	0.002%
61	9.789	2718	2721	2723	rBV4	596	308	0.01%	0.003%
62	9.873	2743	2747	2748	rBV	406	250	0.01%	0.002%
63	9.940	2766	2768	2772	rBV2	306	185	0.01%	0.002%
64	10.059	2800	2805	2808	rBV2	307	236	0.01%	0.002%
65	10.127	2819	2826	2836	rBV3	1404	2290	0.08%	0.019%
66	10.217	2841	2854	2875	rBV	319354	509612	18.56%	4.332%
67	10.384	2902	2906	2909	rBV2	316	231	0.01%	0.002%
68	10.448	2923	2926	2928	rBV	336	223	0.01%	0.002%
69	10.583	2964	2968	2972	rVV3	428	360	0.01%	0.003%
70	10.606	2972	2975	2978	rVB3	355	211	0.01%	0.002%
71	10.763	3022	3024	3029	rVB2	331	238	0.01%	0.002%
72	10.796	3030	3034	3036	rBV2	271	174	0.01%	0.001%
73	10.812	3036	3039	3040	rBV2	371	165	0.01%	0.001%
74	10.870	3053	3057	3060	rBV2	267	253	0.01%	0.002%
75	10.921	3067	3073	3075	rBV3	1260	1081	0.04%	0.009%
76	11.111	3129	3132	3134	rBV2	389	279	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022212.D
 Acq On : 18 Sep 2021 02:18
 Operator : SY/MD
 Sample : M3787-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	11.140	3138	3141	3144	rBV2	514	447	0.02%	0.004%
78	11.252	3164	3176	3195	rBV	455911	713142	25.97%	6.062%
79	11.574	3272	3276	3277	rBV	331	180	0.01%	0.002%
80	11.625	3280	3292	3313	rBV	493735	775262	28.23%	6.591%
81	12.181	3462	3465	3466	rBV2	380	200	0.01%	0.002%
82	12.255	3486	3488	3492	rVV3	233	144	0.01%	0.001%
83	12.275	3492	3494	3497	rVB2	320	152	0.01%	0.001%
84	12.378	3524	3526	3529	rBV2	302	212	0.01%	0.002%
85	12.619	3597	3601	3604	rBV2	283	179	0.01%	0.002%
86	12.805	3656	3659	3661	rBV	355	155	0.01%	0.001%
87	13.040	3729	3732	3735	rBV	268	164	0.01%	0.001%
88	13.165	3770	3771	3774	rBV2	235	141	0.01%	0.001%
89	13.188	3774	3778	3780	rVV2	359	243	0.01%	0.002%
90	13.255	3796	3799	3803	rBV2	377	353	0.01%	0.003%
91	13.291	3808	3810	3814	rVV2	255	182	0.01%	0.002%
92	13.381	3835	3838	3839	rBV2	297	159	0.01%	0.001%
93	13.432	3852	3854	3857	rBV	307	190	0.01%	0.002%
94	13.644	3917	3920	3923	rVB	669	344	0.01%	0.003%
95	13.667	3923	3927	3934	rBV2	304	358	0.01%	0.003%
96	13.795	3964	3967	3972	rBV3	408	388	0.01%	0.003%
97	13.889	3993	3996	3998	rBV3	382	239	0.01%	0.002%
98	13.908	4000	4002	4005	rBV2	449	247	0.01%	0.002%
99	14.107	4062	4064	4067	rBV2	244	178	0.01%	0.002%
100	15.387	4460	4462	4465	rBV2	621	288	0.01%	0.002%




Sum of corrected areas: 11763168

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022212.D
Acq On : 18 Sep 2021 02:18
Operator : SY/MD
Sample : M3787-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

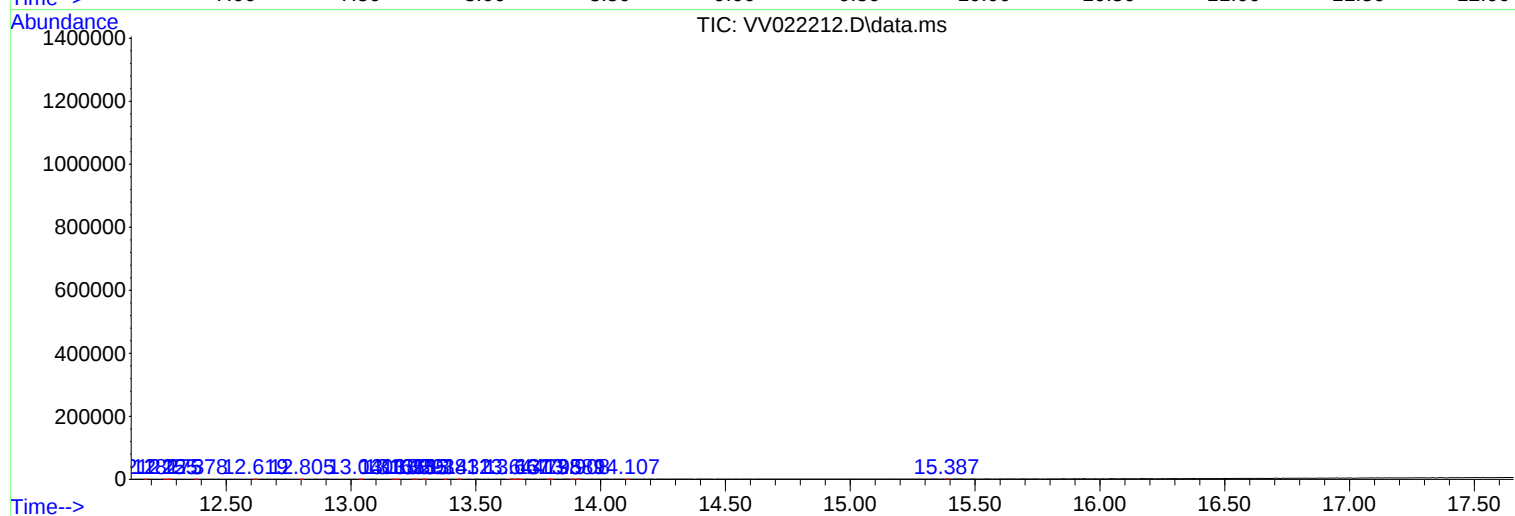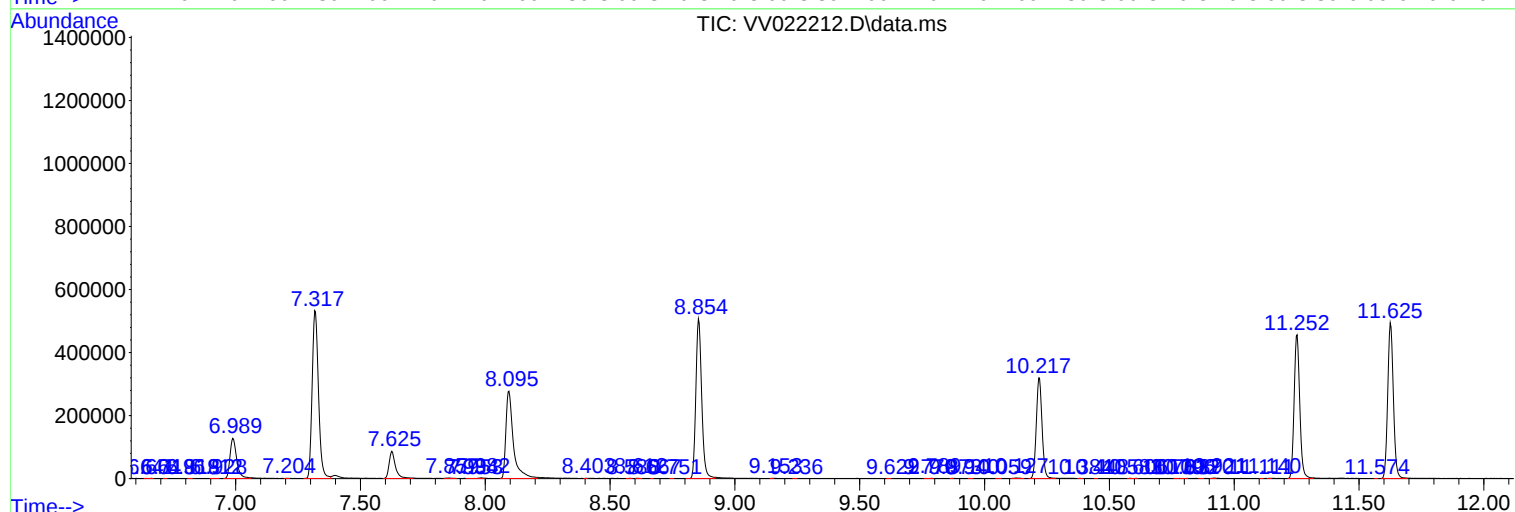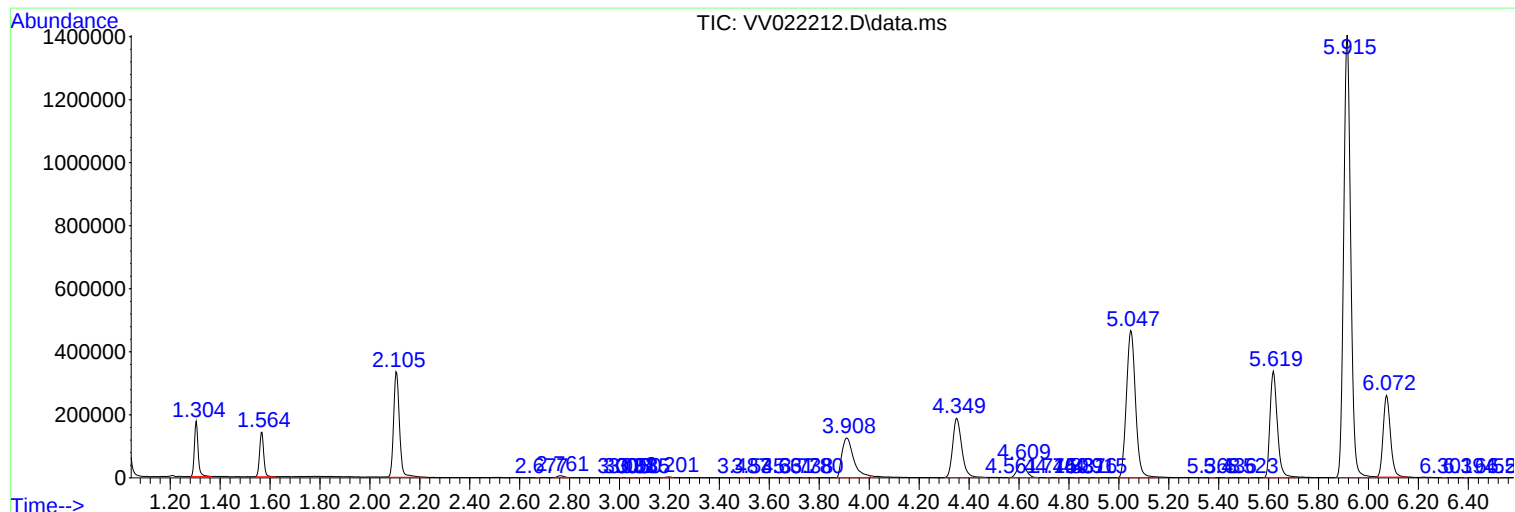

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022212.D
Acq On : 18 Sep 2021 02:18
Operator : SY/MD
Sample : M3787-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022212.D
Acq On : 18 Sep 2021 02:18
Operator : SY/MD
Sample : M3787-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
