

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022216.D
 Acq On : 18 Sep 2021 03:55
 Operator : SY/MD
 Sample : M3787-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022216.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rBV	164944	171987	15.05%	1.831%
2	1.565	156	163	177	rVB	135265	154377	13.51%	1.643%
3	2.105	322	331	361	rVB2	306324	464128	40.60%	4.940%
4	2.828	553	556	560	rBV4	522	372	0.03%	0.004%
5	2.915	579	583	590	rVB	647	537	0.05%	0.006%
6	2.950	590	594	595	rBV2	295	215	0.02%	0.002%
7	2.989	605	606	607	rBV2	204	45	0.00%	0.000%
8	3.127	644	649	651	rBV2	284	253	0.02%	0.003%
9	3.320	707	709	710	rBV	185	86	0.01%	0.001%
10	3.365	720	723	725	rBV2	257	170	0.01%	0.002%
11	3.404	731	735	738	rBV2	425	312	0.03%	0.003%
12	3.574	786	788	793	rVB	388	231	0.02%	0.002%
13	3.603	793	797	799	rBV	256	207	0.02%	0.002%
14	3.651	803	812	814	rBV	474	590	0.05%	0.006%
15	3.690	822	824	825	rBV2	156	42	0.00%	0.000%
16	3.780	847	852	855	rBV2	231	186	0.02%	0.002%
17	3.812	860	862	868	rVB2	213	163	0.01%	0.002%
18	3.863	876	878	879	rBV	211	70	0.01%	0.001%
19	3.908	879	892	936	rBV3	95000	337227	29.50%	3.589%
20	4.349	1015	1029	1053	rBV	175923	436658	38.20%	4.648%
21	4.748	1150	1153	1155	rBV2	294	164	0.01%	0.002%
22	4.777	1159	1162	1167	rBV2	515	381	0.03%	0.004%
23	4.802	1167	1170	1175	rVB3	487	353	0.03%	0.004%
24	4.857	1185	1187	1188	rBV3	230	84	0.01%	0.001%
25	4.989	1226	1228	1229	rBV	207	63	0.01%	0.001%
26	5.047	1229	1246	1284	rVV2	450785	1143063	100.00%	12.167%
27	5.352	1338	1341	1342	rBV	382	165	0.01%	0.002%
28	5.378	1347	1349	1351	rBV2	266	88	0.01%	0.001%
29	5.619	1412	1424	1450	rBV	329309	668701	58.50%	7.118%
30	5.915	1501	1516	1541	rBV2	471811	947845	82.92%	10.089%
31	6.072	1553	1565	1587	rBV	249543	506912	44.35%	5.396%
32	6.561	1714	1717	1720	rVB	619	342	0.03%	0.004%
33	6.580	1720	1723	1726	rVB2	214	114	0.01%	0.001%
34	6.600	1726	1729	1732	rBV2	242	195	0.02%	0.002%
35	6.654	1744	1746	1749	rBV2	342	223	0.02%	0.002%
36	6.680	1752	1754	1757	rVB2	348	186	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022216.D
 Acq On : 18 Sep 2021 03:55
 Operator : SY/MD
 Sample : M3787-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.699	1757	1760	1762	rBV	402	214	0.02%	0.002%
38	6.822	1794	1798	1799	rBV	222	131	0.01%	0.001%
39	6.867	1810	1812	1816	rBV	224	132	0.01%	0.001%
40	6.937	1832	1834	1837	rVB2	408	185	0.02%	0.002%

41	6.989	1838	1850	1875	rBV	119775	221665	19.39%	2.359%
42	7.211	1913	1919	1920	rBV2	469	407	0.04%	0.004%
43	7.317	1941	1952	1971	rBV	520298	899330	78.68%	9.572%
44	7.625	2038	2048	2071	rBV	81097	142431	12.46%	1.516%
45	7.850	2116	2118	2121	rBV2	372	294	0.03%	0.003%

46	7.915	2135	2138	2140	rBV2	346	214	0.02%	0.002%
47	7.985	2155	2160	2167	rVB5	1378	1612	0.14%	0.017%
48	8.095	2181	2194	2231	rBV2	269716	554797	48.54%	5.905%
49	8.484	2311	2315	2316	rBV2	320	266	0.02%	0.003%
50	8.519	2324	2326	2329	rBV	339	169	0.01%	0.002%

51	8.600	2349	2351	2353	rBV2	315	158	0.01%	0.002%
52	8.783	2404	2408	2409	rBV2	286	179	0.02%	0.002%
53	8.854	2418	2430	2457	rBV	487305	803276	70.27%	8.550%
54	9.098	2505	2506	2508	rBV	240	51	0.00%	0.001%
55	9.227	2544	2546	2549	rVB	276	84	0.01%	0.001%

56	9.262	2555	2557	2558	rBV	234	84	0.01%	0.001%
57	9.474	2620	2623	2628	rVB	438	271	0.02%	0.003%
58	9.519	2635	2637	2639	rBV	279	140	0.01%	0.001%
59	9.567	2651	2652	2653	rBV	230	60	0.01%	0.001%
60	9.628	2669	2671	2674	rVB3	348	165	0.01%	0.002%

61	9.677	2682	2686	2689	rBV3	417	304	0.03%	0.003%
62	9.693	2689	2691	2694	rVB	229	104	0.01%	0.001%
63	9.809	2723	2727	2729	rBV2	354	250	0.02%	0.003%
64	10.053	2800	2803	2805	rBV	271	177	0.02%	0.002%
65	10.130	2821	2827	2832	rBV5	1614	1901	0.17%	0.020%

66	10.169	2836	2839	2843	rVB2	408	305	0.03%	0.003%
67	10.220	2843	2855	2873	rBV	306175	489405	42.82%	5.209%
68	10.445	2922	2925	2927	rBV	340	245	0.02%	0.003%
69	10.477	2933	2935	2937	rBV	202	95	0.01%	0.001%
70	10.538	2951	2954	2956	rVB	264	149	0.01%	0.002%

71	10.580	2962	2967	2973	rBV5	383	646	0.06%	0.007%
72	10.645	2984	2987	2991	rBV	391	283	0.02%	0.003%
73	10.831	3042	3045	3046	rBV	306	152	0.01%	0.002%
74	10.854	3051	3052	3058	rVB2	263	204	0.02%	0.002%
75	10.908	3065	3069	3071	rBV3	901	657	0.06%	0.007%

76	11.027	3103	3106	3107	rBV3	283	129	0.01%	0.001%
----	--------	------	------	------	------	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022216.D
Acq On : 18 Sep 2021 03:55
Operator : SY/MD
Sample : M3787-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Title : VOC Analysis

77	11.178	3152	3153	3156	rVB	321	87	0.01%	0.001%
78	11.252	3164	3176	3200	rBV	450358	695094	60.81%	7.399%
79	11.625	3280	3292	3319	rBV	473867	740764	64.81%	7.885%
80	11.808	3347	3349	3355	rVB3	509	370	0.03%	0.004%
81	11.873	3368	3369	3371	rBV2	529	267	0.02%	0.003%
82	12.654	3610	3612	3614	rBV	287	142	0.01%	0.002%
83	13.316	3815	3818	3822	rBV2	280	226	0.02%	0.002%



Sum of corrected areas: 9395006

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022216.D
Acq On : 18 Sep 2021 03:55
Operator : SY/MD
Sample : M3787-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

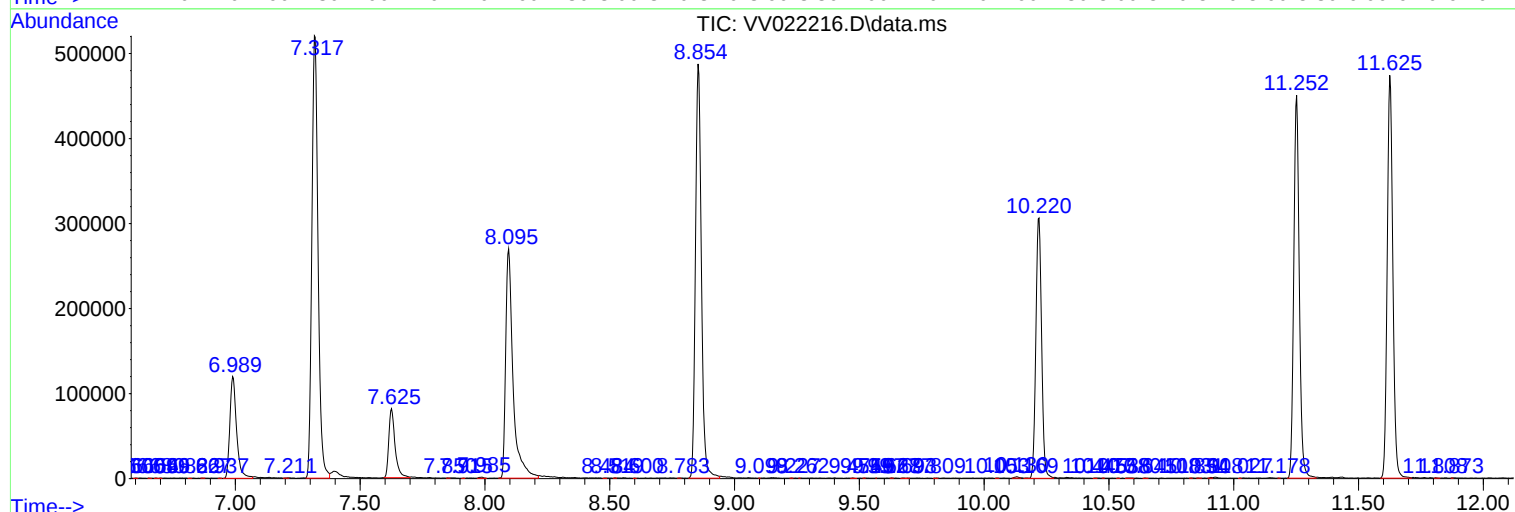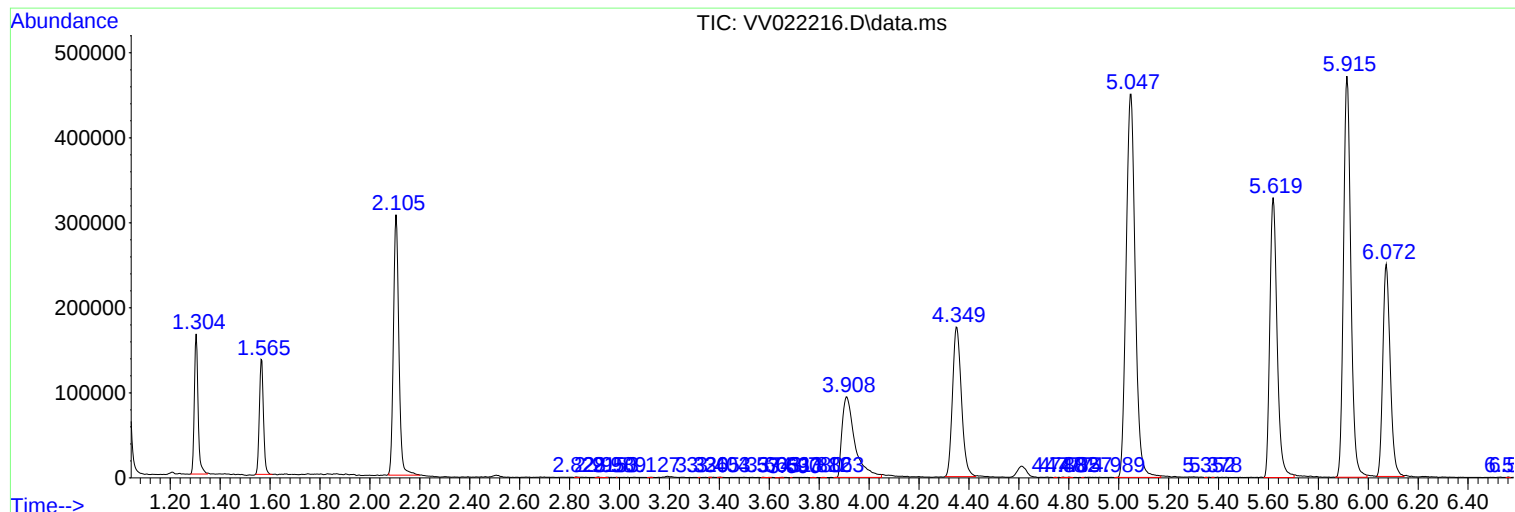

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022216.D
Acq On : 18 Sep 2021 03:55
Operator : SY/MD
Sample : M3787-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022216.D
Acq On : 18 Sep 2021 03:55
Operator : SY/MD
Sample : M3787-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
