


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022170.D
Acq On : 17 Sep 2021 08:31
Operator : SY/MD
Sample : BFB232
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB232

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Title : VOC Analysis
Last Update : Sat Sep 18 04:25:40 2021

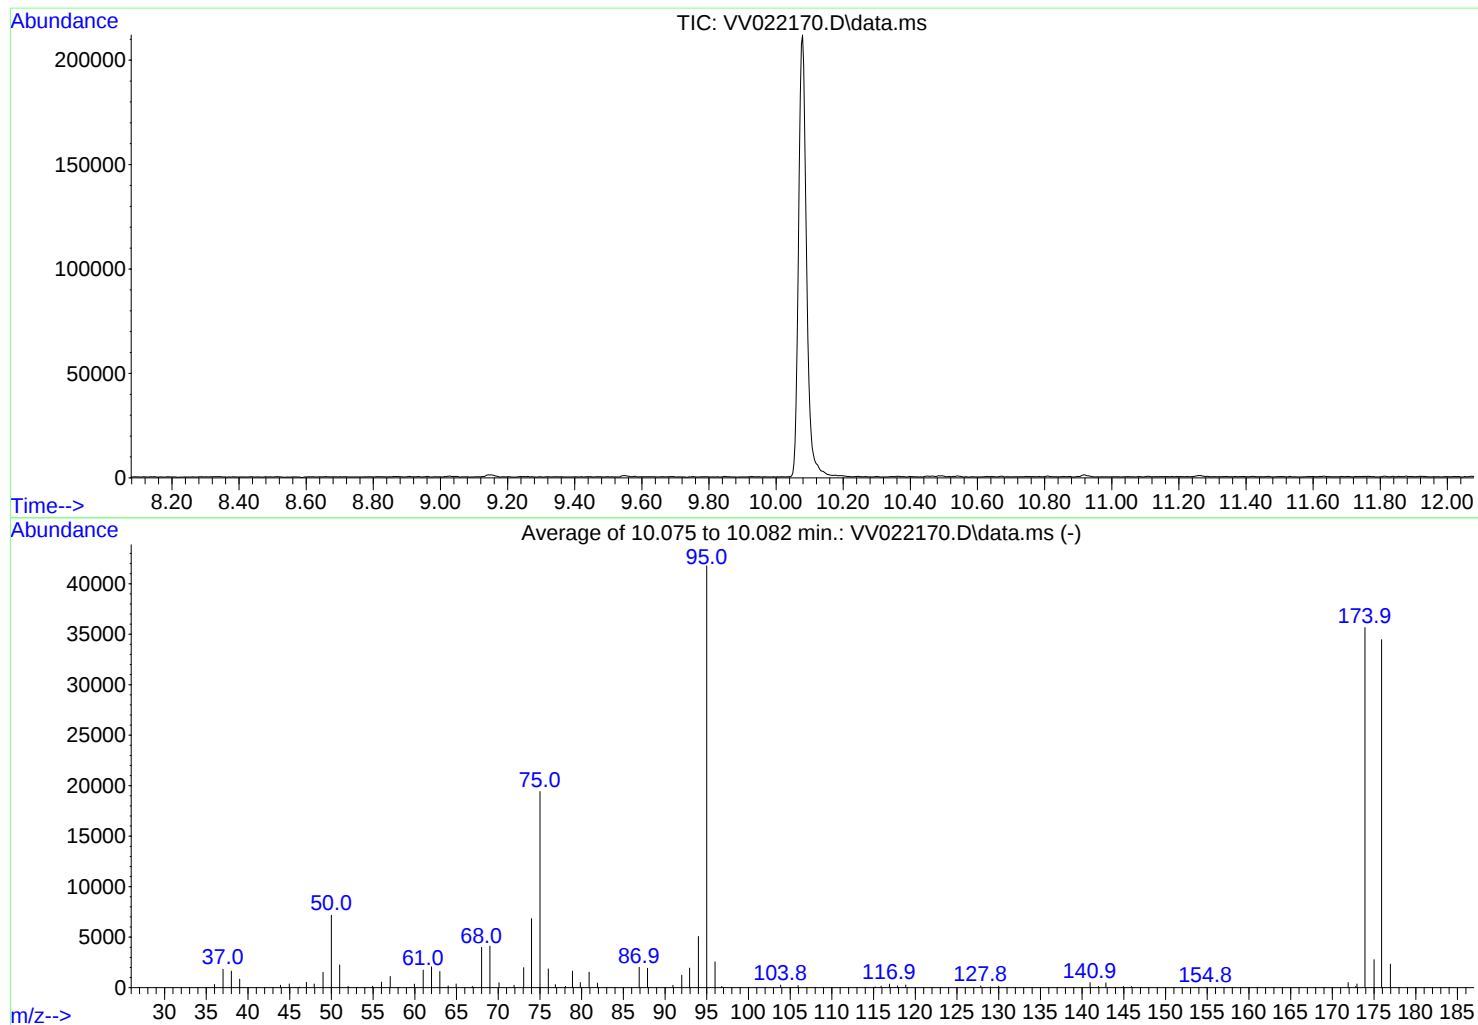

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.2	7171	PASS
75	95	30	80	46.5	19427	PASS
95	95	100	100	100.0	41773	PASS
96	95	5	9	6.1	2547	PASS
173	174	0.00	2	1.0	359	PASS
174	95	50	120	85.3	35653	PASS
175	174	5	9	7.8	2773	PASS
176	174	95	105	96.7	34467	PASS
177	176	5	10	6.8	2335	PASS

m/z	Abundance
36.00	308.0
37.00	1802.0
38.00	1701.0
39.00	856.0
43.90	583.0
44.90	385.0
47.00	588.0
47.90	400.0
49.00	1495.0
50.00	7266.0
51.00	2302.0
52.00	112.0
55.00	155.0
56.00	581.0
57.00	1127.0
59.90	377.0
61.00	1838.0
62.00	2182.0
63.00	1555.0
64.00	211.0
65.00	346.0
66.90	136.0
68.00	4141.0
69.00	4344.0
70.10	487.0
71.90	265.0
73.10	1861.0
74.00	6857.0
75.00	19944.0
76.00	1929.0
76.90	243.0
78.10	207.0
78.90	1615.0
79.90	517.0
80.90	1605.0
81.90	422.0
86.90	2077.0
87.90	2061.0
90.90	214.0
92.00	1286.0
93.00	1950.0
94.00	5123.0
95.00	42160.0
96.00	2700.0
96.80	146.0
103.80	237.0
106.00	190.0
115.00	114.0
115.90	198.0
116.90	352.0
117.80	176.0
118.80	285.0
127.90	183.0
129.00	126.0
130.00	164.0
130.90	105.0
140.90	519.0
142.00	101.0
142.90	481.0
145.00	121.0
145.90	115.0
154.80	105.0
171.90	451.0
172.80	323.0
173.00	324.0
173.90	35352.0
175.00	2821.0
175.90	33968.0
177.00	2457.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

m/z	Abundance
39.80	200.0
43.90	329.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

m/z	Abundance
36.00	318.0
37.00	1925.0
38.00	1686.0
39.00	891.0
40.00	148.0
43.90	585.0
45.00	386.0
47.00	536.0
47.90	364.0
49.00	1576.0
50.00	7416.0
51.00	2317.0
52.00	121.0
55.00	141.0
56.00	564.0
57.00	1159.0
60.00	346.0
61.00	1786.0
62.00	2139.0
63.00	1677.0
64.00	172.0
65.00	371.0
66.90	134.0
68.00	4105.0
69.00	4239.0
70.10	507.0
71.90	247.0
73.00	2046.0
74.00	7010.0
75.00	19968.0
76.00	1951.0
76.80	280.0
78.90	1717.0
79.90	513.0
80.90	1573.0
81.90	460.0
86.90	2095.0
87.90	1941.0
90.90	231.0
92.00	1282.0
93.00	1980.0
94.00	5249.0
95.00	43128.0
96.00	2627.0
96.80	140.0
103.80	260.0
105.90	226.0
115.20	130.0
115.90	154.0
116.90	374.0
117.80	182.0
118.90	263.0
127.80	174.0
129.00	120.0
130.00	145.0
141.00	513.0
142.00	135.0
142.80	484.0
144.90	107.0
145.90	116.0
171.90	498.0
172.90	350.0
173.90	36824.0
175.00	2854.0
175.90	35640.0
176.90	2415.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

m/z	Abundance
36.00	323.0
37.00	1737.0
38.00	1508.0
39.00	800.0
40.00	215.0
43.90	538.0
44.90	332.0
46.20	128.0
47.00	432.0
48.00	326.0
49.00	1504.0
50.00	6832.0
51.00	2118.0
52.00	132.0
54.90	145.0
56.00	521.0
57.10	1021.0
60.00	338.0
61.00	1587.0
62.00	1845.0
63.00	1592.0
64.00	158.0
64.90	369.0
66.90	120.0
68.00	3733.0
69.00	3729.0
70.10	475.0
71.90	213.0
73.00	2032.0
74.00	6639.0
75.00	18368.0
76.00	1682.0
76.90	393.0
78.00	162.0
78.90	1553.0
79.80	472.0
80.90	1442.0
81.90	455.0
86.90	1855.0
87.90	1727.0
91.00	250.0
92.00	1143.0
92.90	1867.0
94.00	4826.0
95.00	40032.0
96.00	2315.0
96.80	105.0
103.90	261.0
105.90	213.0
115.20	101.0
115.90	122.0
116.90	331.0
117.90	164.0
118.90	245.0
127.90	149.0
130.00	133.0
141.00	454.0
141.90	131.0
142.80	468.0
144.90	103.0
145.90	108.0
171.90	552.0
172.90	404.0
173.90	34784.0
175.00	2644.0
175.90	33792.0
176.90	2133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232