

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091724\
 Data File : VV037308.D
 Acq On : 17 Sep 2024 11:31
 Operator : SY/MD
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 18 05:37:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM091324.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Sep 14 03:38:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	13853	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	13519	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	6749	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	7553	0.510	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	102.000%
4) 1,2-Dichloroethane-d4	4.969	65	4621	0.547	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	110.000%
7) 1,2-Dichloropropane-d6	5.995	67	5745	0.512	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	102.000%
8) Toluene-d8	7.253	98	15254	0.463	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	92.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	4495	0.535	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	108.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.374	75	20	0.020	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091724\
Data File : VV037308.D
Acq On : 17 Sep 2024 11:31
Operator : SY/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Sep 18 05:37:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM091324.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 03:38:32 2024
Response via : Initial Calibration

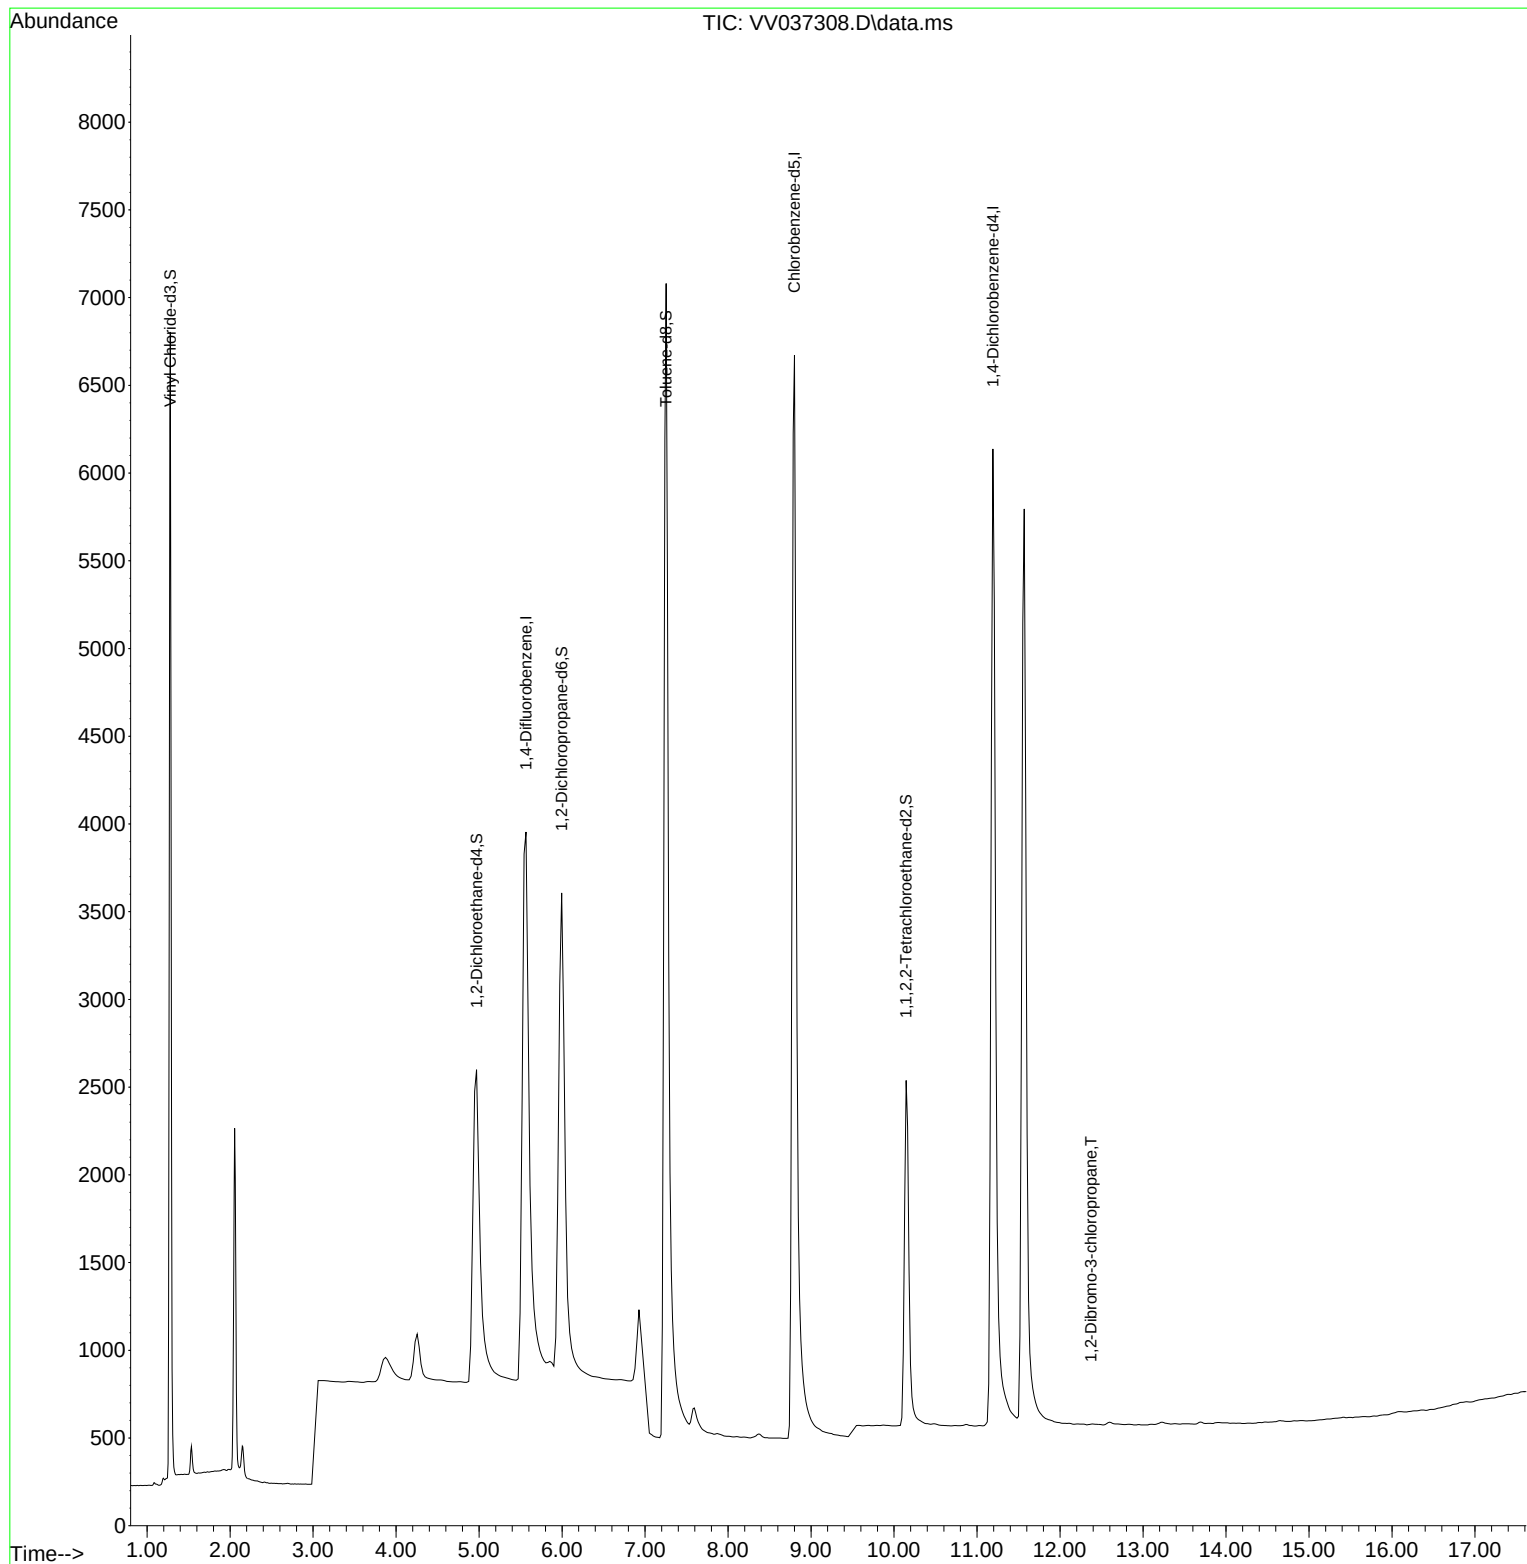

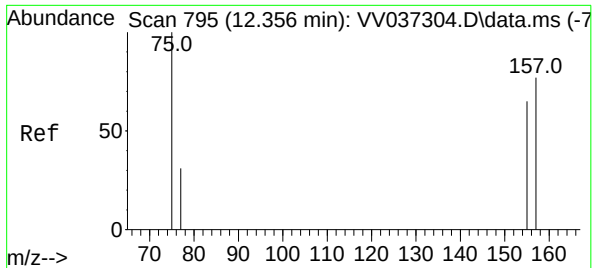

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.020 ug/L
 RT: 12.374 min Scan# 796
 Delta R.T. 0.017 min
 Lab File: VV037308.D
 Acq: 17 Sep 2024 11:31

Instrument :
 MSVOA_V
 ClientSampleId :

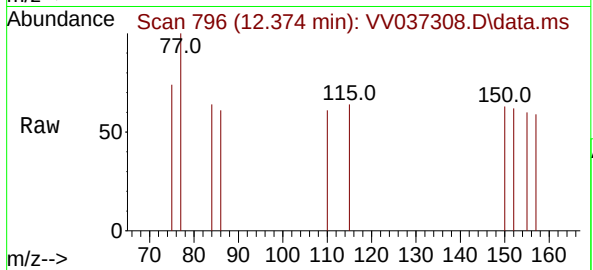

Tgt Ion: 75	Resp: 20
Ion Ratio	Lower Upper
75	100
157	79.7 63.8 95.6
155	81.3 56.1 84.1

