

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091724\
 Data File : VV037307.D
 Acq On : 17 Sep 2024 10:43
 Operator : SY/MD
 Sample : P3391-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MDL-WATER-QT3-2024-06

Quant Time: Sep 18 05:37:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM091324.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Sep 14 03:38:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	12229	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	11983	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	5880	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	7320	0.559	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	112.000%
4) 1,2-Dichloroethane-d4	4.969	65	4395	0.589	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	118.000%
7) 1,2-Dichloropropane-d6	5.996	67	5489	0.552	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	110.000%
8) Toluene-d8	7.254	98	14170	0.485	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	98.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	4131	0.555	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	110.000%
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.280	62	521	0.044	ug/L #	57
6) Trichloroethene	5.852	95	335	0.036	ug/L	94
9) 1,2-Dibromoethane	8.321	107	193	0.034	ug/L #	88
12) 1,2,3-Trichloropropane	10.214	75	182	0.038	ug/L	92
13) 1,2-Dibromo-3-chloropr...	12.374	75	36	0.042	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091724\
Data File : VV037307.D
Acq On : 17 Sep 2024 10:43
Operator : SY/MD
Sample : P3391-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT3-2024-06

Quant Time: Sep 18 05:37:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM091324.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 03:38:32 2024
Response via : Initial Calibration

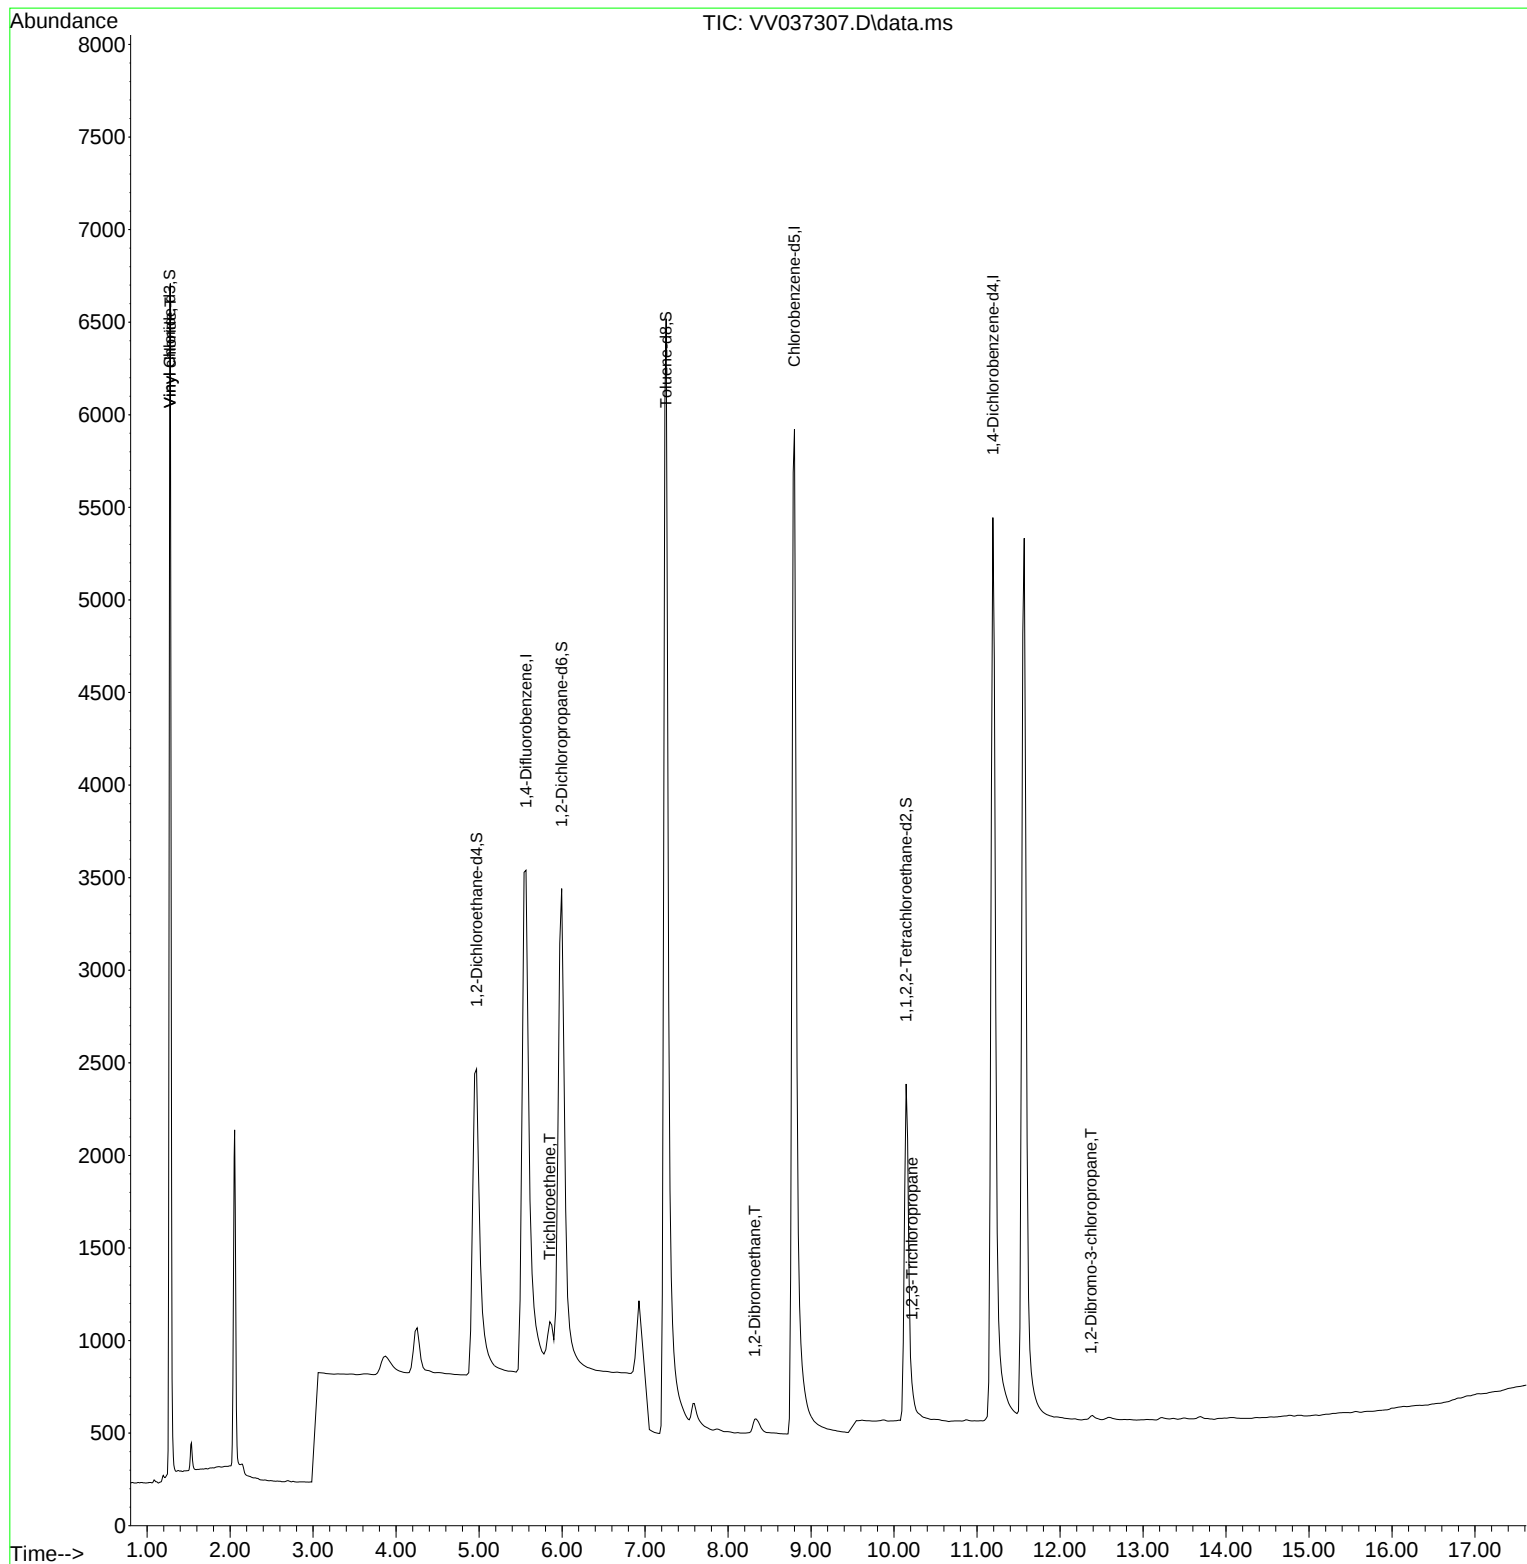

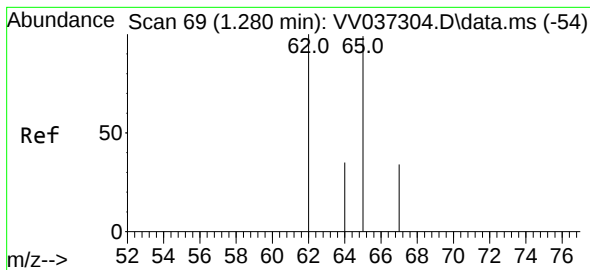

#3

Vinyl chloride

Concen: 0.044 ug/L

RT: 1.280 min Scan# 69

Delta R.T. 0.000 min

Lab File: VV037307.D

Acq: 17 Sep 2024 10:43

Instrument :

MSVOA_V

ClientSampleId :





MDL-WATER-QT3-2024-06

Tgt Ion: 62 Resp: 521

Ion Ratio Lower Upper

62 100

64 60.1 24.6 45.6#

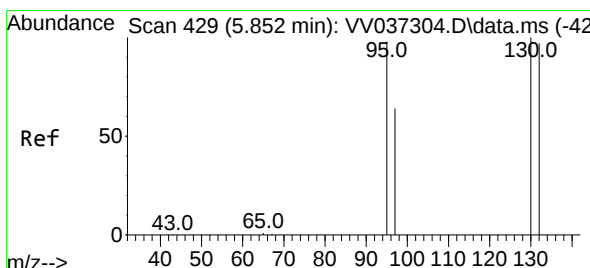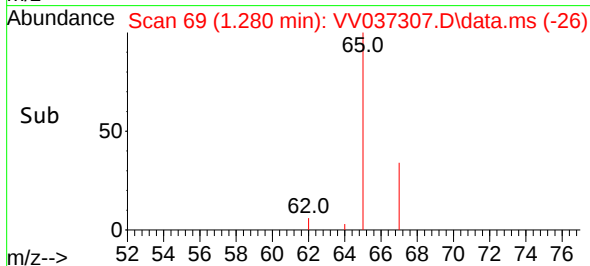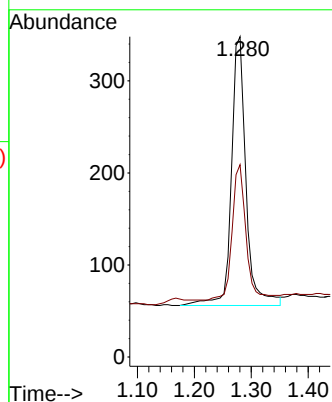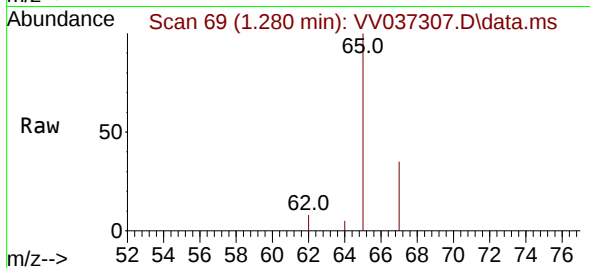

#6

Trichloroethene

Concen: 0.036 ug/L

RT: 5.852 min Scan# 429

Delta R.T. 0.000 min

Lab File: VV037307.D

Acq: 17 Sep 2024 10:43

Tgt Ion: 95 Resp: 335




Ion Ratio Lower Upper


95 100

97 80.2 46.4 86.2

132 95.7 67.5 125.4

130 96.6 70.3 130.7


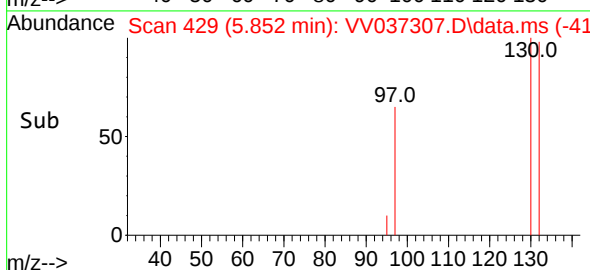
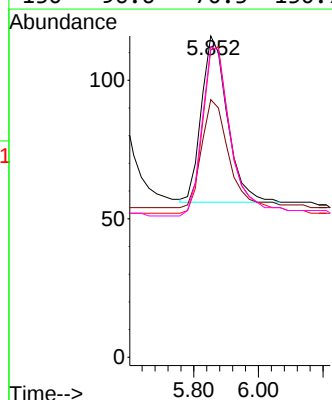
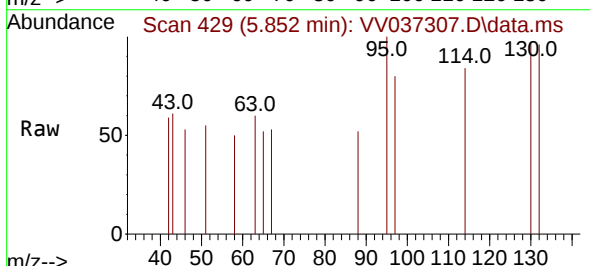


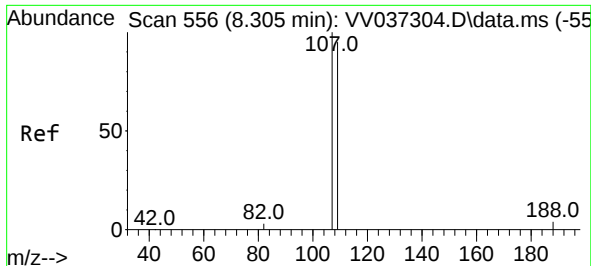

#9
1,2-Dibromoethane
Concen: 0.034 ug/L
RT: 8.321 min Scan# 51
Delta R.T. 0.016 min
Lab File: VV037307.D
Acq: 17 Sep 2024 10:43




Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT3-2024-06


Tgt Ion:107 Resp: 193
Ion Ratio Lower Upper
107 100
109 96.7 67.0 124.4
188 57.8 6.9 10.3#

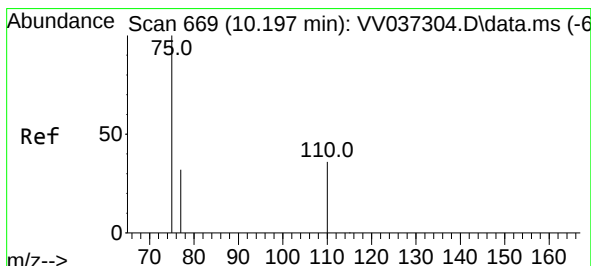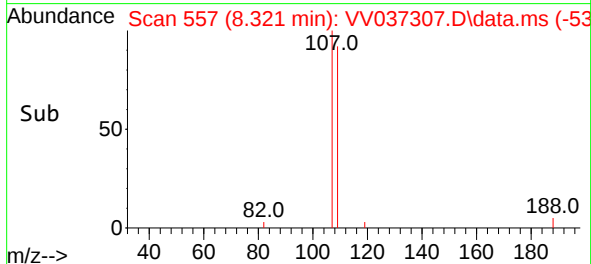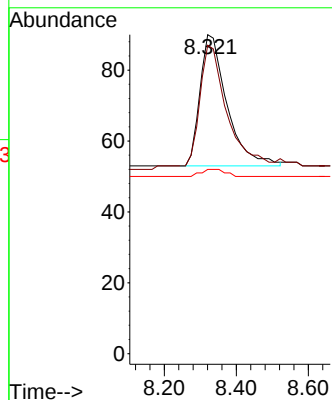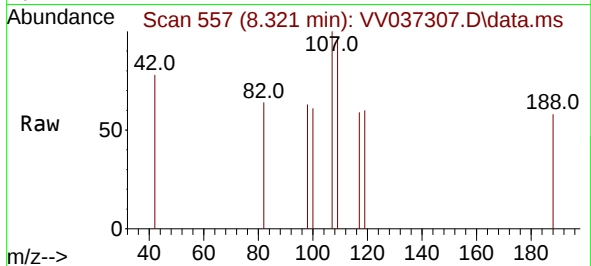

#12
1,2,3-Trichloropropane
Concen: 0.038 ug/L
RT: 10.214 min Scan# 670
Delta R.T. 0.017 min
Lab File: VV037307.D
Acq: 17 Sep 2024 10:43


Tgt Ion: 75 Resp: 182
Ion Ratio Lower Upper
75 100
110 46.2 32.7 49.1
77 28.0 26.1 39.1

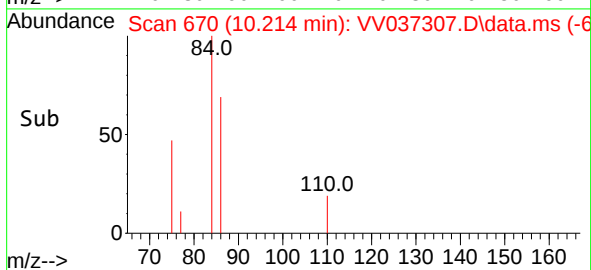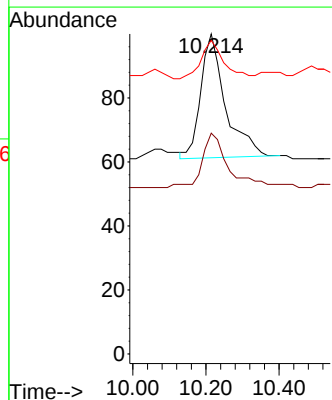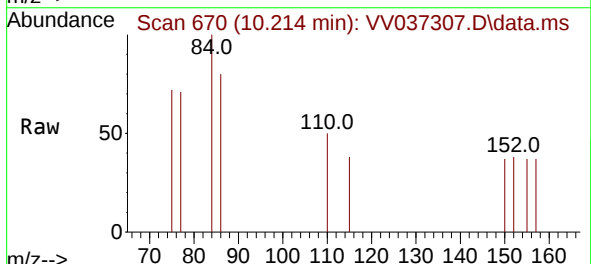

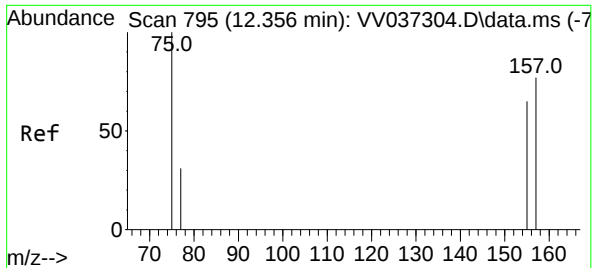

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.042 ug/L
 RT: 12.374 min Scan# 796
 Delta R.T. 0.017 min
 Lab File: VV037307.D
 Acq: 17 Sep 2024 10:43

Instrument :
 MSVOA_V
 ClientSampleId :
 MDL-WATER-QT3-2024-06

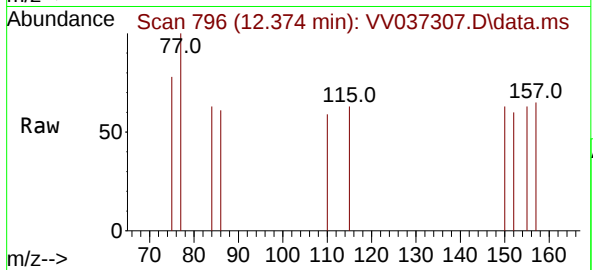

Tgt Ion: 75	Resp:	36
Ion	Ratio	Lower Upper
75	100	
157	82.6	63.8 95.6
155	79.7	56.1 84.1

