

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091724\
 Data File : VV037309.D
 Acq On : 17 Sep 2024 11:55
 Operator : SY/MD
 Sample : P3967-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP3

Quant Time: Sep 18 05:37:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM091324.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Sep 14 03:38:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	12878	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	12665	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	6387	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	7324	0.531	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	106.000%
4) 1,2-Dichloroethane-d4	4.970	65	4397	0.560	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	112.000%
7) 1,2-Dichloropropane-d6	5.996	67	5439	0.517	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	104.000%
8) Toluene-d8	7.254	98	14949	0.485	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	96.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	4286	0.545	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	108.000%
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.280	62	1183	0.095	ug/L	83
6) Trichloroethene	5.853	95	7213	0.729	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091724\
Data File : VV037309.D
Acq On : 17 Sep 2024 11:55
Operator : SY/MD
Sample : P3967-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP3

Quant Time: Sep 18 05:37:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM091324.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 03:38:32 2024
Response via : Initial Calibration

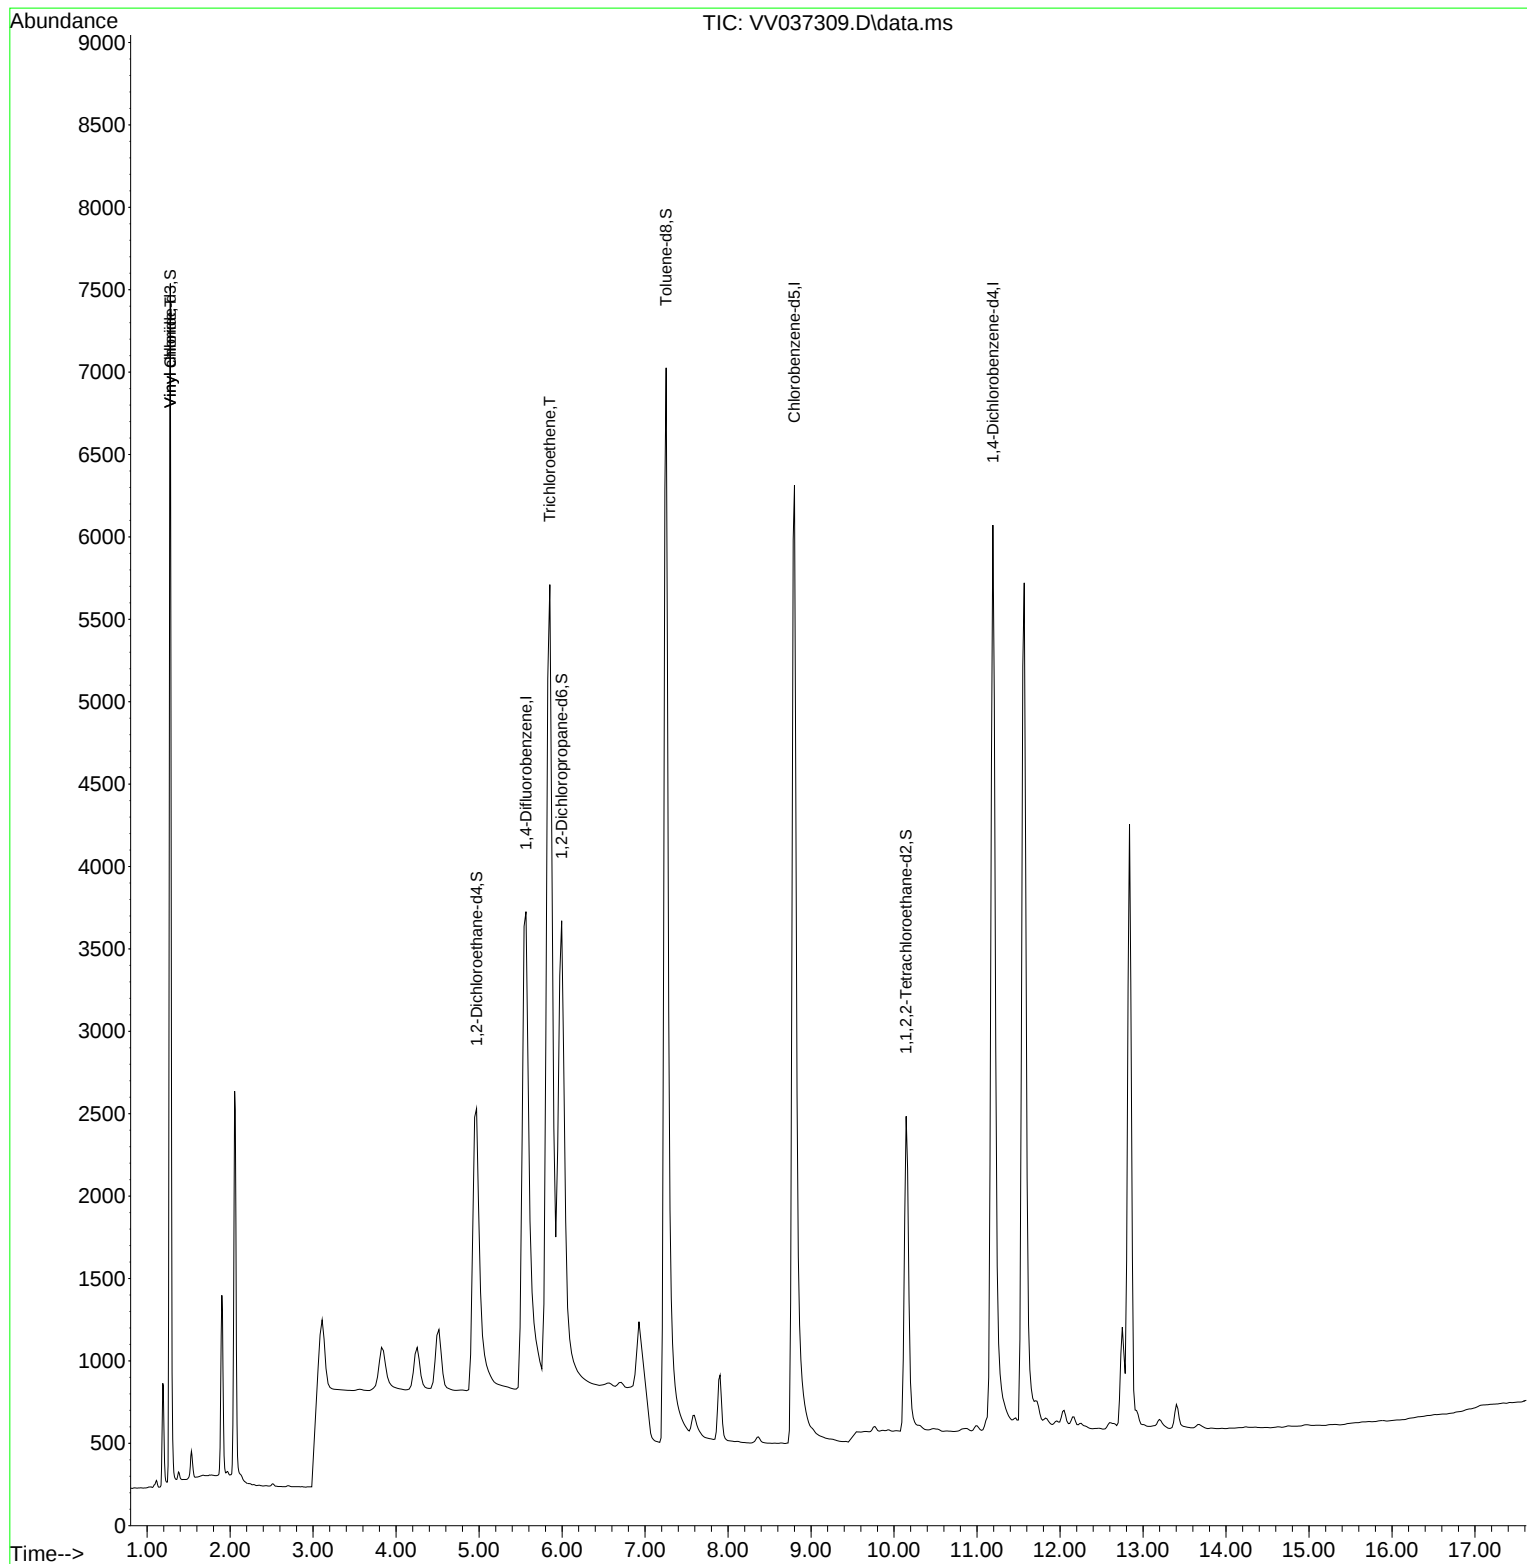

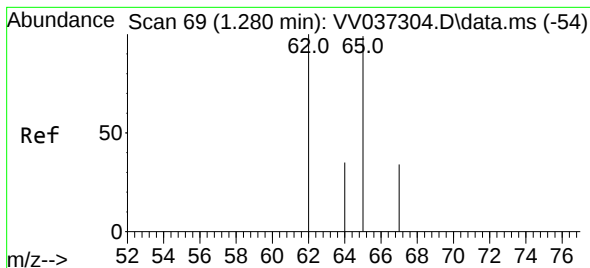

#3

Vinyl chloride

Concen: 0.095 ug/L

RT: 1.280 min Scan# 69

Delta R.T. 0.000 min

Lab File: VV037309.D

Acq: 17 Sep 2024 11:55

Instrument :

MSVOA_V

ClientSampleId :





C0AP3

Tgt Ion: 62 Resp: 1183

Ion Ratio Lower Upper

62 100

64 44.9 24.6 45.6

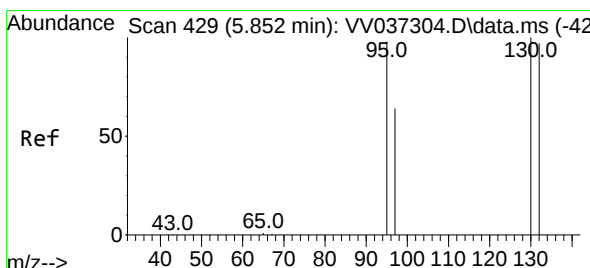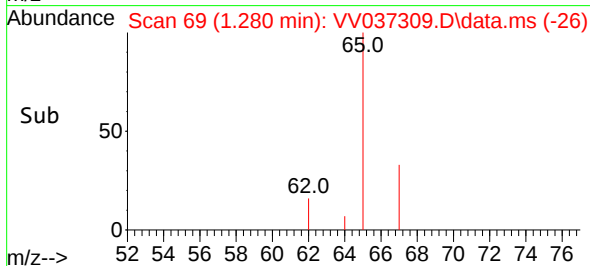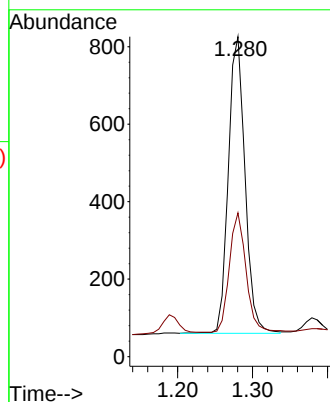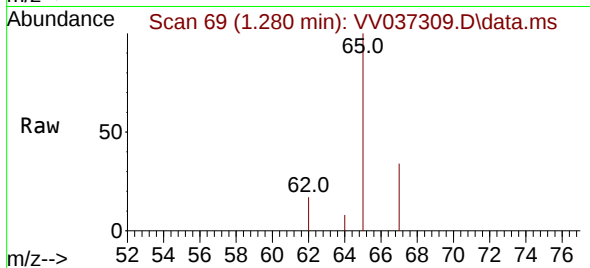

#6

Trichloroethene

Concen: 0.729 ug/L

RT: 5.853 min Scan# 429

Delta R.T. 0.000 min

Lab File: VV037309.D

Acq: 17 Sep 2024 11:55

Tgt Ion: 95 Resp: 7213

Ion Ratio Lower Upper

95 100

97 65.6 46.4 86.2

132 96.6 67.5 125.4

130 100.2 70.3 130.7

