

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091724\
 Data File : VV037317.D
 Acq On : 17 Sep 2024 15:08
 Operator : SY/MD
 Sample : P3990-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM4

Quant Time: Sep 18 05:39:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM091324.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Sep 14 03:38:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	12096	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	12012	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	6066	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	7117	0.550	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	110.000%
4) 1,2-Dichloroethane-d4	4.970	65	4371	0.593	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	118.000%
7) 1,2-Dichloropropane-d6	5.996	67	5369	0.539	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	108.000%
8) Toluene-d8	7.254	98	14278	0.488	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	98.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	4229	0.567	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	114.000%
Target Compounds						
6) Trichloroethene	5.852	95	2036	0.217	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091724\
Data File : VV037317.D
Acq On : 17 Sep 2024 15:08
Operator : SY/MD
Sample : P3990-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM4


Quant Time: Sep 18 05:39:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM091324.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 03:38:32 2024
Response via : Initial Calibration

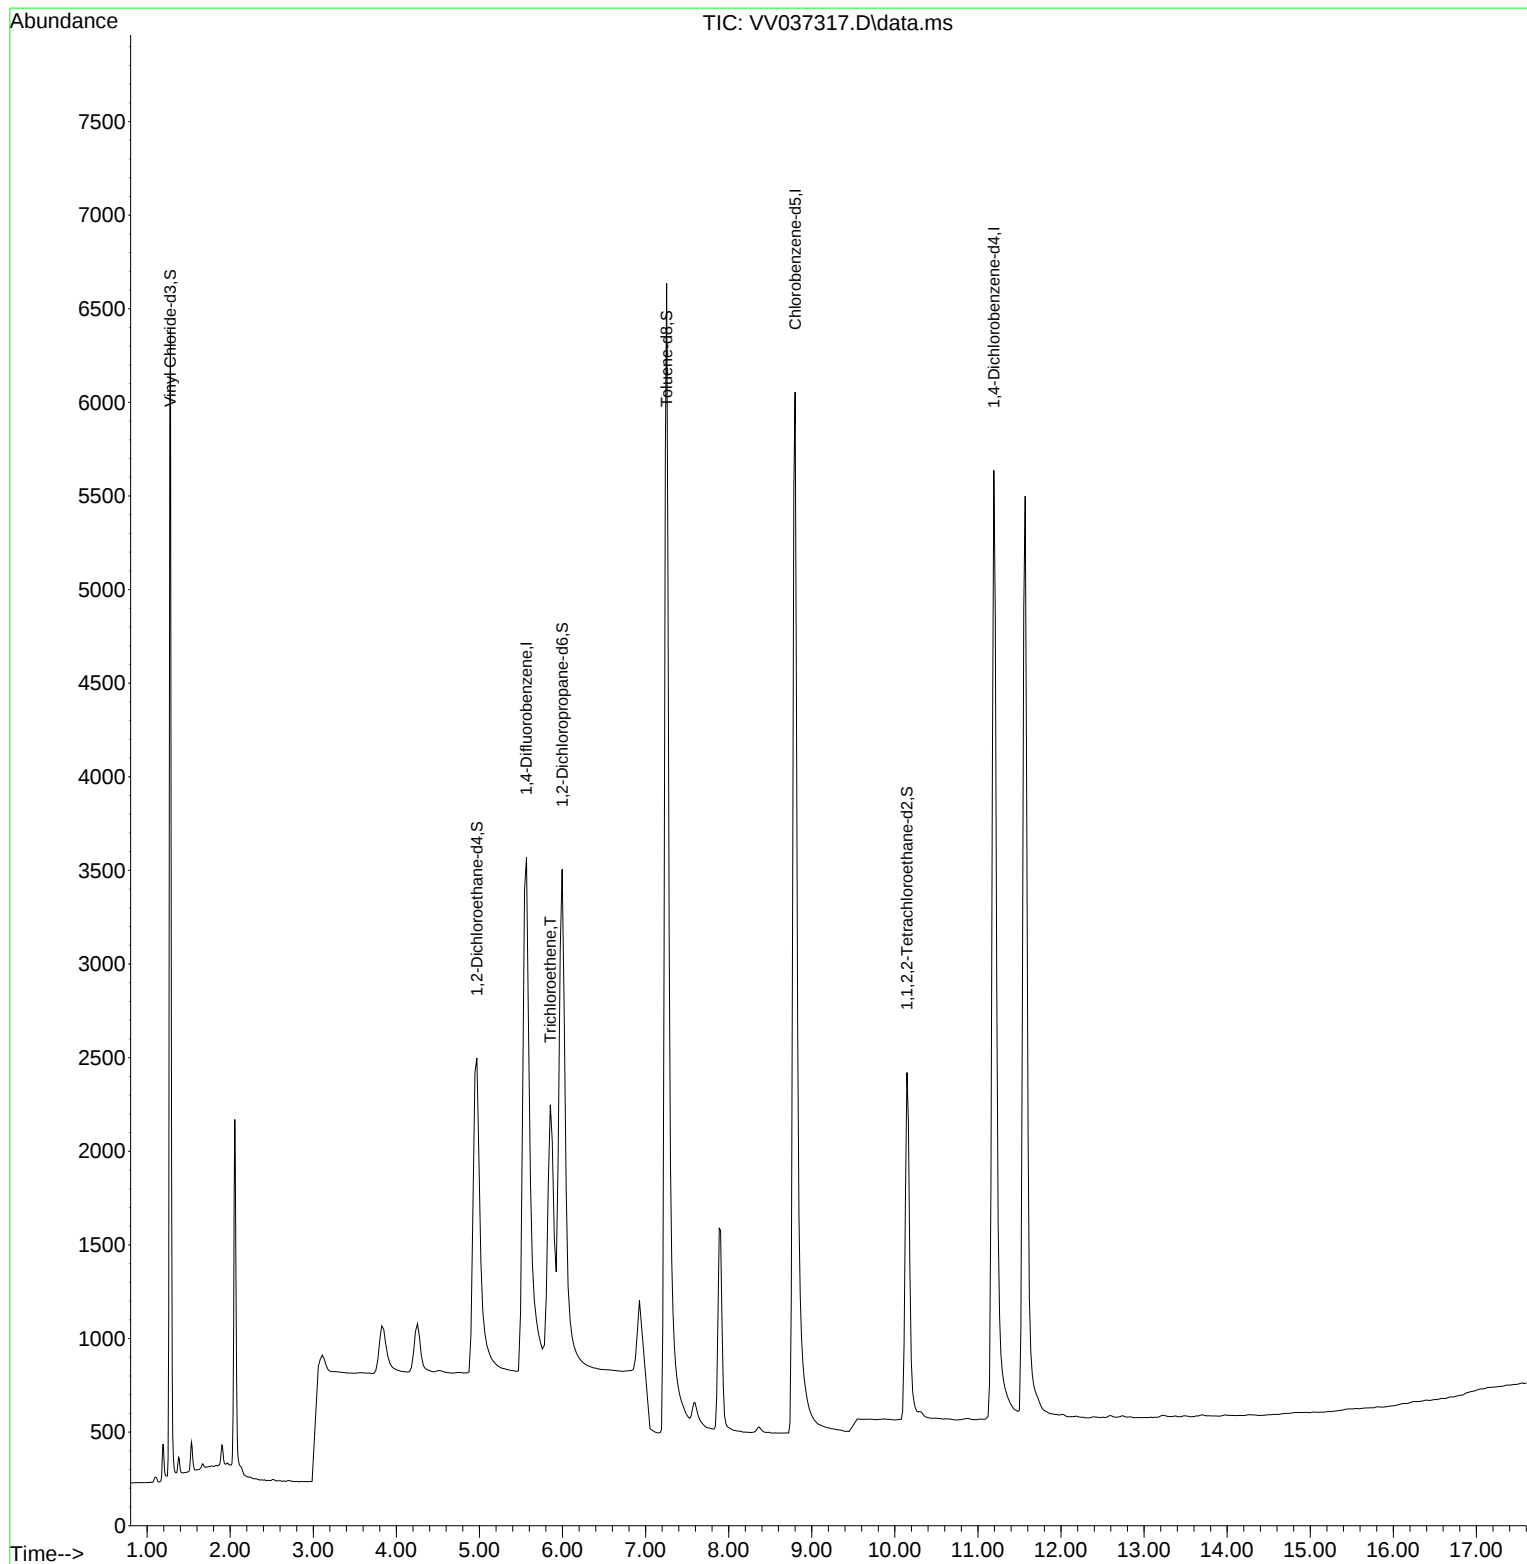

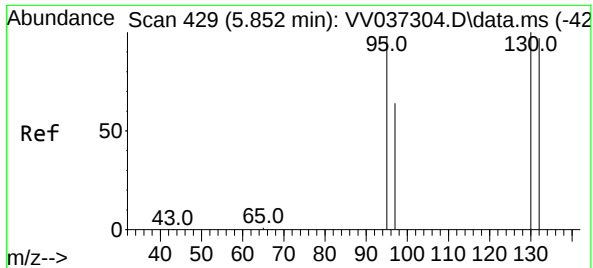

#6
 Trichloroethene
 Concen: 0.217 ug/L
 RT: 5.852 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VV037317.D
 Acq: 17 Sep 2024 15:08

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM4

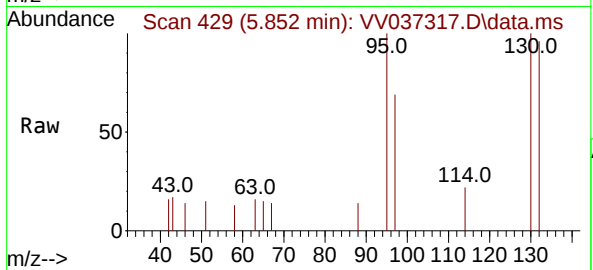

Tgt Ion: 95	Resp: 2036
Ion Ratio	Lower Upper
95 100	
97 68.8	46.4 86.2
132 95.6	67.5 125.4
130 100.0	70.3 130.7

