


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091724\
Data File : VV037303.D
Acq On : 17 Sep 2024 07:53
Operator : SY/MD
Sample : BFB221
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB221

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM091324.M
Title : TRACE VOA SOM01.0
Last Update : Sat Sep 14 03:38:32 2024

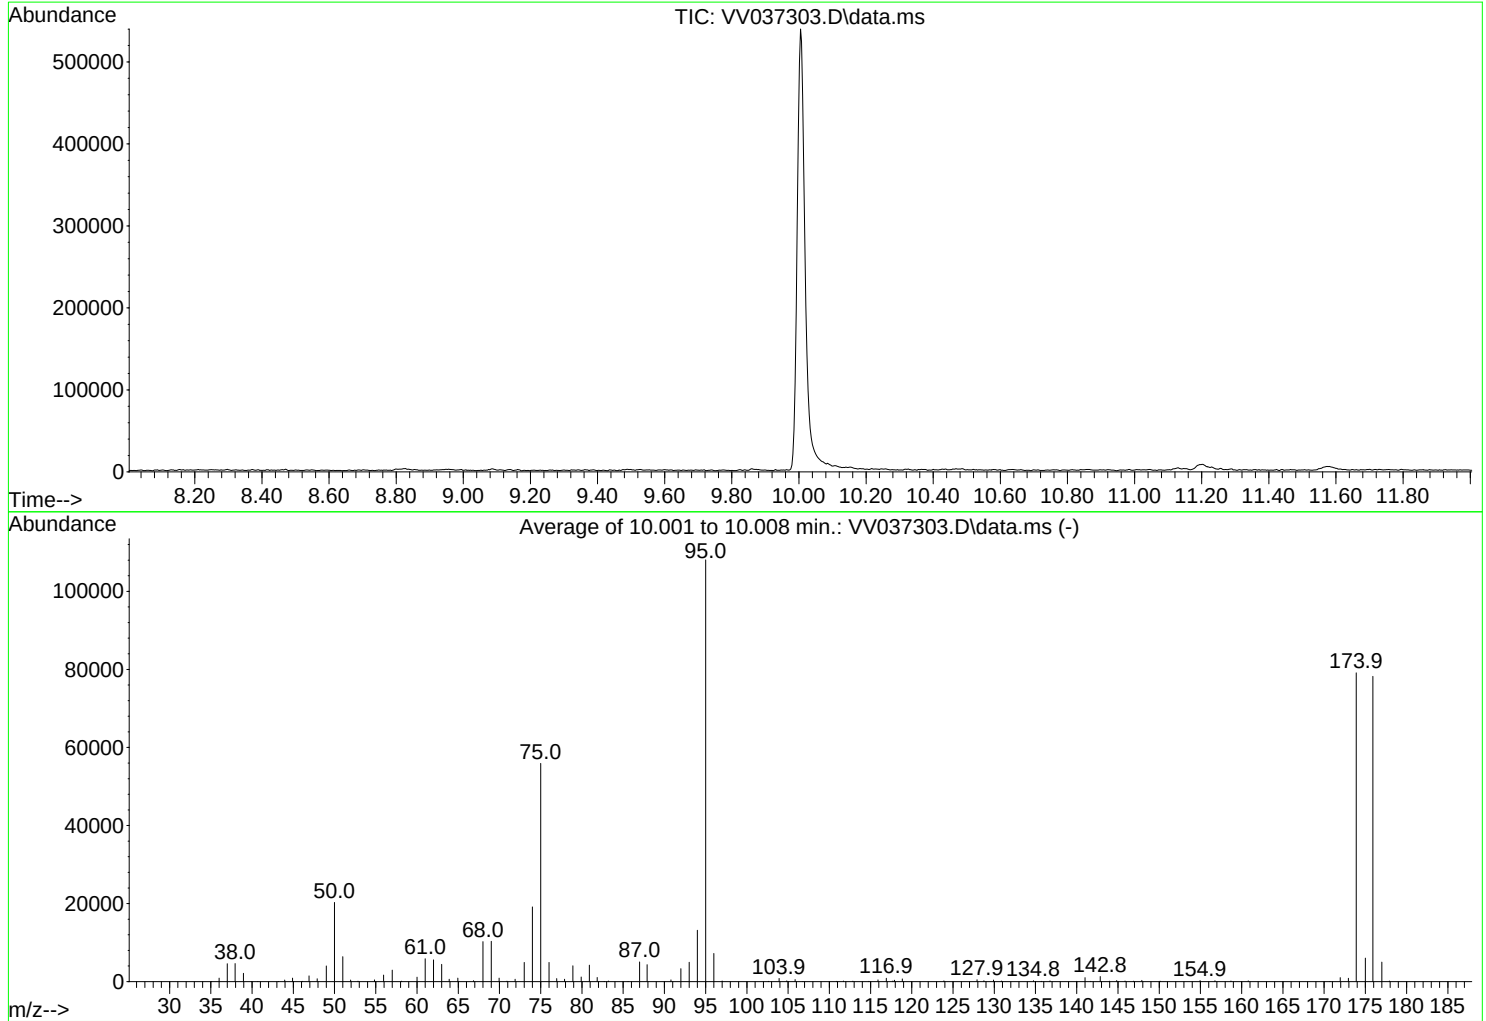

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2775

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.8	20283	PASS
75	95	30	80	51.7	55904	PASS
95	95	100	100	100.0	108075	PASS
96	95	5	9	6.7	7215	PASS
173	174	0.00	2	1.1	879	PASS
174	95	50	120	73.2	79120	PASS
175	174	5	9	7.6	6041	PASS
176	174	95	101	98.9	78235	PASS
177	176	5	9	6.4	5001	PASS

m/z	Abundance
36.20	109.0
37.00	112.0
37.90	107.0
38.90	115.0
40.00	331.0
41.00	105.0
41.80	108.0
42.20	104.0
43.00	201.0
43.90	718.0
54.10	139.0
55.10	121.0
62.00	146.0
76.70	125.0
79.10	114.0
133.20	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

m/z	Abundance
36.00	1073.0
37.00	4848.0
38.00	4659.0
39.00	2211.0
39.80	333.0
42.00	114.0
43.00	146.0
44.00	1171.0
44.90	899.0
46.90	1414.0
47.90	691.0
49.00	3951.0
50.00	19944.0
51.00	6345.0
51.90	391.0
52.90	142.0
54.90	451.0
56.00	1686.0
57.00	2915.0
58.10	165.0
60.00	1078.0
61.00	5582.0
62.00	5733.0
63.00	4138.0
63.90	430.0
64.90	891.0
66.90	255.0
68.00	10343.0
69.00	9671.0
70.00	934.0
70.90	124.0
71.90	643.0
73.00	4719.0
74.00	18472.0
75.00	53784.0
76.00	4761.0
77.00	793.0
77.90	601.0
78.90	4014.0
79.90	1105.0
80.90	3823.0
81.80	1090.0
82.70	100.0
83.20	125.0
85.60	104.0
87.00	4963.0
87.90	3968.0
90.80	425.0
92.00	3308.0
93.00	4820.0
94.00	12631.0
95.00	104856.0
96.00	6949.0
97.10	172.0
103.90	690.0
104.90	202.0
105.90	483.0
106.80	129.0
110.90	133.0
111.70	181.0
113.00	102.0
114.80	165.0
115.90	392.0
116.90	890.0
117.70	477.0
118.80	655.0
123.90	221.0
127.90	446.0
128.70	222.0
130.00	391.0
130.90	154.0
134.70	174.0
136.80	223.0
141.00	1024.0
141.70	126.0
142.90	1081.0
144.00	100.0
144.80	255.0
145.80	159.0
146.90	135.0
147.90	318.0
150.10	108.0
155.00	233.0
156.80	278.0
158.80	153.0
160.90	247.0
171.90	933.0
173.00	805.0
173.90	74800.0
175.00	5431.0
175.90	72024.0
177.00	4869.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

177.90

193.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

m/z	Abundance
35.10	101.0
36.00	1057.0
37.00	4824.0
38.00	4985.0
39.00	2377.0
39.90	376.0
43.20	126.0
44.00	1120.0
44.90	924.0
46.10	105.0
46.90	1606.0
47.90	774.0
49.00	4113.0
50.00	20968.0
51.00	6623.0
51.90	442.0
52.90	159.0
54.80	473.0
56.00	1719.0
57.00	3040.0
58.20	153.0
60.00	1204.0
61.00	6206.0
62.00	5912.0
63.00	4629.0
63.90	654.0
64.90	943.0
66.90	254.0
68.00	10621.0
69.00	10705.0
69.90	959.0
70.90	164.0
71.90	660.0
73.00	5124.0
74.00	19968.0
75.00	57960.0
76.00	5180.0
77.00	776.0
77.90	641.0
78.90	4311.0
79.90	1251.0
80.90	4329.0
81.80	1122.0
83.20	187.0
87.00	5154.0
87.90	4485.0
90.80	499.0
92.00	3397.0
93.00	5194.0
94.00	13506.0
95.00	112120.0
96.00	7503.0
97.00	156.0
102.60	123.0
103.90	876.0
104.80	216.0
105.80	519.0
110.90	127.0
111.70	208.0
112.80	133.0
114.80	110.0
115.90	438.0
116.90	914.0
117.90	553.0
118.90	743.0
123.90	244.0
127.90	498.0
128.80	249.0
129.90	409.0
130.90	145.0
134.80	254.0
135.70	144.0
136.70	202.0
140.00	117.0
141.00	1063.0
141.70	109.0
142.80	1351.0
143.90	133.0
144.90	309.0
145.90	171.0
146.90	159.0
147.90	327.0
150.10	118.0
154.90	273.0
156.80	285.0
158.70	146.0
160.80	213.0
172.00	1045.0
173.00	914.0
173.90	81736.0
175.00	6336.0
175.90	81128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

177.005125.0

177.90198.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

m/z	Abundance
36.00	935.0
37.00	4447.0
38.00	4620.0
39.00	2216.0
39.90	421.0
40.70	144.0
42.80	143.0
44.00	1123.0
44.90	860.0
46.10	136.0
46.90	1413.0
47.90	737.0
49.00	3966.0
50.00	19936.0
51.00	6207.0
52.00	421.0
52.80	140.0
54.80	427.0
55.90	1679.0
57.00	2886.0
58.20	116.0
60.00	1155.0
61.00	5821.0
62.00	5488.0
63.00	4515.0
63.90	834.0
65.00	863.0
66.80	274.0
68.00	9802.0
69.00	10645.0
69.90	830.0
70.90	123.0
71.90	592.0
73.00	4968.0
74.00	18952.0
75.00	55968.0
76.00	4782.0
76.90	807.0
77.90	587.0
78.90	4170.0
79.90	1214.0
80.90	4489.0
81.90	1021.0
83.20	202.0
87.00	5011.0
87.90	4574.0
90.80	473.0
92.00	3291.0
93.00	4888.0
94.00	13297.0
95.00	107248.0
96.00	7192.0
96.90	210.0
102.60	177.0
103.90	848.0
104.80	218.0
105.80	556.0
111.70	149.0
112.80	137.0
115.90	491.0
116.90	812.0
117.90	611.0
118.90	709.0
123.90	177.0
127.90	535.0
128.70	242.0
129.80	423.0
130.80	147.0
134.80	272.0
135.70	156.0
136.80	180.0
140.00	176.0
141.00	959.0
142.80	1463.0
143.90	150.0
144.90	351.0
145.90	179.0
146.90	133.0
147.90	313.0
150.10	106.0
154.90	307.0
156.70	227.0
158.60	166.0
160.70	190.0
170.70	113.0
172.00	1150.0
172.90	917.0
173.90	80824.0
175.00	6357.0
175.90	81552.0
177.00	5009.0
177.90	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221