


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091818\
 Data File : VV007595.D
 Acq On : 18 Sep 2018 10:23
 Operator : SY/MD
 Sample : BFB75
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB75

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091818WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Sep 19 04:15:09 2018

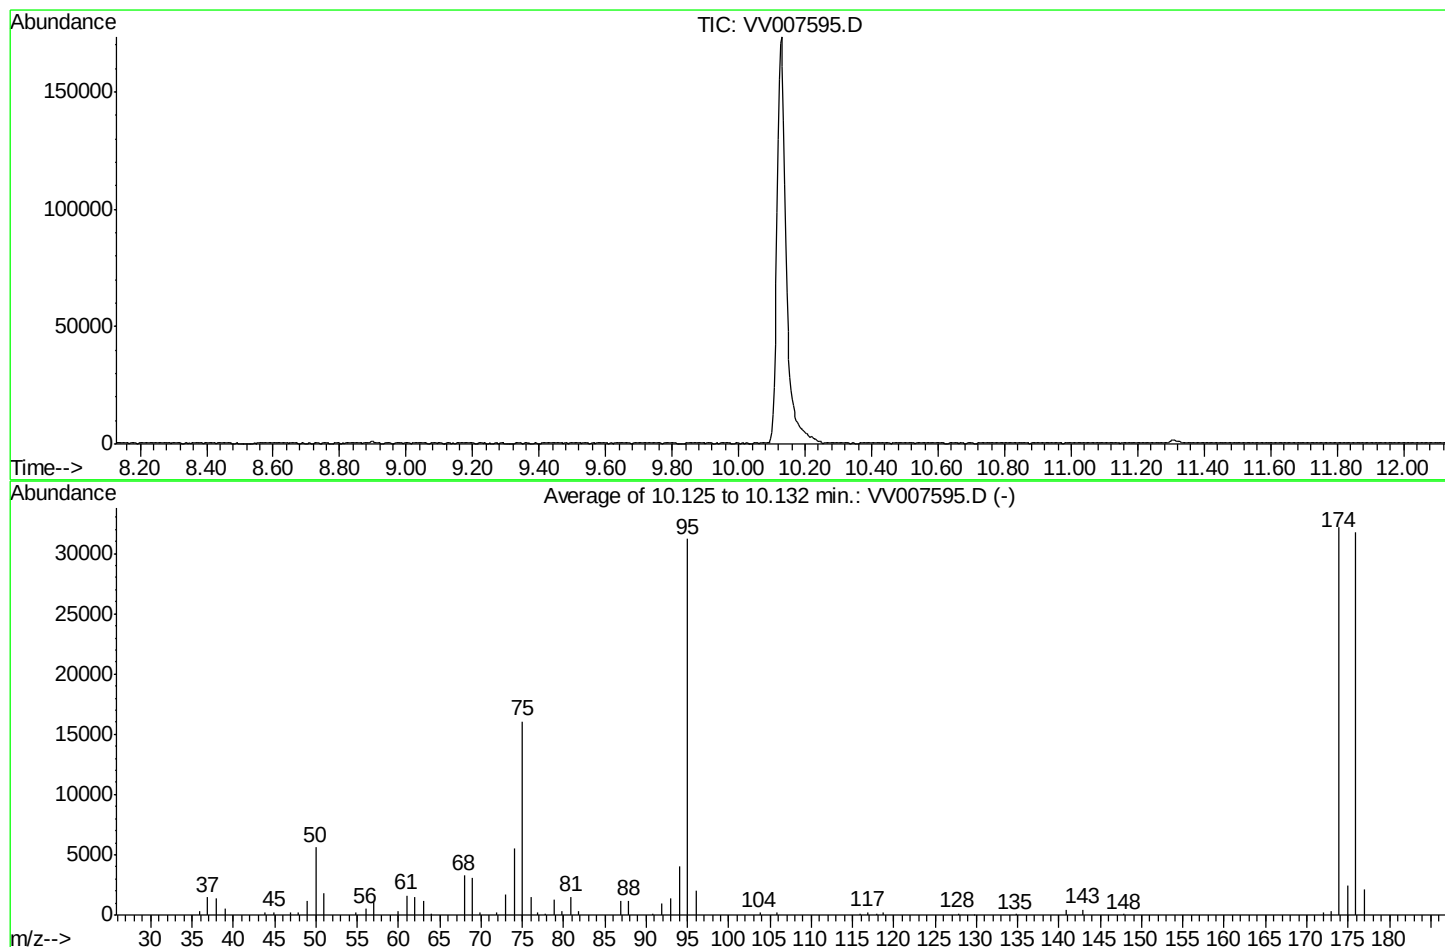

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	5584	PASS
75	95	30	80	51.4	16054	PASS
95	95	100	100	100.0	31216	PASS
96	95	5	9	6.4	1996	PASS
173	174	0.00	2	0.9	289	PASS
174	95	50	120	103.1	32178	PASS
175	174	5	9	7.4	2394	PASS
176	174	95	101	98.6	31722	PASS
177	176	5	9	6.6	2080	PASS

m/z	Abundance
43.90	334.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
35.90	306.0
36.90	1470.0
38.00	1457.0
38.90	513.0
43.90	543.0
44.90	276.0
47.00	229.0
47.90	228.0
49.00	1290.0
50.00	5613.0
51.00	1795.0
54.90	211.0
56.00	518.0
57.00	1097.0
59.90	325.0
61.00	1705.0
62.00	1593.0
63.00	1280.0
63.90	157.0
68.00	3346.0
69.00	3095.0
69.90	285.0
72.00	211.0
72.90	1617.0
74.00	5797.0
75.00	16584.0
76.00	1510.0
76.90	192.0
78.90	1218.0
79.80	365.0
80.90	1479.0
81.90	257.0
86.90	1259.0
87.90	1219.0
90.80	182.0
91.90	1000.0
92.90	1412.0
94.00	4103.0
95.00	31648.0
96.00	2039.0
103.80	181.0
105.90	174.0
115.80	147.0
116.90	199.0
117.90	129.0
118.70	200.0
127.80	129.0
134.80	102.0
140.90	414.0
142.90	422.0
172.00	181.0
172.90	449.0
173.90	32304.0
174.90	2415.0
175.90	31880.0
176.90	2197.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
35.90	300.0
36.90	1538.0
38.00	1396.0
39.00	557.0
43.90	567.0
44.90	247.0
47.00	234.0
47.90	214.0
49.00	1244.0
50.00	5747.0
51.00	1835.0
54.90	203.0
56.00	504.0
57.00	1057.0
59.90	345.0
61.00	1722.0
62.00	1574.0
63.00	1217.0
63.90	136.0
68.00	3348.0
69.00	3203.0
69.90	271.0
71.90	227.0
73.00	1713.0
74.00	5663.0
75.00	16520.0
76.00	1489.0
76.80	213.0
77.80	104.0
78.90	1275.0
79.80	353.0
80.90	1533.0
81.90	288.0
86.90	1164.0
87.90	1238.0
90.70	154.0
91.90	951.0
92.90	1456.0
94.00	4074.0
95.00	32128.0
96.00	2040.0
103.80	184.0
105.90	181.0
115.90	141.0
116.80	235.0
117.90	138.0
118.70	209.0
127.80	153.0
134.80	104.0
140.90	453.0
142.90	478.0
147.90	120.0
171.90	175.0
173.00	420.0
173.90	33072.0
174.90	2452.0
175.90	32656.0
176.90	2174.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
35.90	247.0
36.90	1440.0
38.00	1295.0
39.00	559.0
43.90	545.0
45.00	232.0
46.90	232.0
47.90	194.0
49.00	1140.0
50.00	5392.0
51.00	1665.0
54.90	160.0
56.00	434.0
56.90	916.0
60.00	332.0
61.00	1521.0
62.00	1350.0
63.00	1106.0
68.00	3078.0
69.00	3091.0
69.90	236.0
71.90	214.0
73.00	1646.0
74.00	5121.0
75.00	15058.0
76.00	1358.0
76.90	184.0
77.70	131.0
78.90	1239.0
79.90	342.0
80.90	1453.0
81.80	311.0
86.90	1035.0
87.90	1122.0
91.90	854.0
92.90	1391.0
94.00	3831.0
95.00	29872.0
96.00	1911.0
103.80	185.0
105.90	156.0
115.80	122.0
116.80	240.0
117.90	119.0
118.80	182.0
127.80	148.0
129.70	105.0
140.80	448.0
142.90	439.0
147.90	121.0
171.90	139.0
173.90	31160.0
174.90	2317.0
175.90	30632.0
176.90	1870.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75