
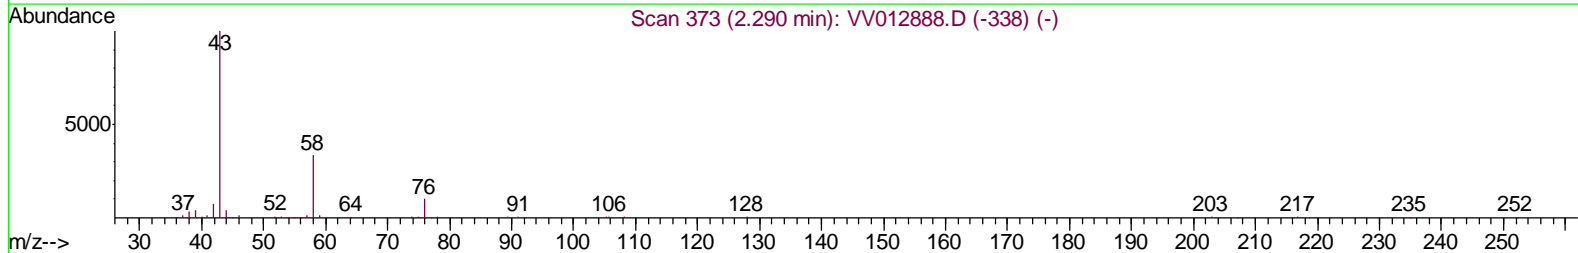
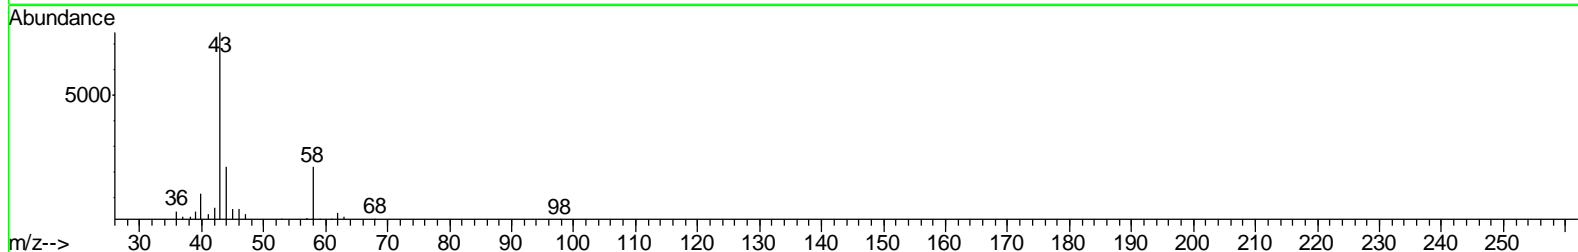


Data File : VV012895.D
Acq On : 18 Sep 2019 14:42
Operator : SY/MD
Sample : K4833-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 19 01:58:23 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 19 01:01:31 2019
Response via : Initial Calibration

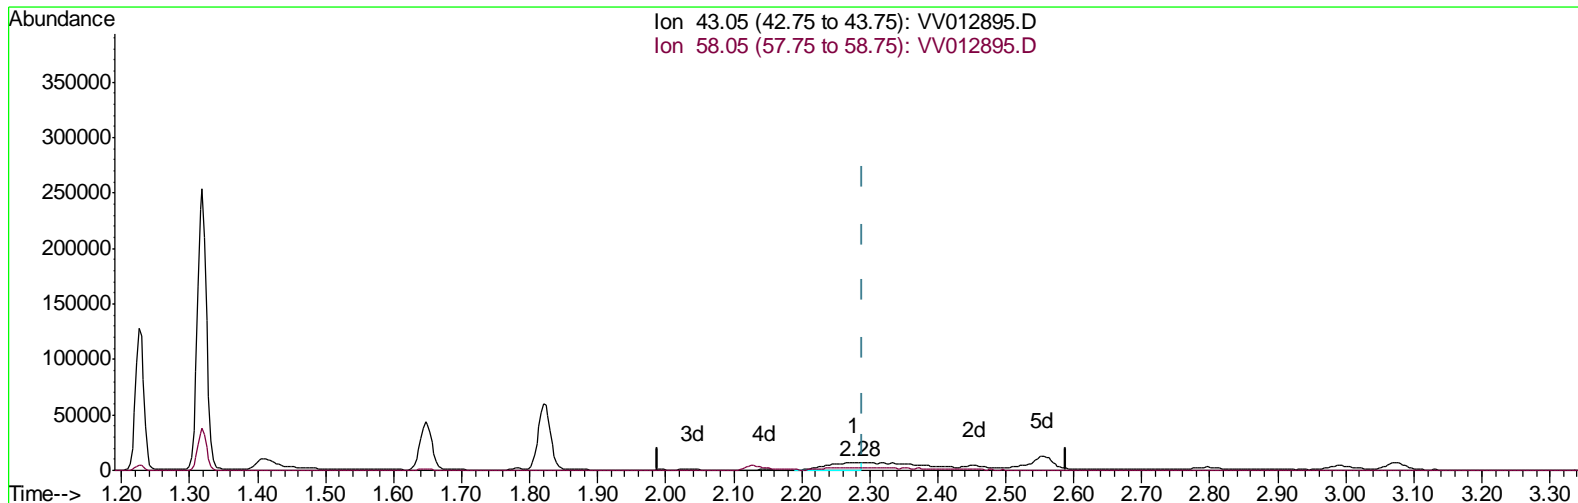

TIC: VV012895.D

(13) Acetone (T)
2.277min (-0.013) 4.99ug/L
response 22763

Ion	Exp%	Act%
43.05	100	100
58.05	12.20	2.38
0.00	0.00	0.00
0.00	0.00	0.00