

Data File : VV012903.D
Acq On : 18 Sep 2019 18:34
Operator : SY/MD
Sample : K4954-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CWK26

Manual Integrations
APPROVED

MMDadoda
9/19/2019 8:19:29 AM

Quant Time: Sep 19 04:37:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 19 01:01:31 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	374320	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	364559	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	128437	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	156126	4.21	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.20%
7) Chloroethane-d5	1.58	69	137892	4.72	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.40%
11) 1,1-Dichloroethene-d2	2.13	63	197812	3.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.40%
20) 2-Butanone-d5	3.99	46	325423m	41.95	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.90%
24) Chloroform-d	4.40	84	282651	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.40%
26) 1,2-Dichloroethane-d4	5.08	65	144239	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.60%
32) Benzene-d6	5.10	84	566738	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.80%
36) 1,2-Dichloropropane-d6	6.12	67	180394	4.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.00%
41) Toluene-d8	7.36	98	450425	4.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.00%
43) trans-1,3-Dichloropropene-	7.67	79	55633	4.21	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.20%
46) 2-Hexanone-d5	8.14	63	232503	41.82	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.64%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	127190	4.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	148180	5.34	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.80%

Target Compounds					Qvalue
3) Chloromethane	1.25	50	9628	0.370 ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data File : VV012903.D
Acq On : 18 Sep 2019 18:34
Operator : SY/MD
Sample : K4954-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
CWK26

Manual Integrations
APPROVED

MMDadoda
9/19/2019 8:19:29 AM

Quant Time: Sep 19 04:37:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 19 01:01:31 2019
Response via : Initial Calibration

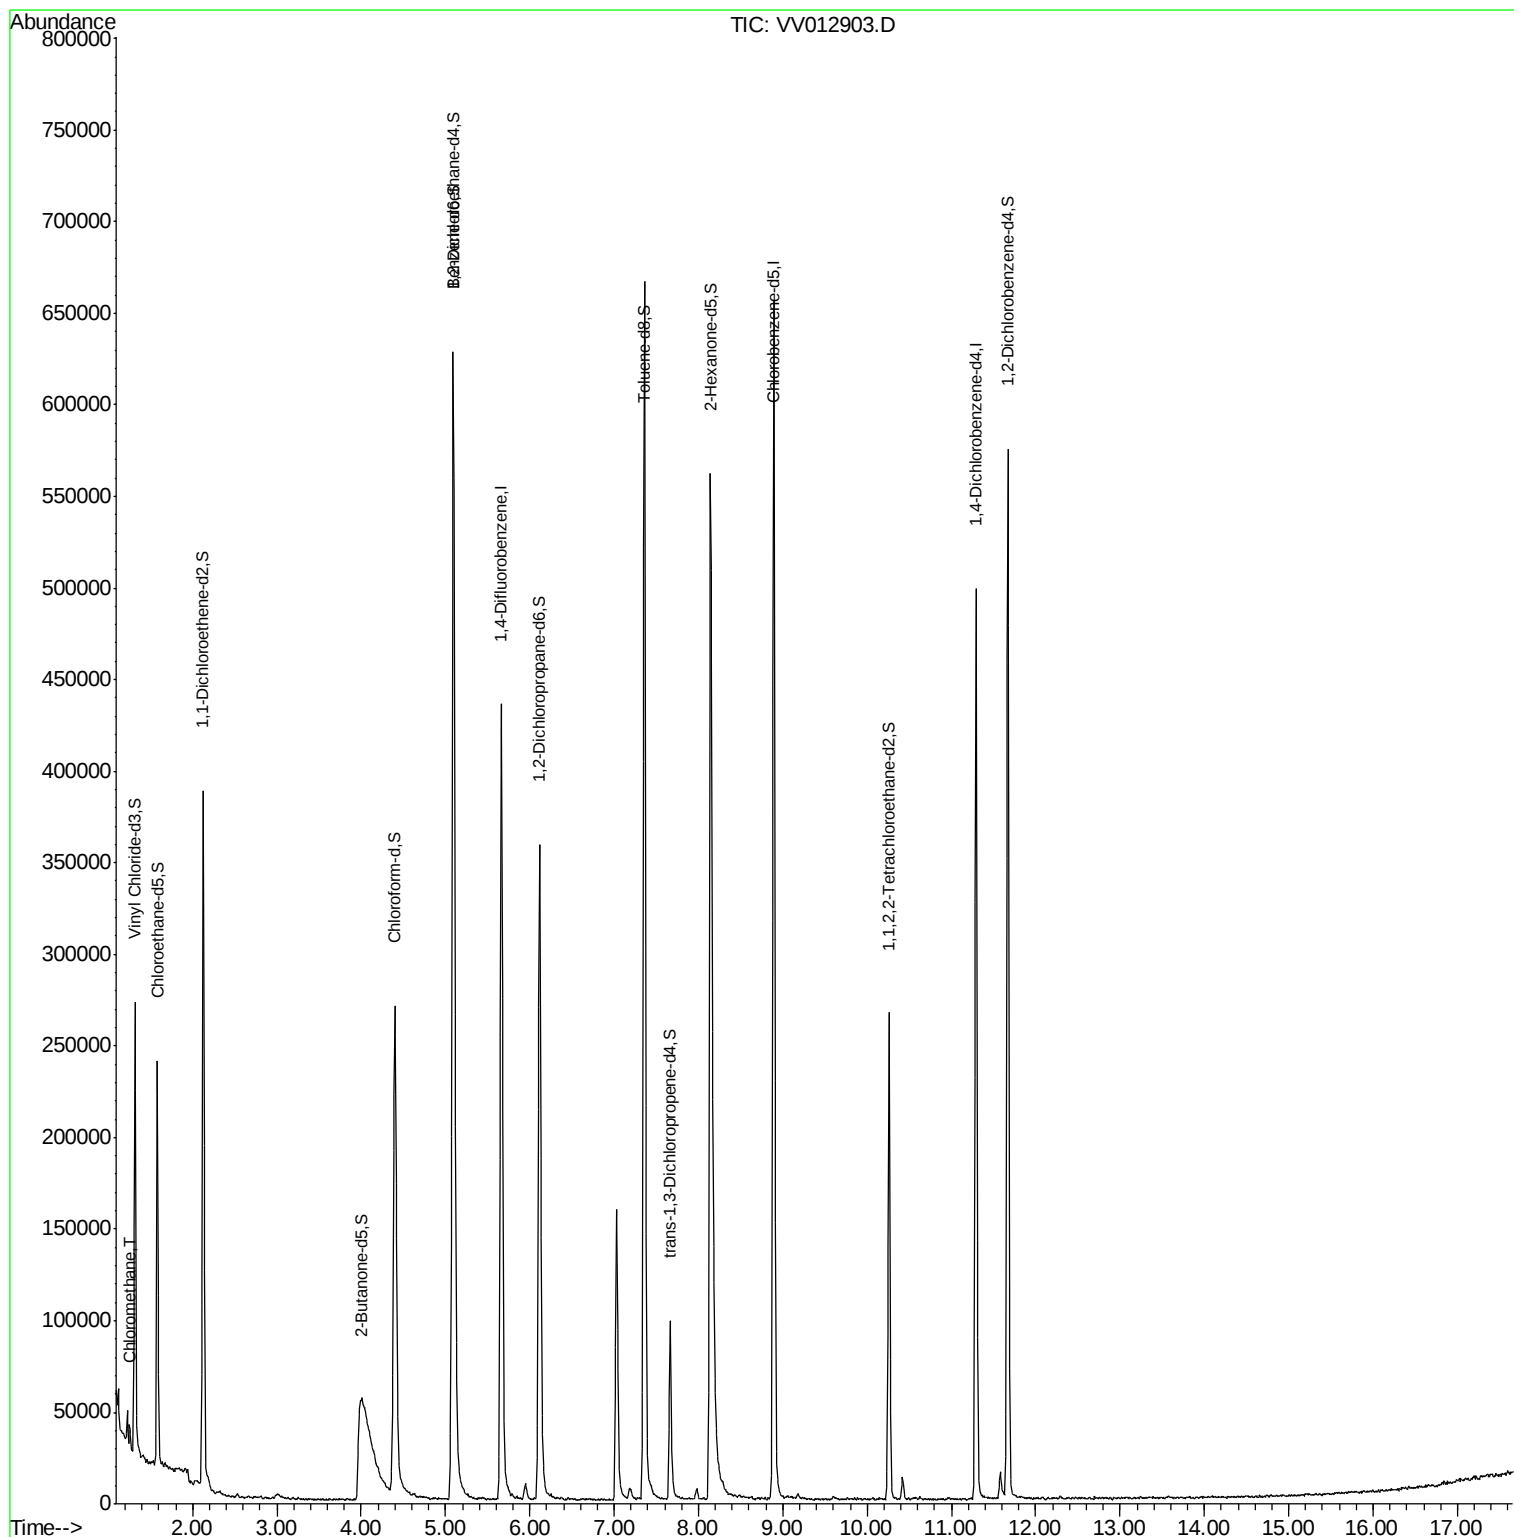

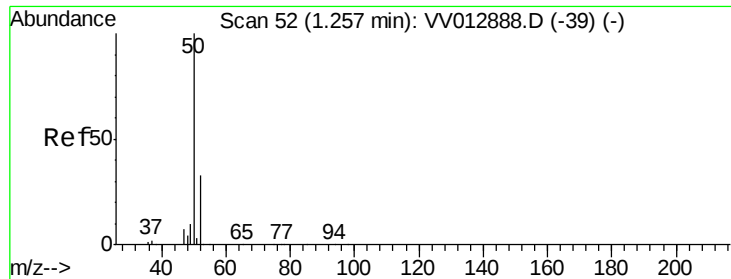

#3
 Chloromethane
 Concen: 0.370 ug/L
 RT: 1.25 min Scan# 51
 Delta R.T. -0.00 min
 Lab File: VV012903.D
 Acq: 18 Sep 2019 18:34

Instrument :
 MSVOA_V
 ClientSampleId :
 CWK26

Tgt Ion	Ratio	Lower	Upper
50	100		
52	30.3	22.8	42.4

Manual Integrations
 APPROVED

MMDadoda
 9/19/2019 8:19:29 AM

