


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091819\
 Data File : VV012887.D
 Acq On : 18 Sep 2019 08:33
 Operator : SY/MD
 Sample : BFB40
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB40

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091719WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Sep 19 03:01:33 2019

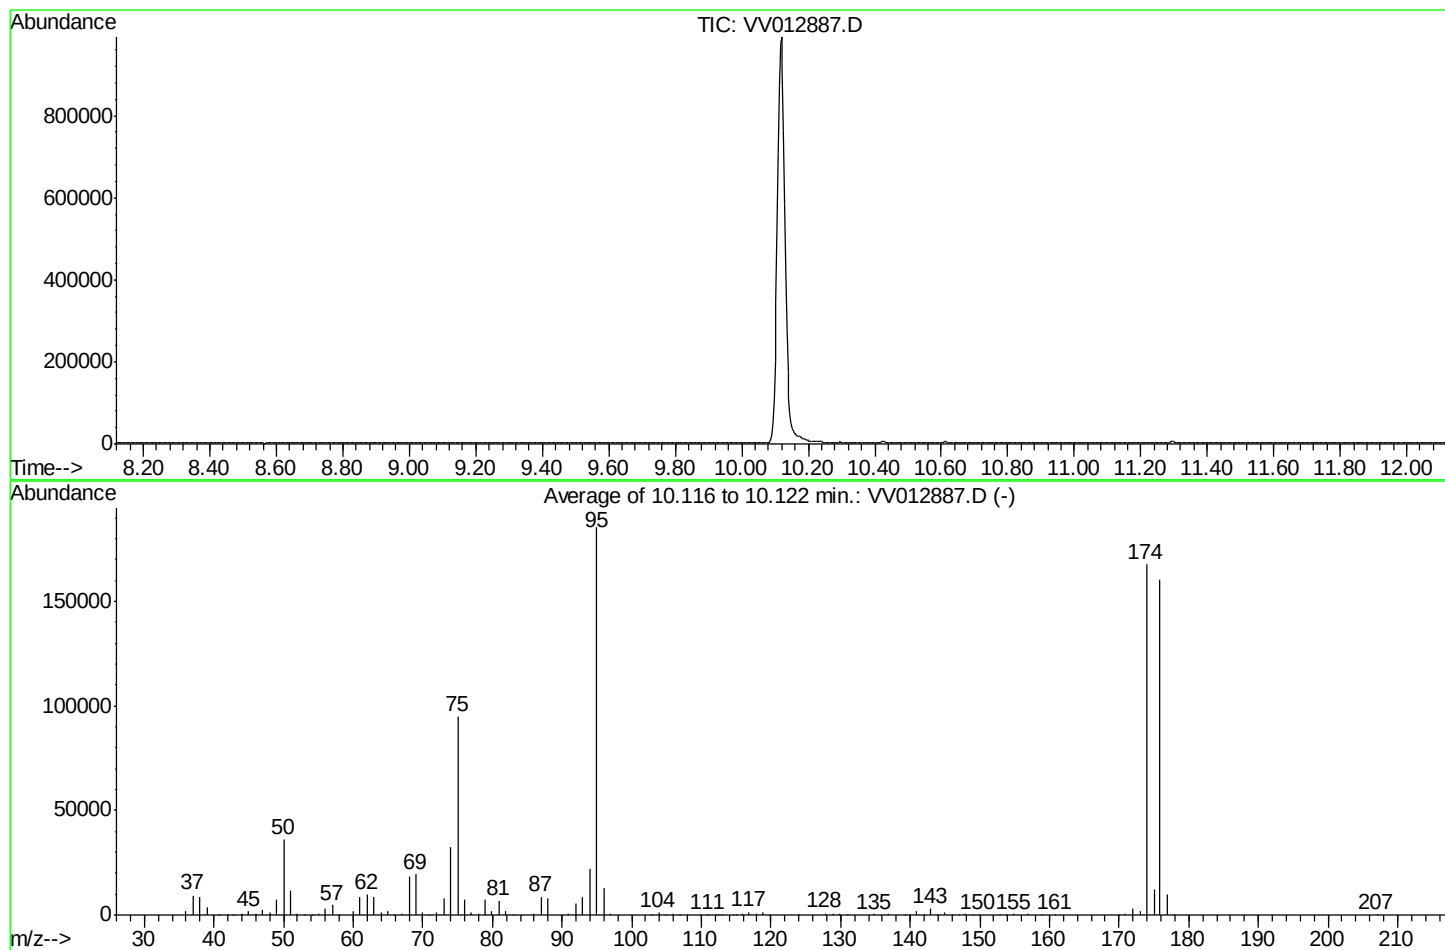

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	35936	PASS
75	95	30	80	51.2	94874	PASS
95	95	100	100	100.0	185408	PASS
96	95	5	9	6.8	12592	PASS
173	174	0.00	2	1.2	2084	PASS
174	95	50	120	90.4	167530	PASS
175	174	5	9	7.3	12188	PASS
176	174	95	101	95.6	160149	PASS
177	176	5	9	6.2	9960	PASS

m/z	Abundance
38.20	161.0
39.90	1104.0
40.70	102.0
42.90	128.0
43.90	910.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

m/z	Abundance
36.00	1928.0
37.00	9497.0
38.00	8883.0
39.00	3644.0
39.90	1050.0
40.70	243.0
42.80	170.0
44.00	1726.0
45.00	1691.0
46.00	503.0
47.00	2778.0
48.00	1210.0
49.00	7645.0
50.00	36808.0
51.00	11774.0
52.00	655.0
53.00	327.0
54.10	132.0
55.10	706.0
56.00	3137.0
57.00	4879.0
58.00	302.0
60.00	1861.0
61.00	9009.0
62.00	9781.0
63.00	8913.0
64.00	1190.0
65.00	2081.0
66.00	233.0
67.00	499.0
68.00	19104.0
69.00	19744.0
70.00	1329.0
70.90	118.0
71.90	1220.0
73.00	8535.0
74.00	33280.0
75.00	97888.0
76.00	8093.0
77.00	1474.0
78.00	767.0
78.90	7362.0
79.90	1886.0
80.90	7447.0
81.90	1634.0
82.90	238.0
86.00	491.0
86.90	8879.0
87.90	8700.0
90.90	969.0
92.00	5575.0
93.00	8624.0
94.00	22832.0
95.00	189248.0
96.00	12674.0
97.00	439.0
103.90	996.0
104.90	254.0
106.00	776.0
107.00	239.0
107.90	109.0
109.90	131.0
111.00	175.0
112.00	125.0
112.90	201.0
114.60	143.0
115.00	112.0
115.80	688.0
116.90	1525.0
117.80	735.0
118.90	1246.0
127.80	752.0
128.80	510.0
129.80	711.0
131.00	322.0
134.90	402.0
136.90	386.0
139.90	173.0
140.90	1821.0
141.90	261.0
142.90	3096.0
143.80	276.0
144.90	1188.0
146.00	293.0
146.90	190.0
147.80	517.0
148.90	137.0
149.90	234.0
152.80	151.0
153.70	106.0
154.90	473.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

156.80	386.0
158.90	186.0
160.90	263.0
170.00	116.0
170.90	477.0
172.00	2859.0
173.00	2172.0
173.90	166720.0
175.00	12366.0
175.90	159424.0
177.00	10103.0
177.90	284.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

m/z	Abundance
36.00	1982.0
37.00	9469.0
38.00	8833.0
39.00	3674.0
39.90	1030.0
40.80	213.0
42.80	201.0
44.00	1692.0
45.00	1672.0
45.90	509.0
47.00	2827.0
48.00	1363.0
49.00	7868.0
50.00	37232.0
51.00	11715.0
52.00	654.0
53.00	303.0
54.00	149.0
55.10	643.0
56.00	2901.0
57.00	5034.0
58.00	333.0
60.00	1882.0
61.00	8833.0
62.00	9969.0
63.00	8707.0
64.00	1279.0
65.00	2086.0
65.90	204.0
67.00	542.0
68.00	18744.0
69.00	20168.0
70.00	1310.0
70.90	155.0
71.90	1216.0
73.00	8384.0
74.00	33224.0
75.00	97840.0
76.00	7790.0
77.00	1365.0
77.90	776.0
78.90	7292.0
79.90	1954.0
80.90	7298.0
81.90	1693.0
82.90	241.0
86.00	511.0
87.00	9181.0
87.90	8530.0
90.90	842.0
92.00	5578.0
93.00	8565.0
94.00	22752.0
95.00	191744.0
96.00	13161.0
97.00	460.0
102.90	111.0
103.90	1068.0
104.80	269.0
106.00	836.0
106.90	199.0
109.90	122.0
111.00	159.0
111.90	155.0
112.90	222.0
114.60	137.0
115.80	733.0
116.90	1527.0
117.90	850.0
118.90	1238.0
119.80	101.0
124.00	148.0
127.80	685.0
128.80	510.0
129.80	654.0
130.90	269.0
134.90	399.0
136.90	327.0
139.90	137.0
140.90	1996.0
141.90	274.0
143.00	3150.0
143.90	273.0
144.90	1043.0
145.90	325.0
147.00	180.0
147.80	515.0
148.90	139.0
149.80	239.0
152.70	173.0
153.80	138.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

154.90	494.0
156.80	371.0
158.90	198.0
160.80	236.0
170.80	414.0
171.90	2993.0
173.00	2129.0
173.90	173120.0
175.00	12554.0
175.90	165248.0
176.90	10257.0
177.90	285.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

m/z	Abundance
36.00	1836.0
37.00	8691.0
38.00	7890.0
39.10	3378.0
39.90	1106.0
40.80	204.0
41.90	102.0
42.80	217.0
44.00	1584.0
44.90	1425.0
46.00	487.0
47.00	2627.0
48.00	1320.0
49.00	7318.0
50.00	33768.0
51.00	10742.0
52.00	495.0
52.90	256.0
54.00	160.0
55.00	546.0
56.00	2459.0
57.00	4614.0
58.00	331.0
59.90	1700.0
61.00	7992.0
62.00	8986.0
63.00	7727.0
64.00	1222.0
65.00	2044.0
65.90	195.0
67.00	479.0
68.00	16840.0
69.00	18584.0
70.00	1217.0
70.80	167.0
71.90	1108.0
73.00	7684.0
74.00	30248.0
75.00	88896.0
76.10	7053.0
77.00	1048.0
77.90	713.0
78.90	6676.0
79.90	1769.0
80.90	6319.0
81.90	1569.0
83.00	243.0
85.90	435.0
87.00	8317.0
88.00	7470.0
90.80	594.0
92.00	5283.0
93.00	7866.0
94.00	20656.0
95.00	175232.0
96.00	11943.0
97.00	391.0
102.80	154.0
103.90	1057.0
104.80	262.0
105.90	846.0
106.80	185.0
111.00	123.0
111.90	143.0
112.40	111.0
112.90	209.0
114.70	146.0
115.90	642.0
116.80	1309.0
117.90	812.0
118.90	1123.0
119.80	113.0
123.90	168.0
127.80	534.0
128.90	454.0
129.80	528.0
130.80	227.0
134.90	315.0
136.80	280.0
139.20	105.0
140.00	108.0
140.90	1974.0
141.90	249.0
143.00	2806.0
143.90	226.0
144.90	881.0
145.90	340.0
147.00	144.0
147.80	470.0
148.90	141.0
149.80	303.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

152.70	158.0
153.80	139.0
154.90	495.0
156.80	300.0
158.80	189.0
160.70	207.0
170.80	334.0
171.90	2802.0
173.00	1952.0
173.90	162752.0
175.00	11644.0
175.90	155776.0
176.90	9520.0
177.90	252.0
207.00	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40