
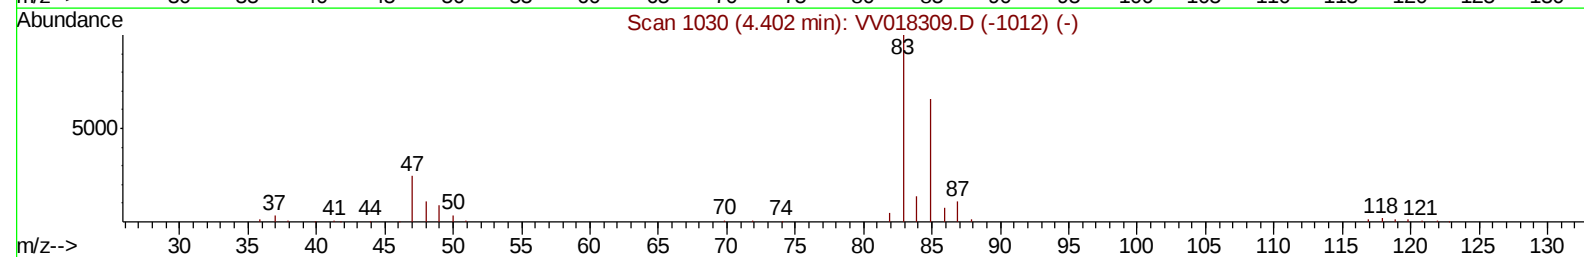
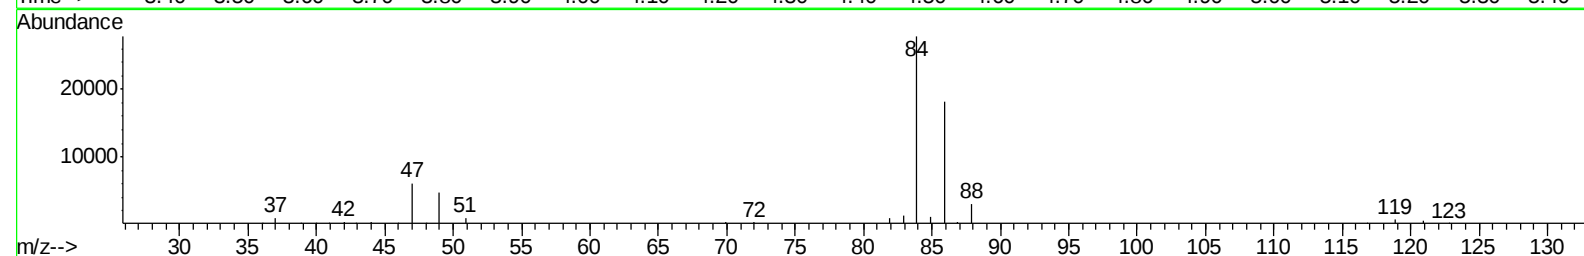


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091820\
 Data File : VV018311.D
 Acq On : 18 Sep 2020 10:59
 Operator : SY/MD
 Sample : L4043-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Sep 19 01:58:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 19 01:35:10 2020
 Response via : Initial Calibration

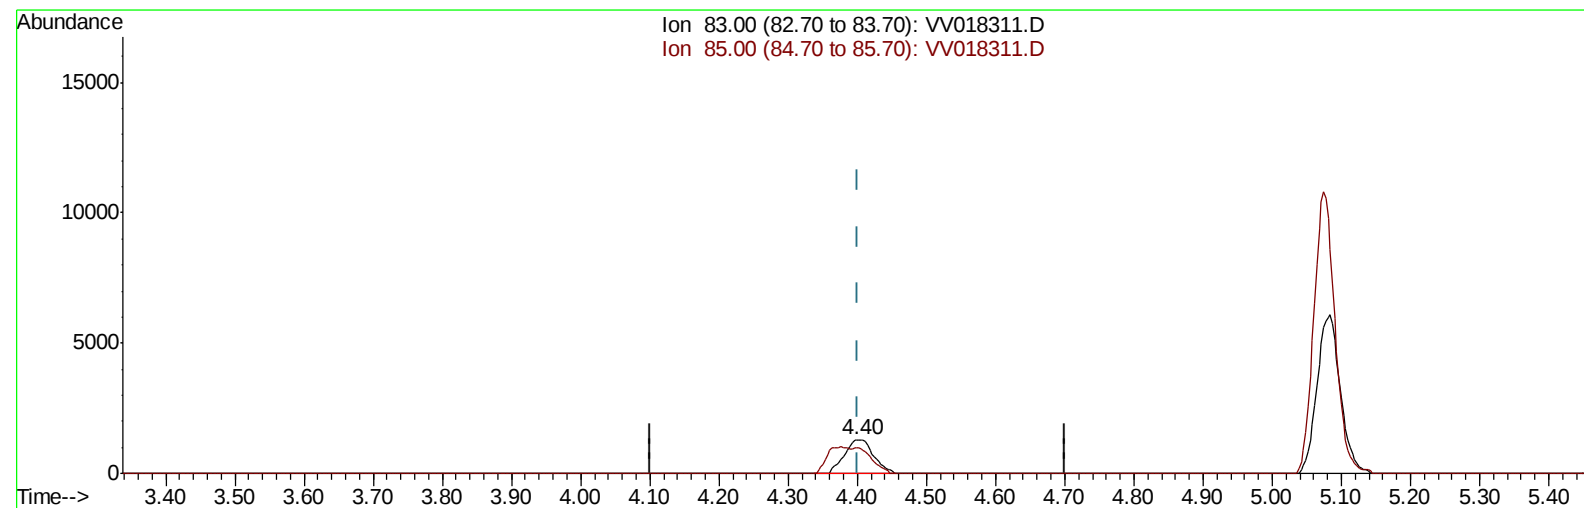

TIC: VV018311.D

(25) Chloroform (T)

4.399min (-0.003) 1.02ug/L m

response 3742

Ion	Exp%	Act%
83.00	100	100
85.00	64.30	77.76
0.00	0.00	0.00
0.00	0.00	0.00