

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091820\
 Data File : VV018325.D
 Acq On : 18 Sep 2020 16:14
 Operator : SY/MD
 Sample : L4065-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0TR1

Quant Time: Sep 19 04:00:10 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 19 01:35:10 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	269823	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	269535	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	130271	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	98019	44.58	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.16%
7) Chloroethane-d5	1.58	69	81856	45.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.98%
11) 1,1-Dichloroethene-d2	2.12	63	141501	35.08	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.16%
21) 2-Butanone-d5	3.92	46	123603	91.83	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.83%
24) Chloroform-d	4.38	84	168352	44.13	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.26%
26) 1,2-Dichloroethane-d4	5.06	65	113008	46.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.42%
32) Benzene-d6	5.08	84	346020	44.84	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.68%
36) 1,2-Dichloropropane-d6	6.09	67	111016	45.28	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.56%
41) Toluene-d8	7.34	98	303551	43.17	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.34%
43) trans-1,3-Dichloropropene-	7.64	79	52258	41.95	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.90%
47) 2-Hexanone-d5	8.11	63	80400	86.57	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	86.57%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	132062	42.92	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.84%
64) 1,2-Dichlorobenzene-d4	11.65	152	127902	47.81	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.62%


Target Compounds					Ovalue
13) Acetone	2.21	43	7857	7.290 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091820\
Data File : VV018325.D
Acq On : 18 Sep 2020 16:14
Operator : SY/MD
Sample : L4065-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0TR1

Quant Time: Sep 19 04:00:10 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 19 01:35:10 2020
Response via : Initial Calibration

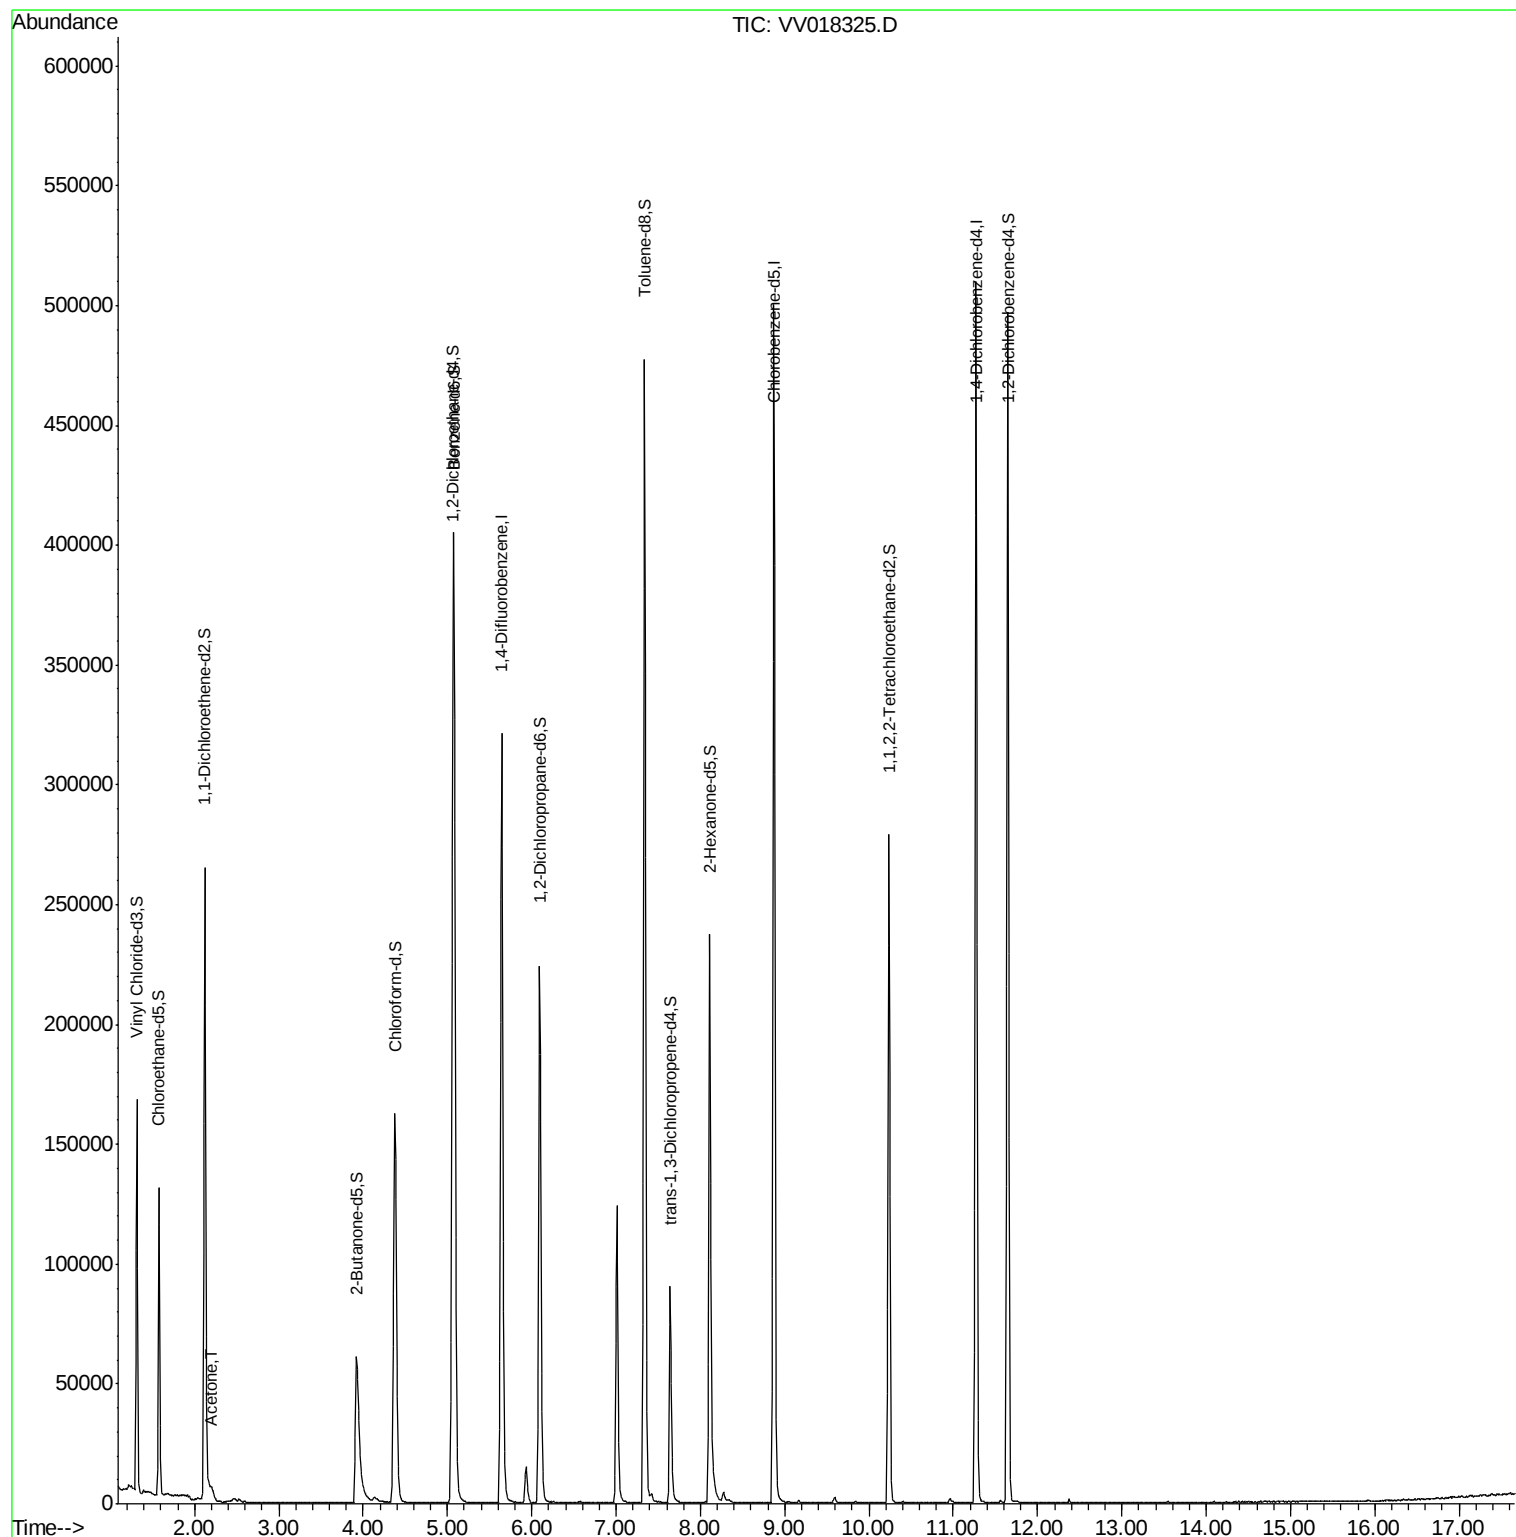

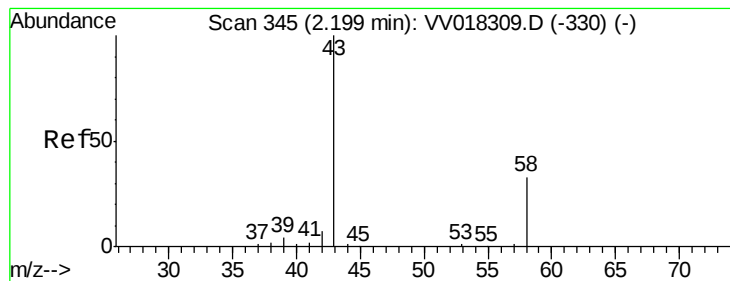

#13
 Acetone
 Concen: 7.290 ug/L
 RT: 2.21 min Scan# 348
 Delta R.T. 0.01 min
 Lab File: VV018325.D
 Acq: 18 Sep 2020 16:14

Instrument :
 MSVOA_V
 ClientSampleId :
 C0TR1

Tot Ion: 43 Resp: 7857
 Ion Ratio Lower Upper
 43 100
 58 33.4 0.0 67.4

