

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091820\
 Data File : VV018326.D
 Acq On : 18 Sep 2020 16:37
 Operator : SY/MD
 Sample : L4065-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ3

Quant Time: Sep 19 04:03:25 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 19 01:35:10 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	279056	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	281413	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	134119	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	97989	43.09	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.18%
7) Chloroethane-d5	1.58	69	80379	43.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	86.38%
11) 1,1-Dichloroethene-d2	2.12	63	140719	33.73	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.46%
21) 2-Butanone-d5	3.92	46	120000	86.21	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.21%
24) Chloroform-d	4.38	84	169271	42.90	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.80%
26) 1,2-Dichloroethane-d4	5.06	65	113371	44.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.64%
32) Benzene-d6	5.08	84	342335	42.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.98%
36) 1,2-Dichloropropane-d6	6.09	67	109011	42.59	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.18%
41) Toluene-d8	7.34	98	302853	41.25	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.50%
43) trans-1,3-Dichloropropene-	7.64	79	51646	39.70	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.40%
47) 2-Hexanone-d5	8.11	63	80081	82.59	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	82.59%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	135608	42.21	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.42%
64) 1,2-Dichlorobenzene-d4	11.65	152	126684	45.99	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.98%


Target Compounds					Ovalue
34) Trichloroethene	5.94	95	11413	5.207 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091820\
Data File : VV018326.D
Acq On : 18 Sep 2020 16:37
Operator : SY/MD
Sample : L4065-15
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ3

Quant Time: Sep 19 04:03:25 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 19 01:35:10 2020
Response via : Initial Calibration

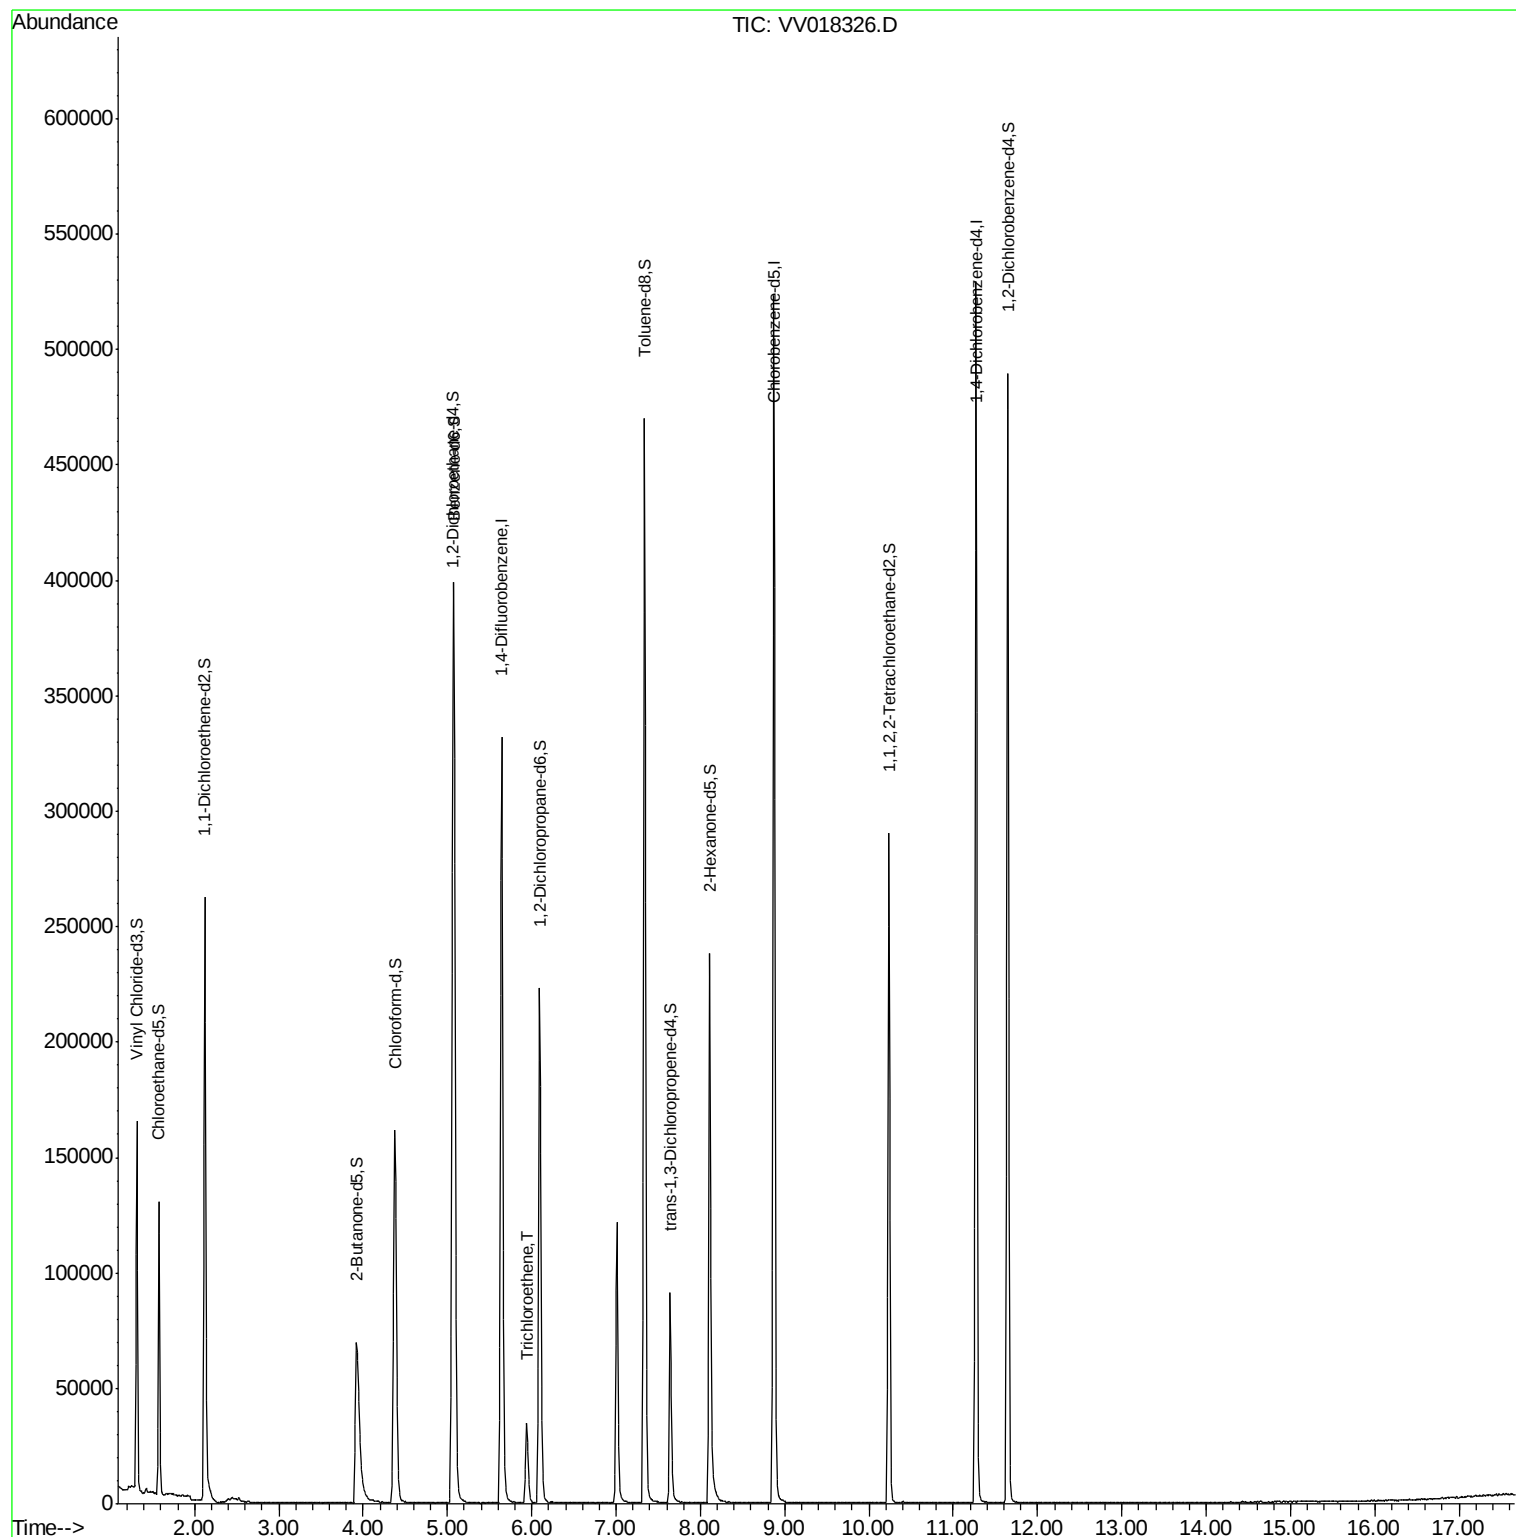

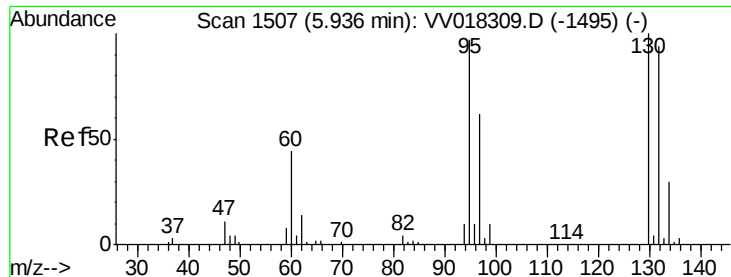

#34

Trichloroethene

Concen: 5.207 ug/L

RT: 5.94 min Scan# 1508

Delta R.T. 0.00 min

Lab File: VV018326.D

Acq: 18 Sep 2020 16:37

Instrument :

MSVOA_V

ClientSampleId :

C0AJ3

Tot Ion: 95 Resp: 11413


Ion Ratio Lower Upper

95 100

97 62.1 46.3 85.9

132 92.4 68.1 126.5

130 94.6 71.5 132.9

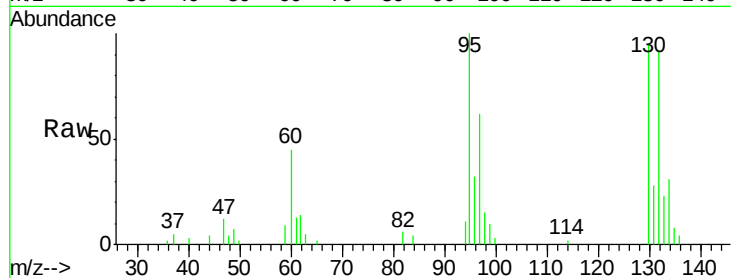

Abundance Ion 95.00 (94.70 to 95.70): VV0

Ion 97.00 (96.70 to 97.70): VV0

Ion 132.00 (131.70 to 132.70): V

Ion 130.00 (129.70 to 130.70): V

