

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091820\
 Data File : VV018353.D
 Acq On : 19 Sep 2020 03:10
 Operator : SY/MD
 Sample : L4066-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWW9

Quant Time: Sep 19 06:31:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 19 05:11:16 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	284854	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	280553	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	134351	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	92868	40.00	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.00%
7) Chloroethane-d5	1.58	69	78969	41.57	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	83.14%
11) 1,1-Dichloroethene-d2	2.12	63	135999	31.94	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.88%
21) 2-Butanone-d5	3.90	46	122125	85.95	ug/L	-0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.95%
24) Chloroform-d	4.38	84	171946	42.69	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.38%
26) 1,2-Dichloroethane-d4	5.06	65	115277	44.65	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.30%
32) Benzene-d6	5.08	84	345648	43.04	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.08%
36) 1,2-Dichloropropane-d6	6.09	67	110051	43.12	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.24%
41) Toluene-d8	7.34	98	305577	41.75	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.50%
43) trans-1,3-Dichloropropene-	7.64	79	50178	38.69	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.38%
47) 2-Hexanone-d5	8.11	63	80070	82.83	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	82.83%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	138771	43.33	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.66%
64) 1,2-Dichlorobenzene-d4	11.65	152	127668	46.27	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.54%


Target Compounds					Ovalue
13) Acetone	2.18	43	4645	4.082 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091820\
Data File : VV018353.D
Acq On : 19 Sep 2020 03:10
Operator : SY/MD
Sample : L4066-20
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWW9

Quant Time: Sep 19 06:31:53 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 19 05:11:16 2020
Response via : Initial Calibration

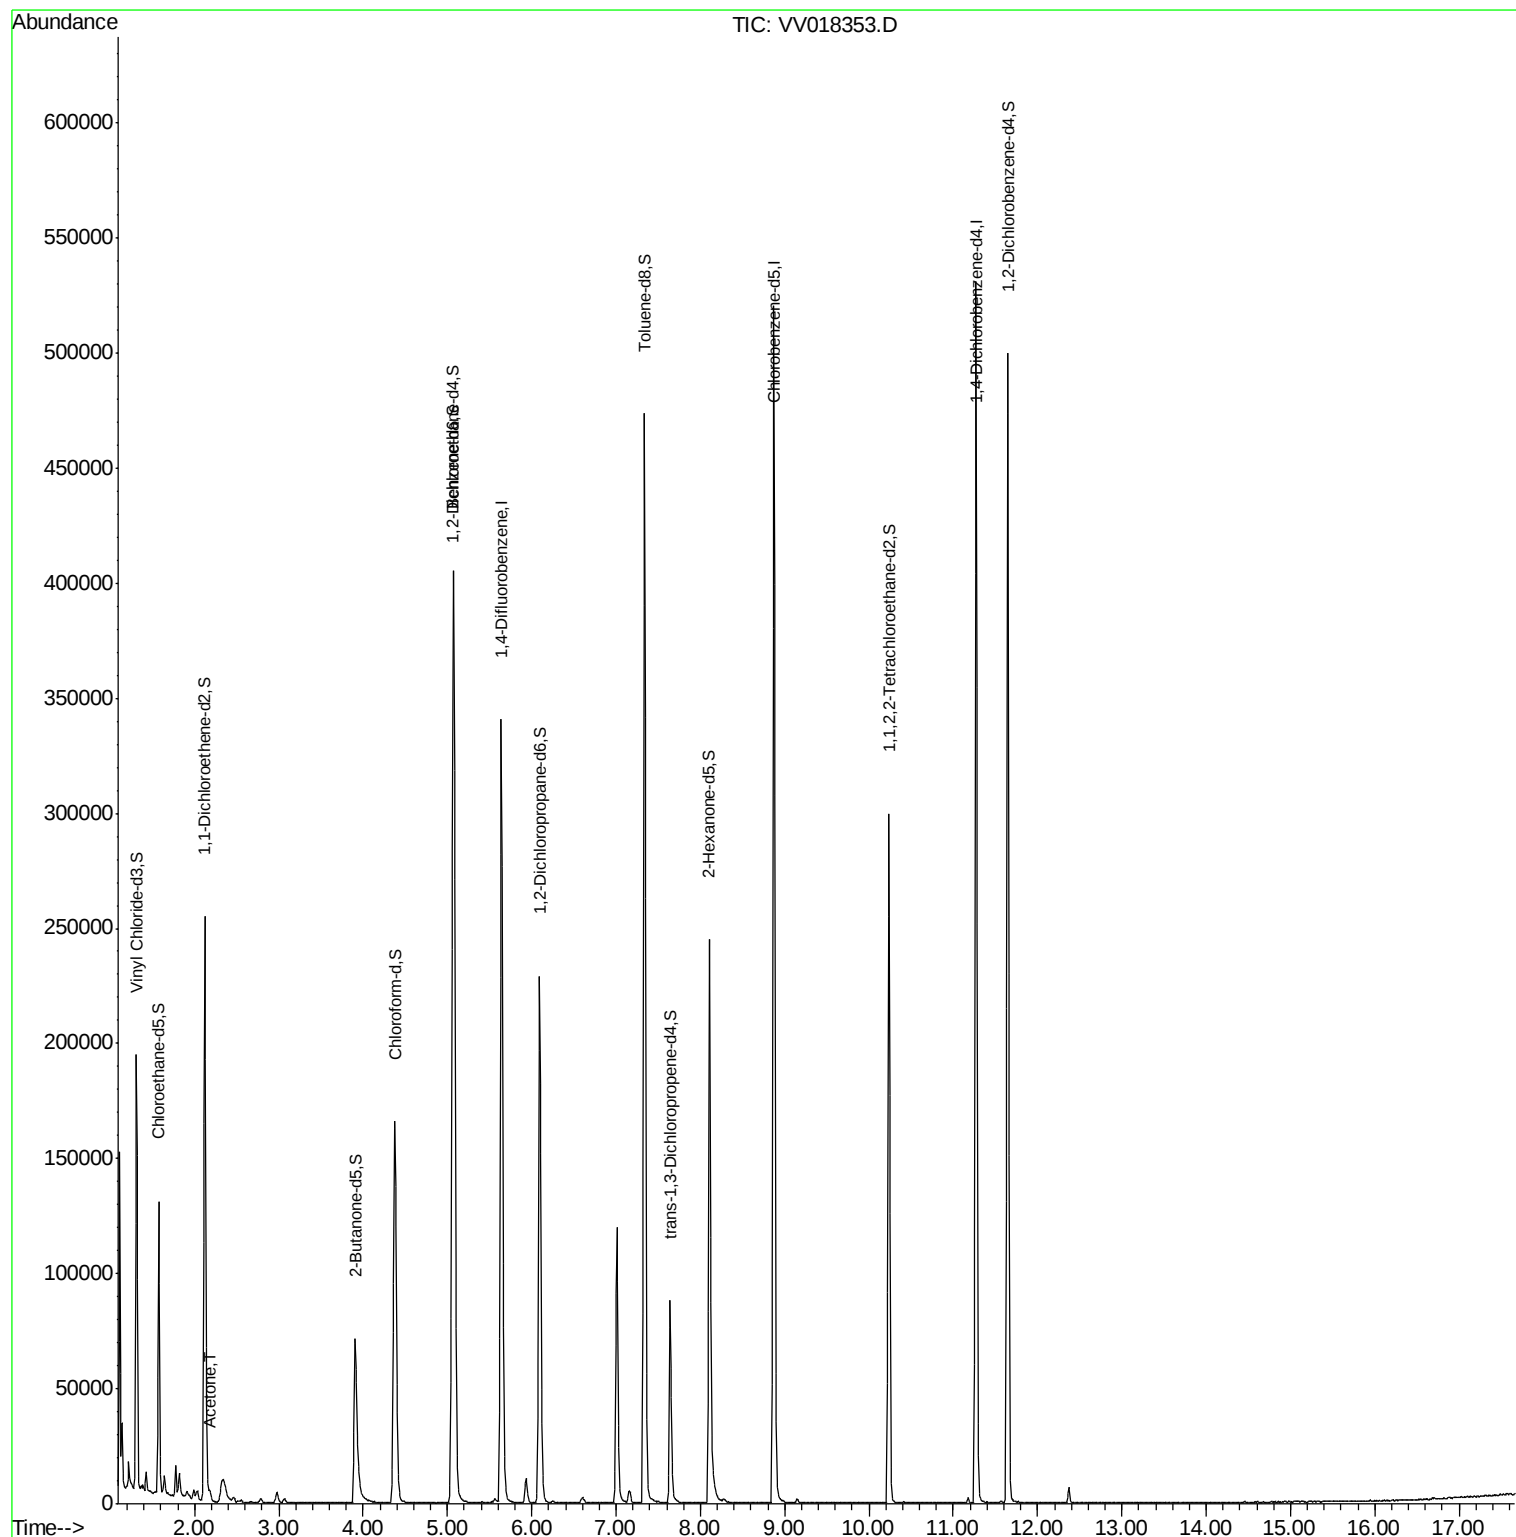

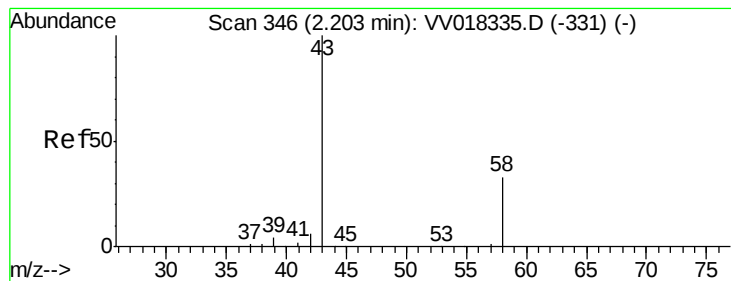

#13
 Acetone
 Concen: 4.082 ug/L
 RT: 2.18 min Scan# 340
 Delta R.T. -0.02 min
 Lab File: VV018353.D
 Acq: 19 Sep 2020 03:10

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWW9

Tot Ion: 43 Resp: 4645
 Ion Ratio Lower Upper
 43 100
 58 33.0 0.0 67.4

