

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091820\
 Data File : VV018318.D
 Acq On : 18 Sep 2020 13:36
 Operator : SY/MD
 Sample : L4065-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	87	rVB	159859	164083	16.26%	2.162%
2	1.579	144	152	165	rBB	127702	142457	14.12%	1.877%
3	2.122	310	321	358	rVB	260700	401821	39.82%	5.296%
4	2.393	403	405	407	rBV2	416	200	0.02%	0.003%
5	2.531	442	448	456	rVB4	958	1538	0.15%	0.020%
6	2.663	487	489	491	rBV	197	77	0.01%	0.001%
7	2.772	520	523	525	rBV	74	47	0.00%	0.001%
8	2.833	539	542	548	rBV2	147	134	0.01%	0.002%
9	2.865	549	552	554	rBV	119	70	0.01%	0.001%
10	2.926	568	571	574	rBV2	113	69	0.01%	0.001%
11	3.171	644	647	651	rVB2	129	97	0.01%	0.001%
12	3.283	679	682	685	rBV	120	77	0.01%	0.001%
13	3.357	699	705	706	rBV	110	125	0.01%	0.002%
14	3.444	729	732	736	rBV2	94	94	0.01%	0.001%
15	3.746	823	826	828	rBV2	56	34	0.00%	0.000%
16	3.804	841	844	851	rVB2	156	155	0.02%	0.002%
17	3.836	851	854	856	rBV	96	70	0.01%	0.001%
18	3.920	869	880	927	rBV	63340	199623	19.78%	2.631%
19	4.380	1006	1023	1052	rBV	160293	392267	38.88%	5.170%
20	4.579	1081	1085	1089	rVB3	282	192	0.02%	0.003%
21	4.663	1108	1111	1112	rBV	139	83	0.01%	0.001%
22	4.669	1112	1113	1115	rVV	201	63	0.01%	0.001%
23	4.682	1115	1117	1121	rVB2	189	108	0.01%	0.001%
24	4.708	1123	1125	1126	rVB	126	33	0.00%	0.000%
25	4.740	1133	1135	1138	rVB2	84	47	0.00%	0.001%
26	4.923	1190	1192	1195	rVB	124	70	0.01%	0.001%
27	4.946	1195	1199	1202	rBV2	150	137	0.01%	0.002%
28	5.074	1222	1239	1272	rBV2	396640	1009000	100.00%	13.298%
29	5.386	1333	1336	1338	rVB2	168	94	0.01%	0.001%
30	5.399	1338	1340	1342	rVB	91	41	0.00%	0.001%
31	5.421	1342	1347	1350	rBV2	120	129	0.01%	0.002%
32	5.537	1380	1383	1387	rBV	134	110	0.01%	0.001%
33	5.592	1398	1400	1403	rVB2	133	58	0.01%	0.001%
34	5.643	1403	1416	1445	rBV	295324	581471	57.63%	7.663%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091820\
 Data File : VV018318.D
 Acq On : 18 Sep 2020 13:36
 Operator : SY/MD
 Sample : L4065-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

35	5.933	1498	1506	1522	rVB2	6022	12189	1.21%	0.161%
36	6.045	1539	1541	1543	rBV	89	51	0.01%	0.001%
37	6.097	1543	1557	1579	rBV	222586	446414	44.24%	5.883%
38	6.238	1599	1601	1607	rVB3	372	380	0.04%	0.005%
39	6.267	1607	1610	1615	rVB	132	102	0.01%	0.001%
40	6.309	1620	1623	1624	rBV	98	61	0.01%	0.001%
41	6.315	1624	1625	1627	rVB	111	23	0.00%	0.000%
42	6.357	1635	1638	1643	rBV2	77	82	0.01%	0.001%
43	6.418	1654	1657	1659	rBV	98	67	0.01%	0.001%
44	6.614	1715	1718	1720	rBV	84	58	0.01%	0.001%
45	6.730	1751	1754	1757	rBV2	86	59	0.01%	0.001%
46	6.810	1776	1779	1783	rBV	102	89	0.01%	0.001%
47	6.846	1788	1790	1792	rBV	97	54	0.01%	0.001%
48	7.010	1830	1841	1867	rBV	119447	216729	21.48%	2.856%
49	7.196	1898	1899	1900	rBV	126	32	0.00%	0.000%
50	7.228	1907	1909	1912	rVB2	190	111	0.01%	0.001%
51	7.338	1931	1943	1970	rBV	462438	798787	79.17%	10.527%
52	7.572	2013	2016	2021	rVB2	195	124	0.01%	0.002%
53	7.643	2028	2038	2064	rBV	88231	152221	15.09%	2.006%
54	7.836	2097	2098	2099	rBV	111	31	0.00%	0.000%
55	7.884	2111	2113	2118	rVB2	102	67	0.01%	0.001%
56	7.961	2130	2137	2146	rVB3	422	695	0.07%	0.009%
57	8.032	2157	2159	2160	rBV	87	41	0.00%	0.001%
58	8.109	2173	2183	2219	rBV	242968	426906	42.31%	5.626%
59	8.450	2287	2289	2292	rVB3	196	111	0.01%	0.001%
60	8.466	2292	2294	2296	rBV	137	74	0.01%	0.001%
61	8.479	2296	2298	2300	rVV	165	69	0.01%	0.001%
62	8.524	2309	2312	2315	rVB2	194	126	0.01%	0.002%
63	8.656	2350	2353	2355	rBV	138	100	0.01%	0.001%
64	8.804	2396	2399	2401	rBV2	141	98	0.01%	0.001%
65	8.875	2408	2421	2460	rBV	458418	739334	73.27%	9.744%
66	9.222	2526	2529	2530	rBV	120	72	0.01%	0.001%
67	9.305	2552	2555	2558	rBV	154	117	0.01%	0.002%
68	9.370	2572	2575	2577	rBV	106	71	0.01%	0.001%
69	9.486	2608	2611	2613	rBV	103	57	0.01%	0.001%
70	9.556	2630	2633	2635	rBV2	97	52	0.01%	0.001%
71	9.952	2752	2756	2759	rBV2	124	127	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091820\
 Data File : VV018318.D
 Acq On : 18 Sep 2020 13:36
 Operator : SY/MD
 Sample : L4065-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

72	10.141	2813	2815	2816	rBV	105	51	0.01%	0.001%
73	10.238	2833	2845	2874	rBV	287440	449001	44.50%	5.917%
74	10.363	2881	2884	2886	rBV	135	97	0.01%	0.001%
75	10.376	2886	2888	2890	rVV	223	110	0.01%	0.001%
76	10.405	2890	2897	2904	rVB2	651	832	0.08%	0.011%
77	10.576	2947	2950	2953	rBV2	135	104	0.01%	0.001%
78	11.270	3154	3166	3189	rBV	458991	694169	68.80%	9.148%
79	11.395	3203	3205	3210	rVB3	507	371	0.04%	0.005%
80	11.415	3210	3211	3212	rBV3	100	25	0.00%	0.000%
81	11.431	3212	3216	3218	rBV	232	180	0.02%	0.002%
82	11.495	3234	3236	3238	rVB2	182	55	0.01%	0.001%
83	11.563	3254	3257	3260	rBV	168	73	0.01%	0.001%
84	11.604	3268	3270	3271	rBV	127	53	0.01%	0.001%
85	11.646	3271	3283	3304	rVV	483569	750724	74.40%	9.894%
86	11.801	3329	3331	3332	rBV	115	43	0.00%	0.001%
87	11.813	3332	3335	3336	rBV	134	59	0.01%	0.001%
88	11.829	3336	3340	3341	rVV	121	76	0.01%	0.001%
89	11.891	3358	3359	3362	rVB	138	39	0.00%	0.001%
90	11.929	3364	3371	3374	rBV2	201	265	0.03%	0.003%
91	11.971	3383	3384	3387	rVB2	282	95	0.01%	0.001%
92	11.990	3387	3390	3393	rBV	152	124	0.01%	0.002%
93	12.315	3483	3491	3494	rBV3	360	442	0.04%	0.006%
94	13.624	3896	3898	3900	rBV	150	44	0.00%	0.001%
95	13.707	3922	3924	3926	rBV	137	55	0.01%	0.001%
96	13.743	3932	3935	3939	rVB	305	175	0.02%	0.002%
97	14.492	4164	4168	4170	rBV	212	175	0.02%	0.002%


Sum of corrected areas: 7587892

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091820\
Data File : VV018318.D
Acq On : 18 Sep 2020 13:36
Operator : SY/MD
Sample : L4065-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

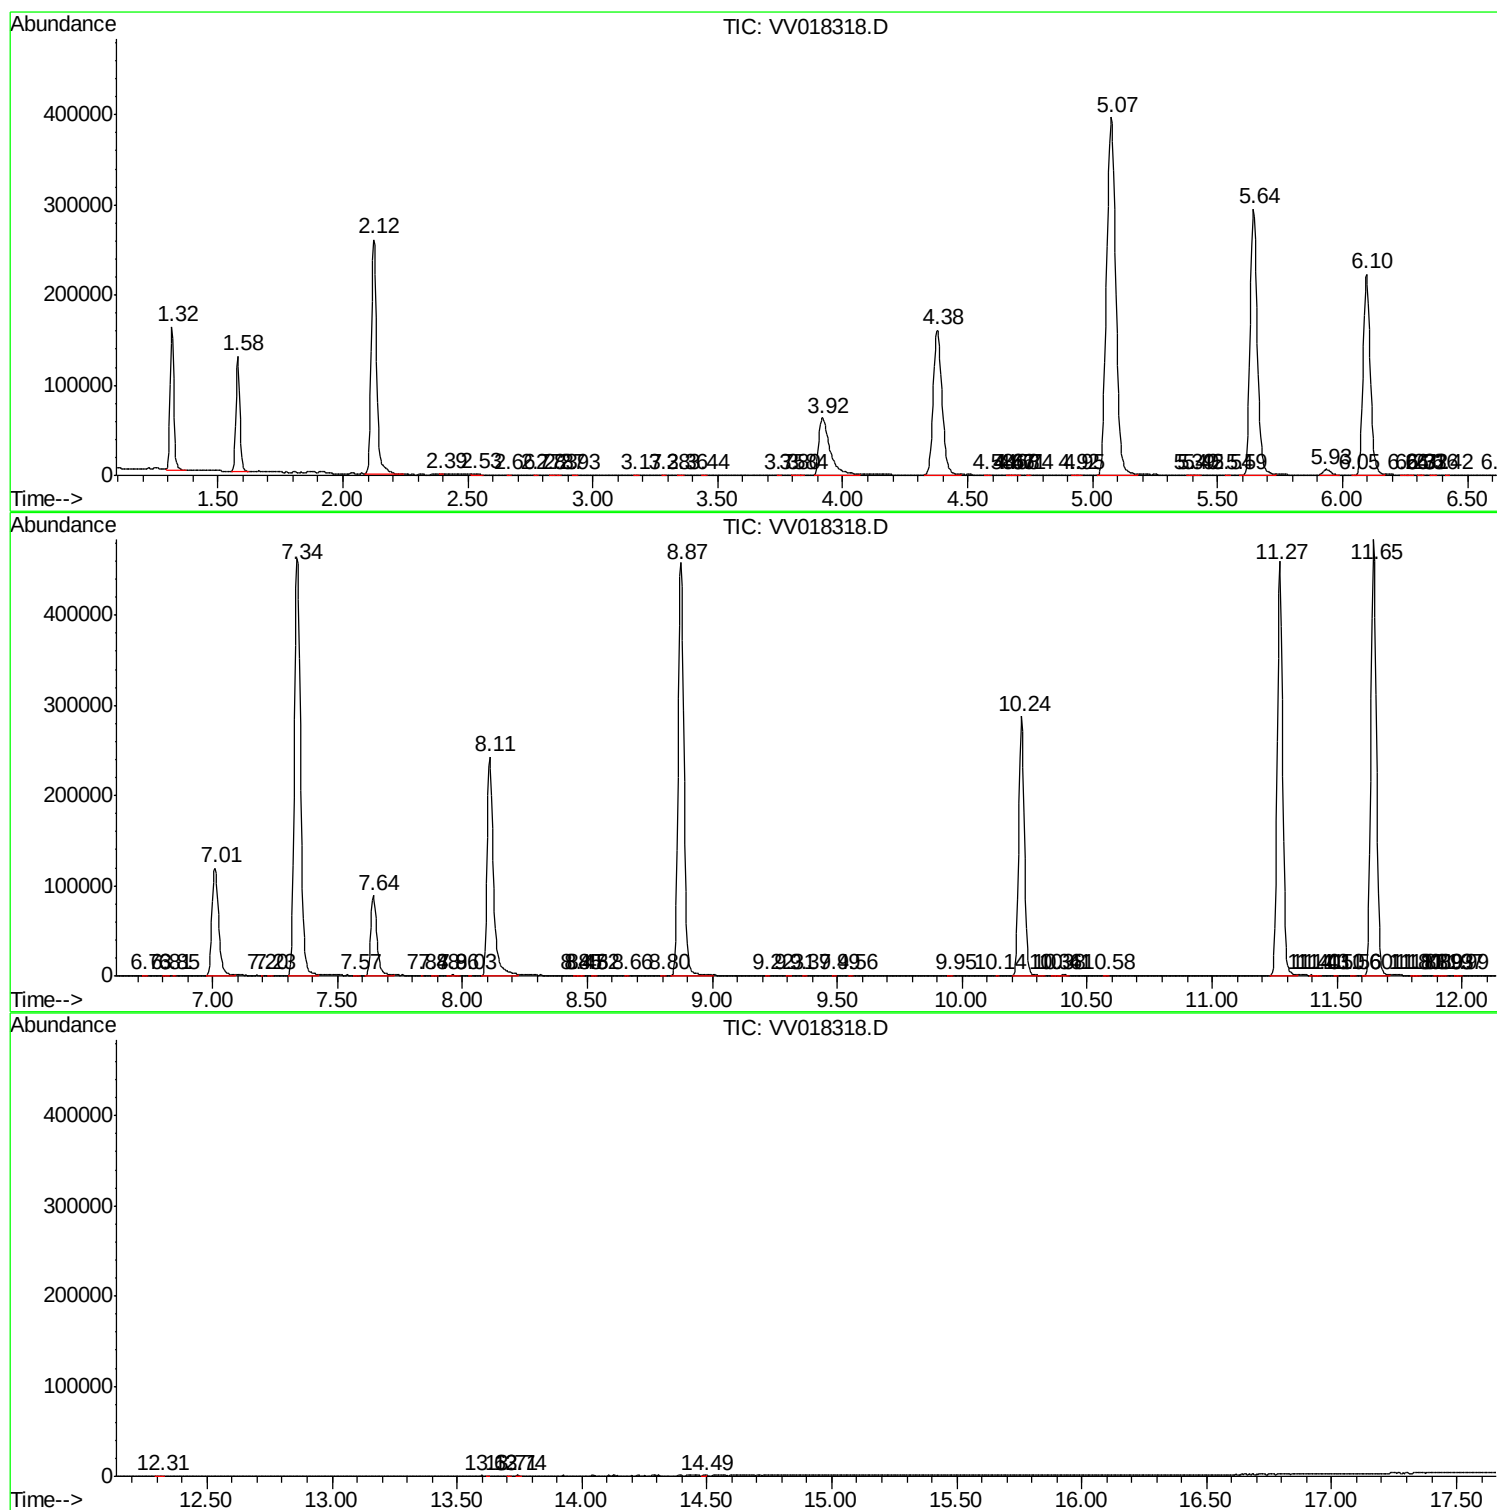

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV091820\
Data File : VV018318.D
Acq On : 18 Sep 2020 13:36
Operator : SY/MD
Sample : L4065-05
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AH1

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV091820\
Data File : VV018318.D
Acq On : 18 Sep 2020 13:36
Operator : SY/MD
Sample : L4065-05
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AH1

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc