

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091820\
 Data File : VV018333.D
 Acq On : 18 Sep 2020 19:15
 Operator : SY/MD
 Sample : L4066-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWT6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	84	rVB	160861	163275	15.80%	2.037%
2	1.579	144	152	166	rBV	127751	144819	14.01%	1.806%
3	2.123	310	321	362	rVB	264662	411267	39.80%	5.130%
4	2.322	375	383	385	rBV3	550	674	0.07%	0.008%
5	2.586	462	465	468	rBV2	267	146	0.01%	0.002%
6	2.868	549	553	558	rVB	194	157	0.02%	0.002%
7	2.894	558	561	568	rVV2	144	171	0.02%	0.002%
8	2.981	583	588	594	rBV2	420	616	0.06%	0.008%
9	3.200	648	656	661	rBV2	105	172	0.02%	0.002%
10	3.331	689	697	700	rBV	150	155	0.01%	0.002%
11	3.415	717	723	728	rBV	115	131	0.01%	0.002%
12	3.473	738	741	746	rVB2	125	125	0.01%	0.002%
13	3.505	746	751	754	rBV2	157	127	0.01%	0.002%
14	3.740	818	824	826	rBV2	136	144	0.01%	0.002%
15	3.756	826	829	832	rBV3	337	262	0.03%	0.003%
16	3.772	832	834	838	rBV2	156	120	0.01%	0.001%
17	3.814	844	847	851	rVB3	216	147	0.01%	0.002%
18	3.917	867	879	910	rBV2	63711	191733	18.55%	2.392%
19	4.376	1004	1022	1053	rBV	164388	403460	39.04%	5.032%
20	4.524	1066	1068	1076	rVB3	359	278	0.03%	0.003%
21	4.563	1076	1080	1082	rBV2	336	257	0.02%	0.003%
22	4.923	1188	1192	1198	rBV2	124	165	0.02%	0.002%
23	4.981	1204	1210	1214	rBV2	130	149	0.01%	0.002%
24	5.074	1220	1239	1267	rBV2	408076	1033414	100.00%	12.890%
25	5.232	1286	1288	1296	rVB3	408	366	0.04%	0.005%
26	5.319	1310	1315	1318	rBV3	170	140	0.01%	0.002%
27	5.376	1330	1333	1336	rVB2	281	171	0.02%	0.002%
28	5.421	1344	1347	1351	rBV2	195	167	0.02%	0.002%
29	5.515	1372	1376	1380	rBV2	270	231	0.02%	0.003%
30	5.544	1380	1385	1389	rVV2	149	123	0.01%	0.002%
31	5.643	1403	1416	1445	rBV	329442	650602	62.96%	8.115%
32	5.936	1495	1507	1526	rVB6	14814	33758	3.27%	0.421%
33	6.093	1543	1556	1585	rBV	230085	462142	44.72%	5.764%
34	6.222	1593	1596	1597	rBV3	344	163	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091820\
 Data File : VV018333.D
 Acq On : 18 Sep 2020 19:15
 Operator : SY/MD
 Sample : L4066-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWT6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

35	6.241	1599	1602	1608	rVB3	452	432	0.04%	0.005%
36	6.341	1628	1633	1637	rVV3	536	698	0.07%	0.009%
37	6.357	1637	1638	1642	rVV3	436	209	0.02%	0.003%
38	6.373	1642	1643	1648	rVV	277	132	0.01%	0.002%
39	6.454	1664	1668	1672	rBV	124	123	0.01%	0.002%
40	6.736	1749	1756	1759	rBV2	104	114	0.01%	0.001%
41	6.891	1801	1804	1809	rBV	101	117	0.01%	0.001%
42	7.010	1829	1841	1870	rBV	122228	222828	21.56%	2.779%
43	7.154	1881	1886	1890	rBV4	417	439	0.04%	0.005%
44	7.241	1904	1913	1915	rVV2	173	170	0.02%	0.002%
45	7.338	1931	1943	1967	rBV	476376	815848	78.95%	10.176%
46	7.643	2028	2038	2058	rBV	89706	155501	15.05%	1.940%
47	7.814	2088	2091	2096	rBV3	226	168	0.02%	0.002%
48	7.958	2129	2136	2137	rBV2	379	401	0.04%	0.005%
49	8.109	2172	2183	2216	rBV	242156	434154	42.01%	5.415%
50	8.273	2226	2234	2252	rVB5	3209	6246	0.60%	0.078%
51	8.437	2283	2285	2294	rVB	314	277	0.03%	0.003%
52	8.482	2295	2299	2302	rBV2	189	132	0.01%	0.002%
53	8.592	2327	2333	2337	rBV	177	158	0.02%	0.002%
54	8.695	2361	2365	2368	rBV2	114	110	0.01%	0.001%
55	8.875	2409	2421	2451	rBV	508023	821945	79.54%	10.252%
56	9.045	2469	2474	2476	rBV2	201	156	0.02%	0.002%
57	9.167	2505	2512	2520	rBV2	372	581	0.06%	0.007%
58	9.537	2624	2627	2635	rBV2	145	218	0.02%	0.003%
59	9.572	2635	2638	2641	rBV2	205	155	0.01%	0.002%
60	9.842	2717	2722	2731	rVB4	925	1354	0.13%	0.017%
61	9.894	2736	2738	2744	rVB	197	148	0.01%	0.002%
62	10.000	2767	2771	2776	rVB2	116	123	0.01%	0.002%
63	10.238	2830	2845	2867	rBV	295762	458731	44.39%	5.722%
64	10.354	2877	2881	2888	rVV2	98	131	0.01%	0.002%
65	10.402	2889	2896	2912	rVB3	1274	1972	0.19%	0.025%
66	10.466	2912	2916	2919	rBV2	191	148	0.01%	0.002%
67	10.595	2953	2956	2958	rBV2	229	142	0.01%	0.002%
68	10.617	2961	2963	2966	rVV2	232	122	0.01%	0.002%
69	10.643	2966	2971	2978	rVB2	133	171	0.02%	0.002%
70	10.781	3011	3014	3018	rBV2	164	140	0.01%	0.002%
71	10.830	3026	3029	3033	rBV2	131	113	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091820\
 Data File : VV018333.D
 Acq On : 18 Sep 2020 19:15
 Operator : SY/MD
 Sample : L4066-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWT6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

72	11.116	3114	3118	3125	rVB2	624	667	0.06%	0.008%
73	11.174	3129	3136	3149	rVB6	2841	3887	0.38%	0.048%
74	11.270	3155	3166	3187	rBV	529052	794142	76.85%	9.906%
75	11.392	3201	3204	3210	rVV2	319	290	0.03%	0.004%
76	11.415	3210	3211	3215	rVB	233	115	0.01%	0.001%
77	11.469	3220	3228	3231	rBV2	250	291	0.03%	0.004%
78	11.563	3250	3257	3261	rBV6	913	1318	0.13%	0.016%
79	11.646	3271	3283	3299	rBV	506268	779833	75.46%	9.727%
80	11.862	3348	3350	3356	rVB	225	145	0.01%	0.002%
81	11.948	3374	3377	3382	rVB2	192	130	0.01%	0.002%
82	12.129	3426	3433	3437	rBV2	273	269	0.03%	0.003%
83	12.267	3471	3476	3481	rBV3	509	613	0.06%	0.008%
84	12.370	3501	3508	3518	rBV2	5975	8020	0.78%	0.100%
85	12.495	3541	3547	3552	rVB2	148	165	0.02%	0.002%
86	12.759	3625	3629	3633	rVB	148	117	0.01%	0.001%
87	12.920	3675	3679	3681	rBV2	169	139	0.01%	0.002%
88	13.270	3784	3788	3791	rBV2	138	153	0.01%	0.002%
89	13.347	3807	3812	3819	rBV2	203	247	0.02%	0.003%
90	13.566	3875	3880	3882	rBV	165	157	0.02%	0.002%
91	13.743	3930	3935	3940	rBV2	246	257	0.02%	0.003%
92	13.865	3970	3973	3979	rVV2	167	164	0.02%	0.002%
93	13.961	4000	4003	4008	rVB	228	169	0.02%	0.002%
94	14.035	4022	4026	4031	rVV2	222	273	0.03%	0.003%
95	14.260	4092	4096	4098	rBV2	244	183	0.02%	0.002%
96	14.399	4136	4139	4143	rVB3	256	199	0.02%	0.002%
97	14.431	4143	4149	4152	rBV3	276	305	0.03%	0.004%
98	14.450	4152	4155	4157	rBV2	177	144	0.01%	0.002%
99	14.501	4169	4171	4175	rBV3	192	188	0.02%	0.002%
100	14.694	4229	4231	4236	rBV2	188	129	0.01%	0.002%


Sum of corrected areas: 8017143

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091820\
Data File : VV018333.D
Acq On : 18 Sep 2020 19:15
Operator : SY/MD
Sample : L4066-15
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWT6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

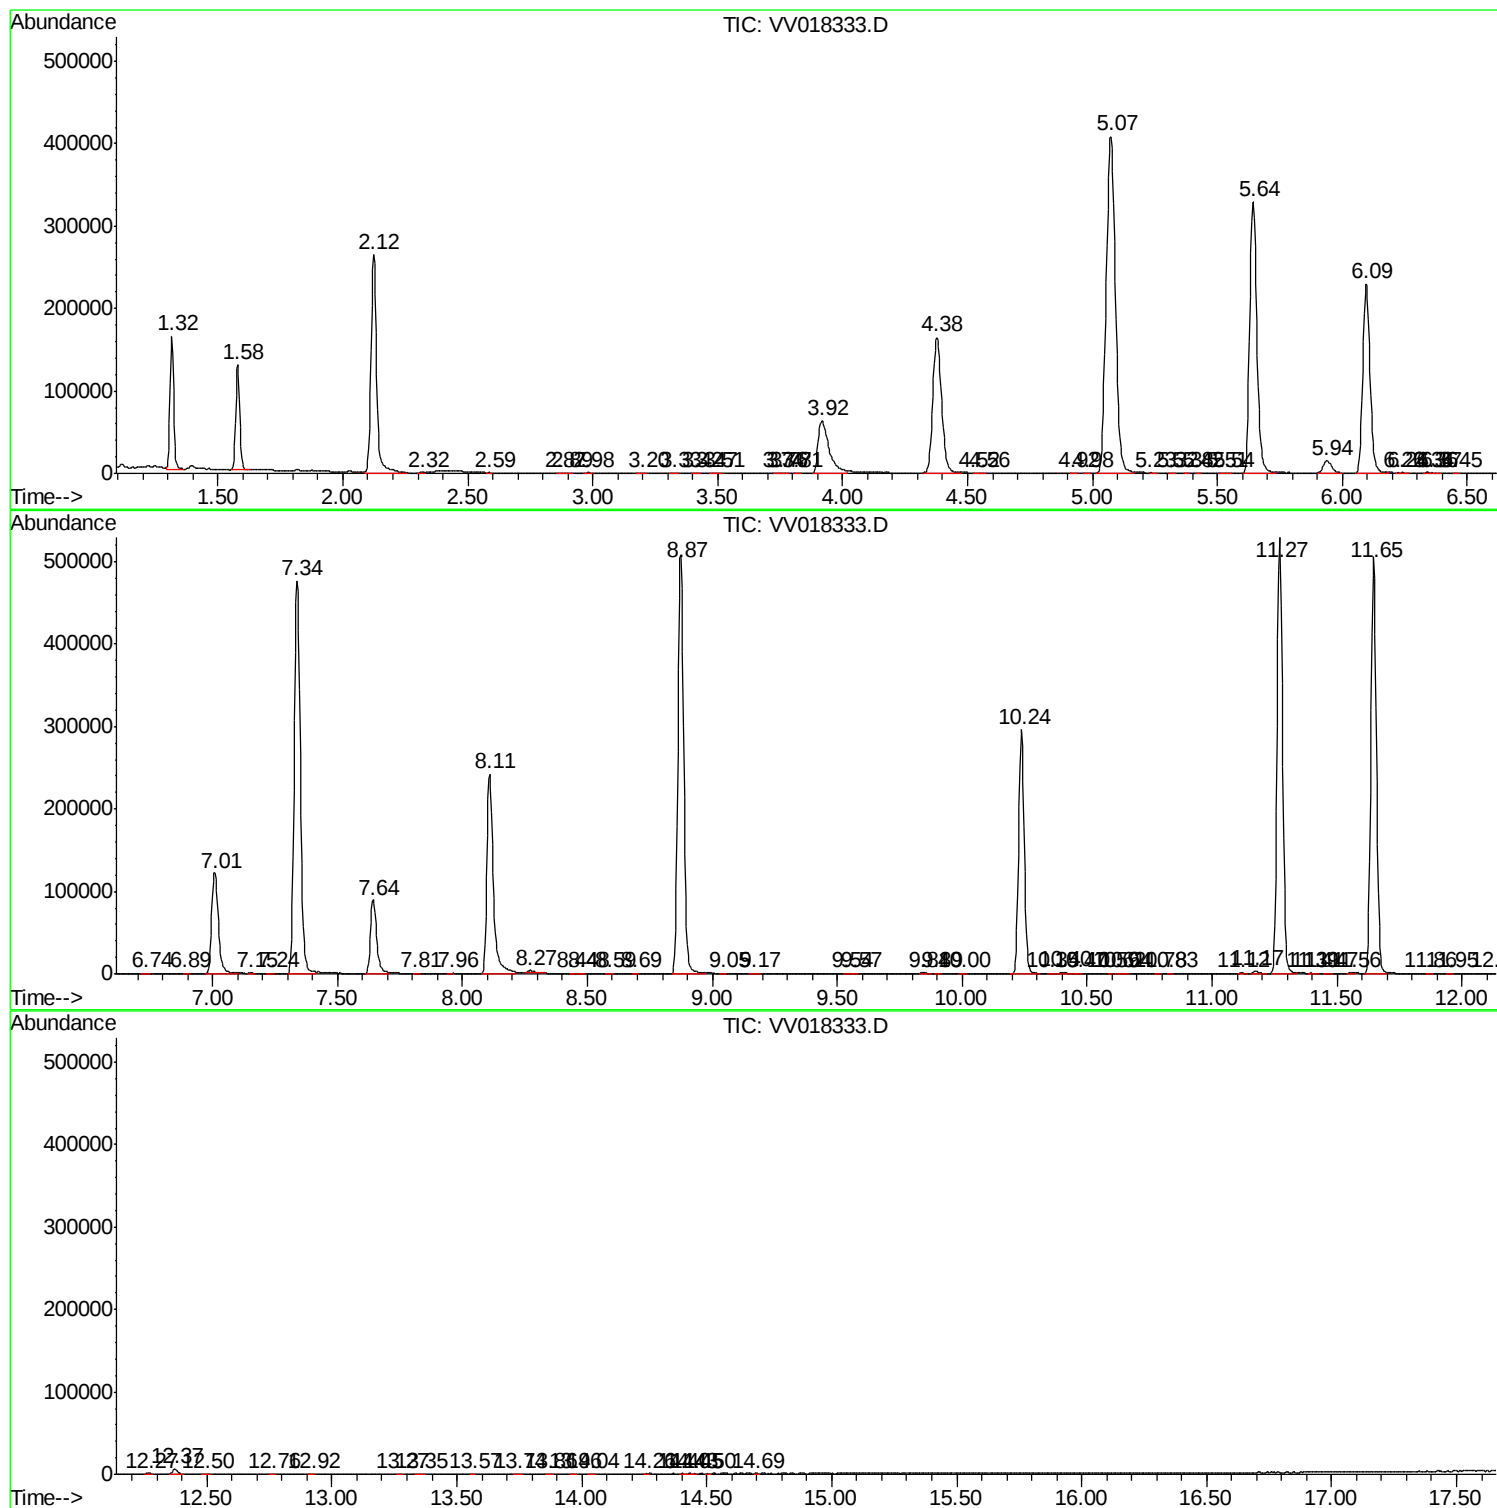

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV091820\
Data File : VV018333.D
Acq On : 18 Sep 2020 19:15
Operator : SY/MD
Sample : L4066-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWT6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091820\
Data File : VV018333.D
Acq On : 18 Sep 2020 19:15
Operator : SY/MD
Sample : L4066-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWT6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc