

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091820\
 Data File : VV018344.D
 Acq On : 18 Sep 2020 23:46
 Operator : SY/MD
 Sample : L4080-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	84	rVB	156308	155334	15.23%	1.983%
2	1.579	144	152	165	rBV	126033	143186	14.04%	1.828%
3	2.122	311	321	354	rVB	261089	399190	39.14%	5.097%
4	2.286	370	372	376	rVB	300	166	0.02%	0.002%
5	2.312	376	380	388	rBV3	524	577	0.06%	0.007%
6	2.344	388	390	391	rBV	167	64	0.01%	0.001%
7	2.383	400	402	403	rBV	205	99	0.01%	0.001%
8	2.402	404	408	410	rVV2	358	305	0.03%	0.004%
9	2.608	470	472	473	rBV2	130	56	0.01%	0.001%
10	2.785	525	527	528	rBV2	203	81	0.01%	0.001%
11	2.833	539	542	545	rBV	146	99	0.01%	0.001%
12	2.987	587	590	592	rBV	90	55	0.01%	0.001%
13	3.019	597	600	603	rBV	128	86	0.01%	0.001%
14	3.199	653	656	659	rBV	128	91	0.01%	0.001%
15	3.225	662	664	667	rVB	149	70	0.01%	0.001%
16	3.280	678	681	683	rBV2	72	51	0.00%	0.001%
17	3.315	689	692	694	rBV	224	183	0.02%	0.002%
18	3.363	705	707	711	rVB2	127	80	0.01%	0.001%
19	3.389	711	715	717	rBV	103	75	0.01%	0.001%
20	3.502	748	750	753	rVB2	91	47	0.00%	0.001%
21	3.540	759	762	763	rBV	104	57	0.01%	0.001%
22	3.682	803	806	809	rVB2	115	68	0.01%	0.001%
23	3.743	823	825	829	rBV	77	50	0.00%	0.001%
24	3.923	869	881	928	rBV	57912	193864	19.01%	2.475%
25	4.376	1006	1022	1053	rBV	162593	400660	39.28%	5.116%
26	4.531	1069	1070	1074	rVB	261	106	0.01%	0.001%
27	4.621	1095	1098	1100	rBV	78	57	0.01%	0.001%
28	4.637	1100	1103	1106	rVV	275	212	0.02%	0.003%
29	4.650	1106	1107	1110	rVV2	231	116	0.01%	0.001%
30	4.669	1110	1113	1116	rVB	228	110	0.01%	0.001%
31	4.688	1116	1119	1121	rBV2	82	49	0.00%	0.001%
32	4.740	1133	1135	1136	rBV	165	49	0.00%	0.001%
33	4.852	1167	1170	1172	rBV2	114	76	0.01%	0.001%
34	5.074	1221	1239	1266	rBV2	399977	1020023	100.00%	13.025%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091820\
 Data File : VV018344.D
 Acq On : 18 Sep 2020 23:46
 Operator : SY/MD
 Sample : L4080-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

35	5.379	1331	1334	1340	rVB2	267	229	0.02%	0.003%
36	5.408	1340	1343	1348	rBV2	271	280	0.03%	0.004%
37	5.441	1352	1353	1355	rVB2	130	48	0.00%	0.001%
38	5.489	1366	1368	1374	rVB2	107	100	0.01%	0.001%
39	5.518	1374	1377	1378	rBV2	124	67	0.01%	0.001%
40	5.534	1378	1382	1385	rBV	98	74	0.01%	0.001%
41	5.643	1403	1416	1450	rBV	327575	649167	63.64%	8.289%
42	5.932	1495	1506	1525	rVB	10839	22641	2.22%	0.289%
43	6.042	1538	1540	1543	rBV	82	64	0.01%	0.001%
44	6.093	1543	1556	1582	rBV	225580	456930	44.80%	5.834%
45	6.235	1596	1600	1601	rBV2	444	293	0.03%	0.004%
46	6.267	1608	1610	1615	rVB	230	160	0.02%	0.002%
47	6.373	1638	1643	1648	rBV2	94	125	0.01%	0.002%
48	6.469	1670	1673	1677	rBV2	109	84	0.01%	0.001%
49	6.495	1677	1681	1682	rBV2	99	71	0.01%	0.001%
50	6.855	1790	1793	1798	rBV2	81	79	0.01%	0.001%
51	6.913	1808	1811	1816	rBV	118	109	0.01%	0.001%
52	7.010	1829	1841	1870	rBV	118402	215674	21.14%	2.754%
53	7.199	1897	1900	1903	rVB	177	110	0.01%	0.001%
54	7.241	1911	1913	1917	rVB2	207	101	0.01%	0.001%
55	7.264	1917	1920	1922	rBV	90	58	0.01%	0.001%
56	7.293	1926	1929	1931	rBV	186	99	0.01%	0.001%
57	7.338	1931	1943	1967	rBV	471452	807433	79.16%	10.310%
58	7.582	2017	2019	2020	rBV	115	65	0.01%	0.001%
59	7.643	2027	2038	2064	rBV	87679	152187	14.92%	1.943%
60	7.830	2094	2096	2099	rVB2	208	116	0.01%	0.001%
61	7.952	2130	2134	2135	rBV2	200	158	0.02%	0.002%
62	8.013	2149	2153	2156	rBV2	116	95	0.01%	0.001%
63	8.109	2173	2183	2217	rBV	224925	411600	40.35%	5.256%
64	8.344	2253	2256	2258	rBV	290	186	0.02%	0.002%
65	8.411	2275	2277	2283	rVB2	251	197	0.02%	0.003%
66	8.457	2283	2291	2295	rBV2	309	500	0.05%	0.006%
67	8.675	2356	2359	2362	rBV2	98	78	0.01%	0.001%
68	8.720	2371	2373	2376	rVB	100	51	0.00%	0.001%
69	8.874	2408	2421	2456	rBV	507604	818949	80.29%	10.457%
70	9.087	2482	2487	2490	rBV2	230	223	0.02%	0.003%
71	9.399	2581	2584	2587	rBV2	102	78	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091820\
 Data File : VV018344.D
 Acq On : 18 Sep 2020 23:46
 Operator : SY/MD
 Sample : L4080-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

72	9.501	2613	2616	2618	rBV2	133	88	0.01%	0.001%
73	9.572	2635	2638	2640	rBV	100	72	0.01%	0.001%
74	9.617	2649	2652	2653	rBV	100	65	0.01%	0.001%
75	9.727	2683	2686	2689	rBV2	108	72	0.01%	0.001%
76	10.238	2833	2845	2868	rBV	276338	433390	42.49%	5.534%
77	10.357	2881	2882	2884	rVB	171	59	0.01%	0.001%
78	10.379	2886	2889	2890	rBV2	119	67	0.01%	0.001%
79	10.437	2903	2907	2911	rBV2	165	124	0.01%	0.002%
80	10.575	2947	2950	2951	rBV2	107	56	0.01%	0.001%
81	11.196	3141	3143	3144	rBV2	165	77	0.01%	0.001%
82	11.270	3154	3166	3190	rBV	517668	775750	76.05%	9.905%
83	11.353	3190	3192	3197	rVV3	389	291	0.03%	0.004%
84	11.450	3220	3222	3223	rBV3	185	60	0.01%	0.001%
85	11.595	3264	3267	3270	rBV2	139	96	0.01%	0.001%
86	11.646	3271	3283	3307	rBV	493749	765656	75.06%	9.777%
87	11.775	3320	3323	3325	rBV	245	176	0.02%	0.002%
88	11.842	3342	3344	3347	rVB2	204	90	0.01%	0.001%
89	11.952	3376	3378	3381	rVB2	186	64	0.01%	0.001%
90	11.971	3382	3384	3390	rVB2	202	168	0.02%	0.002%
91	12.144	3436	3438	3440	rBV	103	52	0.01%	0.001%
92	12.418	3521	3523	3525	rBV	144	91	0.01%	0.001%
93	12.492	3544	3546	3548	rVB	163	65	0.01%	0.001%
94	12.540	3559	3561	3565	rVB2	185	80	0.01%	0.001%
95	12.562	3566	3568	3572	rBV2	144	83	0.01%	0.001%
96	12.685	3604	3606	3609	rVB	260	98	0.01%	0.001%
97	14.148	4055	4061	4063	rBV3	307	306	0.03%	0.004%
98	14.373	4129	4131	4132	rBV	243	92	0.01%	0.001%
99	14.418	4142	4145	4146	rBV	209	140	0.01%	0.002%
100	16.000	4635	4637	4641	rBV	454	264	0.03%	0.003%


Sum of corrected areas: 7831563

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091820\
Data File : VV018344.D
Acq On : 18 Sep 2020 23:46
Operator : SY/MD
Sample : L4080-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

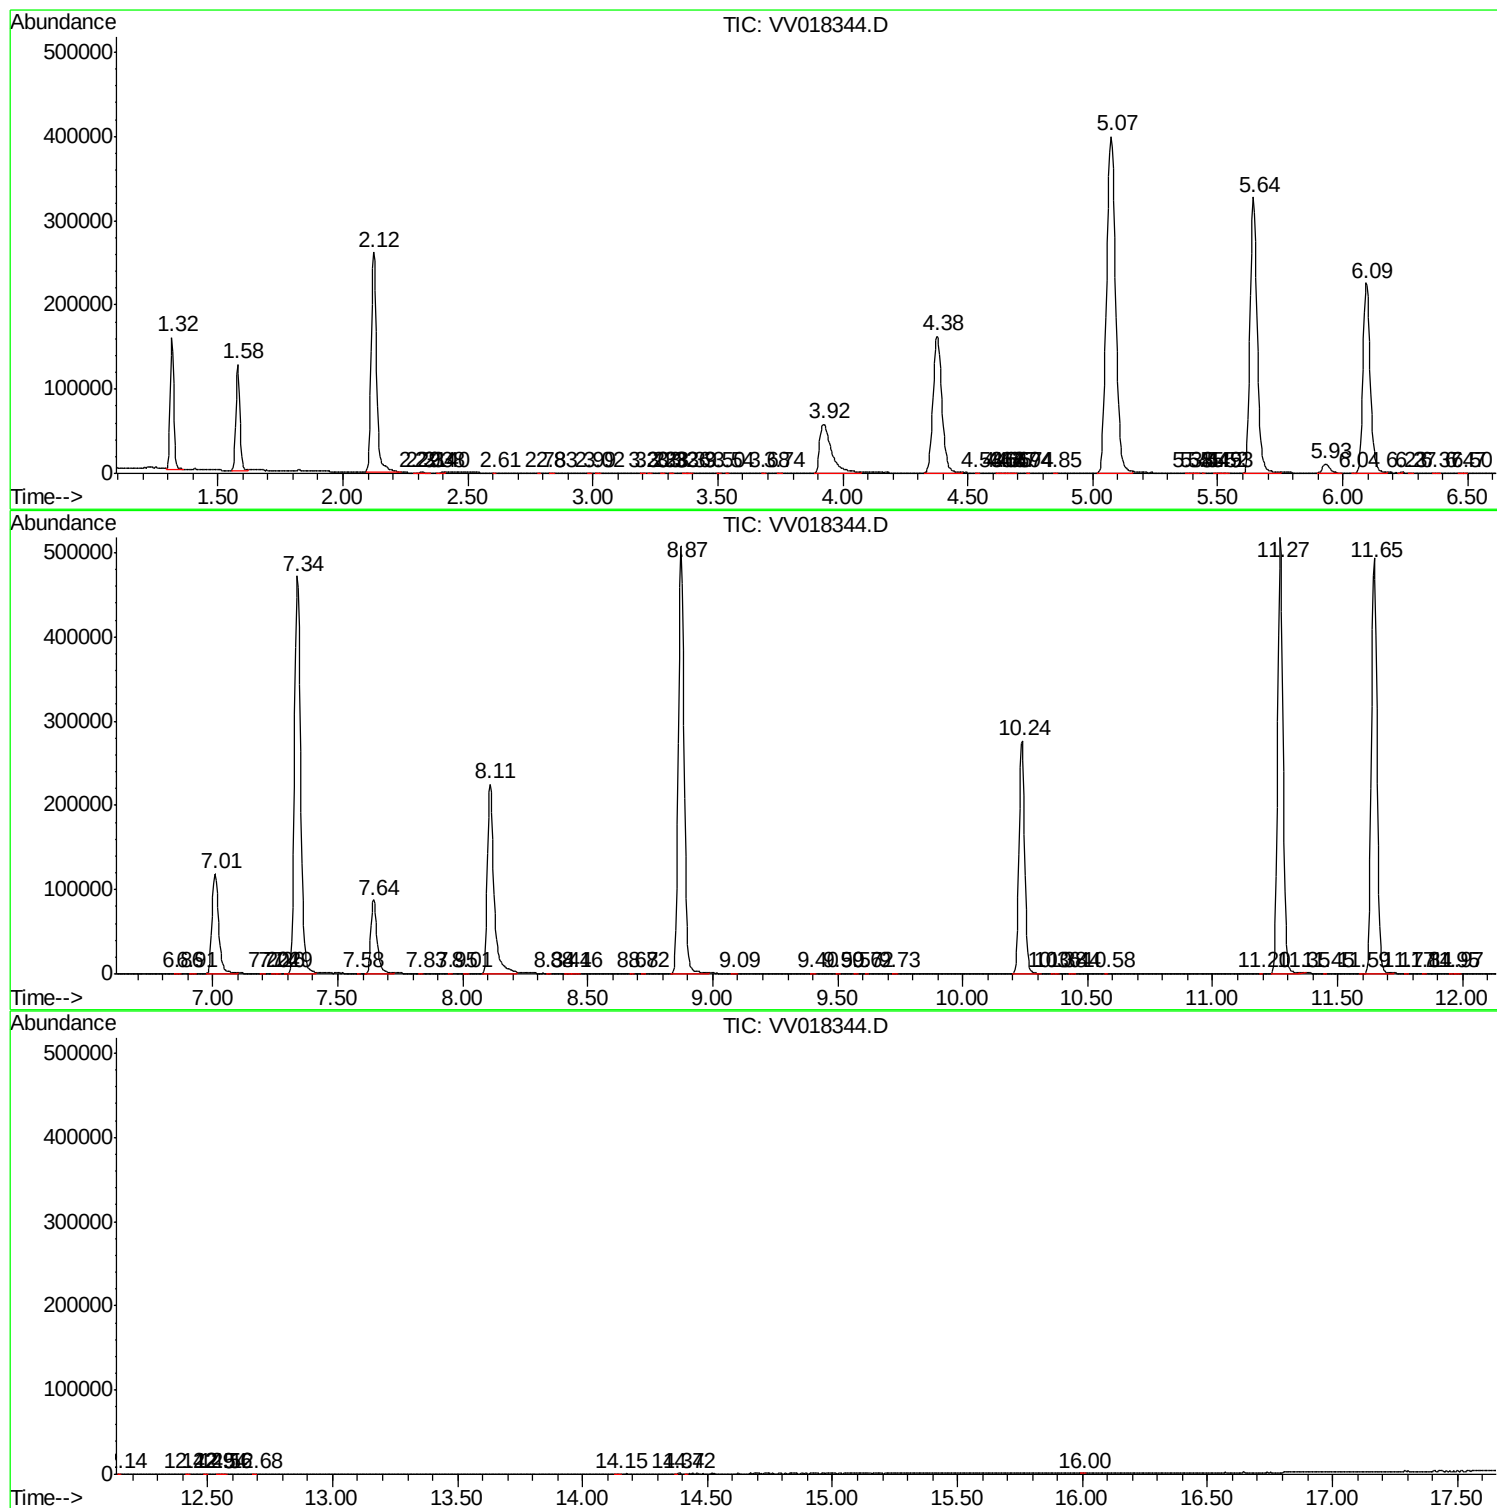

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV091820\
Data File : VV018344.D
Acq On : 18 Sep 2020 23:46
Operator : SY/MD
Sample : L4080-06
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AL8

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV091820\
Data File : VV018344.D
Acq On : 18 Sep 2020 23:46
Operator : SY/MD
Sample : L4080-06
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AL8

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc