

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091820\
 Data File : VV018346.D
 Acq On : 19 Sep 2020 00:31
 Operator : SY/MD
 Sample : L4080-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	63	70	82	rVB	154376	153587	14.99%	1.940%
2	1.579	144	152	169	rBV	124395	143976	14.05%	1.818%
3	2.123	310	321	360	rVB	255218	396706	38.71%	5.010%
4	2.406	406	409	412	rBV2	593	424	0.04%	0.005%
5	2.740	509	513	516	rBV2	155	133	0.01%	0.002%
6	2.807	532	534	535	rBV2	153	48	0.00%	0.001%
7	2.852	545	548	551	rBV2	132	83	0.01%	0.001%
8	2.872	551	554	558	rBV	139	97	0.01%	0.001%
9	2.914	565	567	569	rBV2	150	102	0.01%	0.001%
10	3.029	598	603	605	rBV2	127	127	0.01%	0.002%
11	3.158	639	643	645	rBV2	115	86	0.01%	0.001%
12	3.190	650	653	659	rBV2	138	163	0.02%	0.002%
13	3.290	682	684	686	rVB	160	46	0.00%	0.001%
14	3.492	744	747	750	rBV2	94	62	0.01%	0.001%
15	3.682	804	806	810	rVB	123	71	0.01%	0.001%
16	3.743	823	825	831	rVB2	147	132	0.01%	0.002%
17	3.859	859	861	864	rVB	263	168	0.02%	0.002%
18	3.881	864	868	869	rBV	188	155	0.02%	0.002%
19	3.920	869	880	924	rBV	61590	198729	19.39%	2.510%
20	4.376	1005	1022	1055	rBV	163236	402874	39.31%	5.088%
21	4.524	1066	1068	1070	rVB	125	49	0.00%	0.001%
22	4.540	1070	1073	1076	rBV3	137	83	0.01%	0.001%
23	4.573	1081	1083	1085	rVV3	156	83	0.01%	0.001%
24	4.602	1089	1092	1094	rVB2	154	90	0.01%	0.001%
25	4.663	1108	1111	1118	rBV	103	104	0.01%	0.001%
26	4.724	1127	1130	1134	rVB	161	91	0.01%	0.001%
27	4.759	1138	1141	1142	rBV	84	54	0.01%	0.001%
28	4.785	1147	1149	1152	rBV	76	34	0.00%	0.000%
29	4.939	1194	1197	1201	rBV	93	89	0.01%	0.001%
30	4.997	1212	1215	1220	rBV	138	126	0.01%	0.002%
31	5.074	1221	1239	1272	rBV2	403072	1024802	100.00%	12.943%
32	5.344	1321	1323	1326	rVB	280	149	0.01%	0.002%
33	5.364	1326	1329	1335	rVB2	233	212	0.02%	0.003%
34	5.405	1335	1342	1346	rBV	130	139	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091820\
 Data File : VV018346.D
 Acq On : 19 Sep 2020 00:31
 Operator : SY/MD
 Sample : L4080-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

35	5.466	1354	1361	1362	rBV2	133	152	0.01%	0.002%
36	5.505	1372	1373	1375	rVB2	99	37	0.00%	0.000%
37	5.560	1388	1390	1394	rBV2	98	72	0.01%	0.001%
38	5.579	1394	1396	1398	rBV	136	93	0.01%	0.001%
39	5.640	1403	1415	1446	rBV	336018	668052	65.19%	8.438%
40	5.933	1495	1506	1521	rBV5	11297	23201	2.26%	0.293%
41	6.036	1535	1538	1541	rBV	99	71	0.01%	0.001%
42	6.093	1543	1556	1576	rBV	225339	456464	44.54%	5.765%
43	6.232	1596	1599	1601	rBV3	319	228	0.02%	0.003%
44	6.248	1601	1604	1606	rVV4	358	230	0.02%	0.003%
45	6.331	1627	1630	1633	rBV	125	106	0.01%	0.001%
46	6.499	1678	1682	1686	rBV2	166	147	0.01%	0.002%
47	6.611	1713	1717	1722	rVB2	143	152	0.01%	0.002%
48	6.640	1723	1726	1734	rBV2	177	224	0.02%	0.003%
49	6.701	1738	1745	1752	rBV2	117	191	0.02%	0.002%
50	7.010	1829	1841	1861	rBV	120876	215331	21.01%	2.720%
51	7.187	1895	1896	1898	rVB	157	56	0.01%	0.001%
52	7.200	1898	1900	1901	rBV	105	57	0.01%	0.001%
53	7.245	1910	1914	1916	rBV2	205	120	0.01%	0.002%
54	7.338	1930	1943	1970	rBV	475513	809718	79.01%	10.227%
55	7.643	2028	2038	2059	rBV	87406	149744	14.61%	1.891%
56	7.827	2091	2095	2101	rVB3	328	334	0.03%	0.004%
57	7.958	2131	2136	2143	rVB	306	396	0.04%	0.005%
58	8.109	2172	2183	2219	rBV	224842	415259	40.52%	5.245%
59	8.286	2236	2238	2246	rVB3	646	615	0.06%	0.008%
60	8.412	2274	2277	2280	rVB2	249	167	0.02%	0.002%
61	8.450	2287	2289	2293	rVB	138	45	0.00%	0.001%
62	8.553	2318	2321	2324	rBV	164	105	0.01%	0.001%
63	8.582	2327	2330	2336	rVB2	148	116	0.01%	0.001%
64	8.743	2372	2380	2382	rBV2	137	208	0.02%	0.003%
65	8.830	2404	2407	2409	rBV2	123	74	0.01%	0.001%
66	8.875	2409	2421	2453	rBV	518989	844204	82.38%	10.662%
67	9.116	2489	2496	2500	rBV2	210	293	0.03%	0.004%
68	9.174	2512	2514	2516	rBV2	152	82	0.01%	0.001%
69	9.402	2581	2585	2589	rVB2	176	144	0.01%	0.002%
70	9.425	2589	2592	2599	rBV	134	142	0.01%	0.002%
71	9.579	2637	2640	2647	rVB	133	126	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091820\
 Data File : VV018346.D
 Acq On : 19 Sep 2020 00:31
 Operator : SY/MD
 Sample : L4080-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAMO

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

72	9.797	2706	2708	2710	rBV2	67	36	0.00%	0.000%
73	9.839	2719	2721	2723	rBV	103	63	0.01%	0.001%
74	9.884	2733	2735	2738	rBV	77	46	0.00%	0.001%
75	10.090	2796	2799	2802	rBV	153	94	0.01%	0.001%
76	10.238	2832	2845	2869	rBV	283136	436455	42.59%	5.512%
77	10.322	2869	2871	2873	rVV	154	44	0.00%	0.001%
78	10.376	2885	2888	2890	rBV2	151	100	0.01%	0.001%
79	10.392	2890	2893	2897	rBV3	203	222	0.02%	0.003%
80	10.717	2991	2994	2999	rBV2	95	105	0.01%	0.001%
81	11.270	3155	3166	3192	rBV	529511	803926	78.45%	10.154%
82	11.379	3197	3200	3202	rVB	225	134	0.01%	0.002%
83	11.588	3262	3265	3266	rBV	109	71	0.01%	0.001%
84	11.646	3271	3283	3308	rVV	494828	764426	74.59%	9.655%
85	11.794	3327	3329	3332	rBV	135	61	0.01%	0.001%
86	11.929	3368	3371	3373	rBV	273	151	0.01%	0.002%
87	12.000	3391	3393	3398	rVB	270	170	0.02%	0.002%
88	12.061	3409	3412	3414	rBV2	130	88	0.01%	0.001%
89	12.579	3572	3573	3577	rBV2	138	56	0.01%	0.001%
90	12.640	3590	3592	3593	rBV2	122	55	0.01%	0.001%
91	12.916	3676	3678	3681	rBV2	114	80	0.01%	0.001%
92	13.209	3767	3769	3773	rVB	168	97	0.01%	0.001%
93	13.431	3835	3838	3842	rBV2	245	208	0.02%	0.003%
94	13.521	3863	3866	3869	rBV	205	142	0.01%	0.002%
95	14.093	4042	4044	4046	rBV	170	66	0.01%	0.001%
96	14.334	4116	4119	4121	rBV	161	84	0.01%	0.001%


Sum of corrected areas: 7917610

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091820\
Data File : VV018346.D
Acq On : 19 Sep 2020 00:31
Operator : SY/MD
Sample : L4080-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAM0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

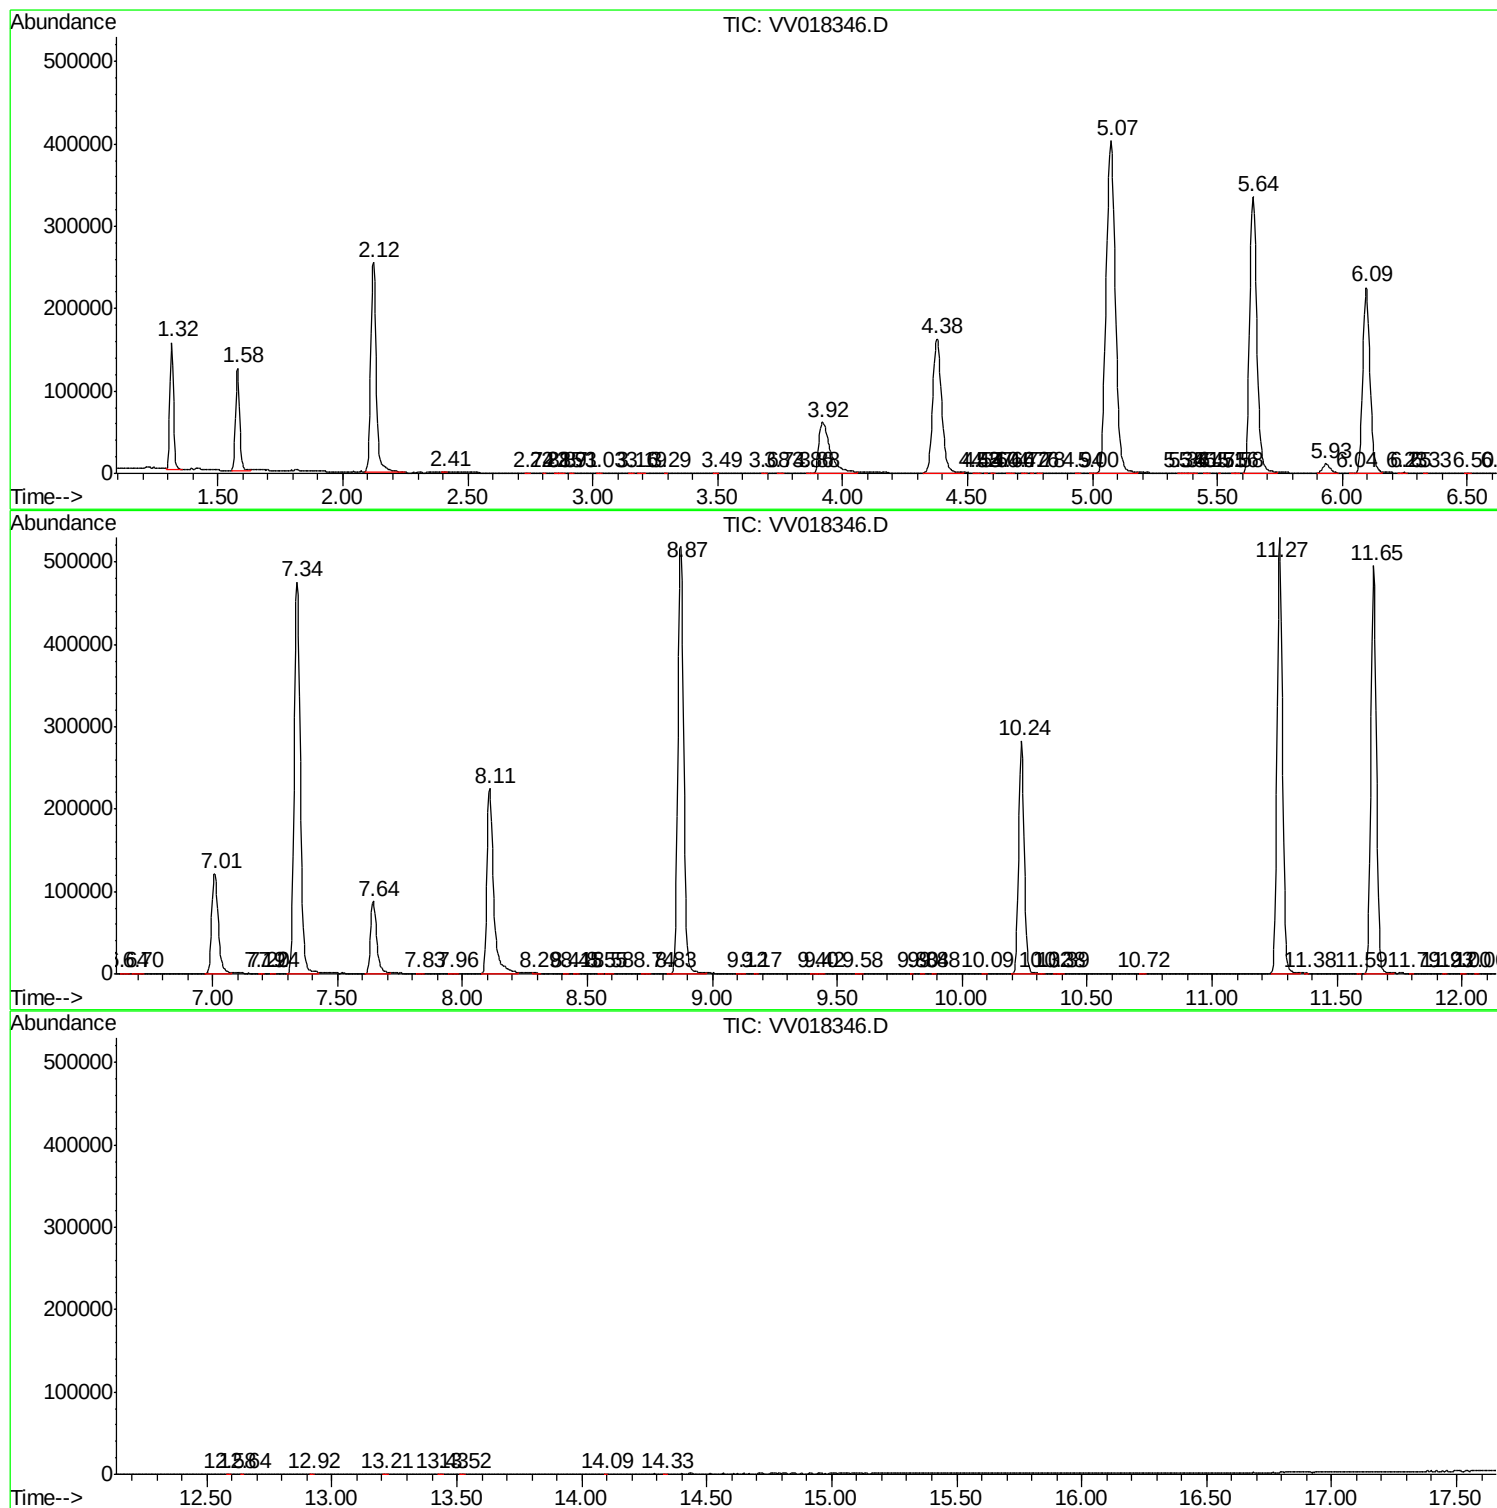

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV091820\
Data File : VV018346.D
Acq On : 19 Sep 2020 00:31
Operator : SY/MD
Sample : L4080-08
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AM0

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV091820\
Data File : VV018346.D
Acq On : 19 Sep 2020 00:31
Operator : SY/MD
Sample : L4080-08
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AM0

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc