


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091918\
 Data File : VV007636.D
 Acq On : 19 Sep 2018 19:42
 Operator : SY/MD
 Sample : BFB99
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB99

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Sep 21 03:27:29 2018

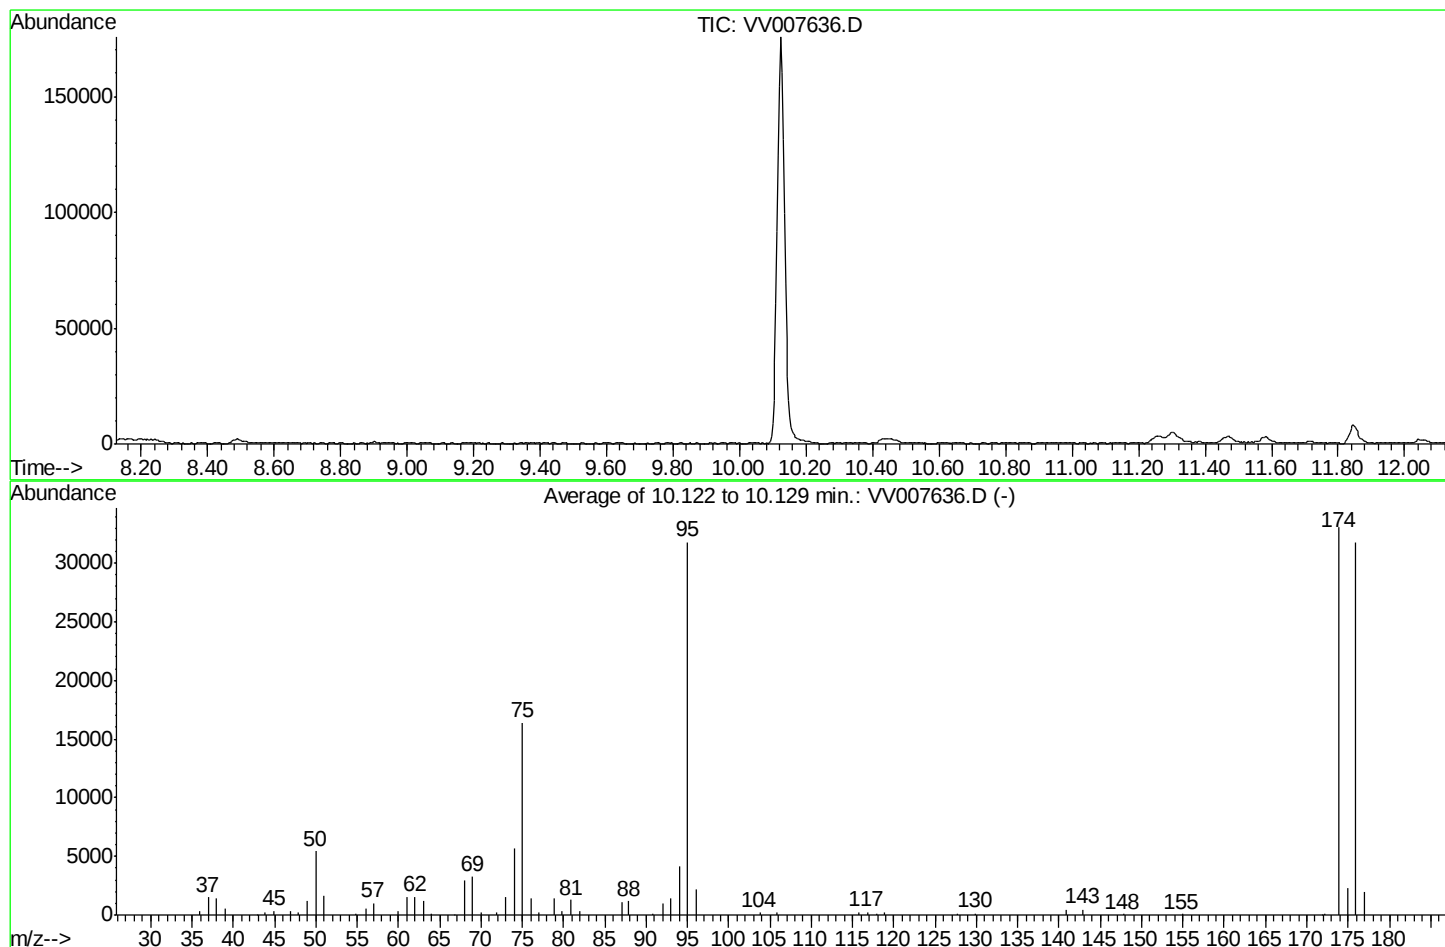

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	5417	PASS
75	95	30	80	51.6	16418	PASS
95	95	100	100	100.0	31818	PASS
96	95	5	9	6.7	2145	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	103.9	33056	PASS
175	174	5	9	7.0	2314	PASS
176	174	95	101	96.2	31784	PASS
177	176	5	9	6.3	2009	PASS

m/z	Abundance
43.90	298.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
35.80	348.0
37.00	1636.0
38.00	1495.0
39.00	517.0
43.90	504.0
44.90	362.0
46.90	338.0
47.80	199.0
48.90	1131.0
50.00	5814.0
51.00	1636.0
54.90	109.0
56.00	555.0
57.00	1090.0
60.00	314.0
61.00	1654.0
62.00	1598.0
63.00	1194.0
66.80	112.0
68.00	3209.0
69.00	3335.0
70.00	260.0
71.80	204.0
73.00	1493.0
74.00	5890.0
75.00	16712.0
76.00	1488.0
77.10	178.0
78.90	1517.0
79.90	327.0
80.90	1331.0
81.90	310.0
87.00	1148.0
87.90	1216.0
90.80	158.0
92.00	1023.0
92.90	1504.0
94.00	4190.0
95.00	32752.0
96.00	2235.0
103.80	226.0
105.90	215.0
115.80	189.0
116.80	225.0
117.90	111.0
118.80	209.0
127.70	114.0
129.90	136.0
140.80	455.0
142.90	563.0
172.20	152.0
173.90	33152.0
174.90	2354.0
175.90	32160.0
176.90	1944.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
35.80	302.0
36.90	1554.0
38.00	1449.0
39.00	572.0
43.90	524.0
45.00	347.0
46.90	301.0
47.80	213.0
48.90	1212.0
50.00	5528.0
51.00	1641.0
54.80	114.0
56.00	563.0
57.00	1078.0
59.90	318.0
61.00	1603.0
62.00	1621.0
63.00	1258.0
63.90	103.0
68.00	3016.0
69.00	3341.0
70.00	254.0
71.80	182.0
73.00	1584.0
74.00	5881.0
75.00	17056.0
76.00	1448.0
77.10	192.0
78.90	1463.0
79.80	348.0
80.90	1353.0
81.90	330.0
87.00	1127.0
87.90	1201.0
90.80	178.0
92.00	1060.0
92.90	1525.0
94.00	4295.0
95.00	33024.0
96.00	2254.0
103.80	223.0
105.90	220.0
115.80	194.0
116.80	232.0
117.90	117.0
118.80	203.0
127.80	107.0
129.90	127.0
140.90	461.0
142.90	509.0
147.80	109.0
154.90	103.0
173.90	34328.0
174.90	2387.0
175.90	32912.0
176.90	2073.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
35.90	238.0
36.90	1389.0
38.00	1292.0
39.00	572.0
42.90	107.0
43.90	496.0
45.00	278.0
46.90	257.0
47.90	189.0
49.00	1208.0
50.00	4909.0
51.00	1504.0
54.80	120.0
56.00	508.0
56.90	932.0
59.90	297.0
61.00	1369.0
62.00	1495.0
63.00	1192.0
63.90	125.0
68.00	2659.0
69.00	3042.0
70.00	227.0
71.90	147.0
73.00	1477.0
74.00	5275.0
75.00	15486.0
76.00	1238.0
77.00	197.0
78.90	1287.0
79.80	328.0
80.90	1197.0
81.90	303.0
87.00	1094.0
87.90	1187.0
90.80	160.0
92.00	907.0
92.90	1358.0
94.00	3886.0
95.00	29680.0
96.00	1948.0
103.80	199.0
105.80	184.0
115.80	180.0
116.80	227.0
117.90	101.0
118.80	182.0
129.90	125.0
140.90	427.0
142.90	412.0
147.80	107.0
154.90	102.0
171.80	132.0
172.10	139.0
173.90	31688.0
175.00	2202.0
175.90	30280.0
176.90	2012.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99