


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091919\
 Data File : VV012906.D
 Acq On : 18 Sep 2019 21:08
 Operator : SY/MD
 Sample : BFB41
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB002

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVTR072919WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Dec 20 08:09:34 2019

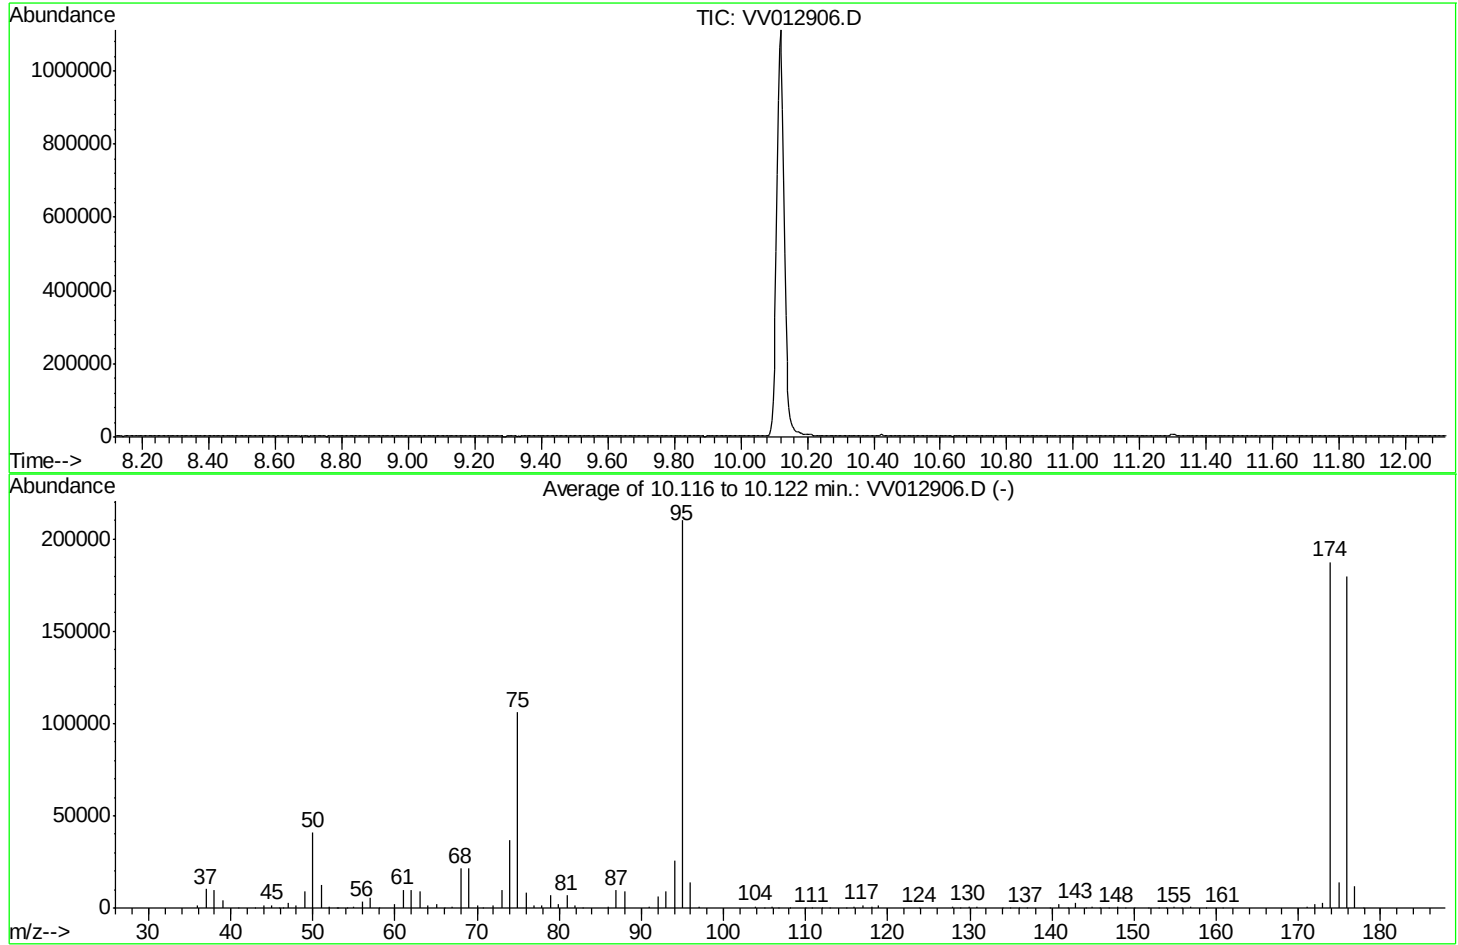

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	40928	PASS
75	95	30	80	50.4	105845	PASS
95	95	100	100	100.0	210133	PASS
96	95	5	9	6.6	13843	PASS
173	174	0.00	2	1.4	2533	PASS
174	95	50	120	89.3	187584	PASS
175	174	5	9	7.6	14182	PASS
176	174	95	101	95.8	179712	PASS
177	176	5	9	6.4	11575	PASS

m/z	Abundance
36.00	1773.0
37.00	9695.0
38.00	8985.0
39.00	3722.0
40.00	1305.0
42.90	135.0
44.00	2141.0
45.00	1567.0
46.00	423.0
47.00	2860.0
47.90	1269.0
49.00	8599.0
50.00	38912.0
51.00	12302.0
52.00	476.0
53.10	203.0
55.00	480.0
56.00	3253.0
57.00	5564.0
58.00	243.0
60.00	2083.0
61.00	9808.0
62.00	9392.0
63.00	8873.0
64.00	1394.0
65.00	1807.0
66.00	230.0
66.90	507.0
68.00	20392.0
69.00	20896.0
70.10	1596.0
70.80	164.0
72.00	1160.0
73.00	8952.0
74.00	35600.0
75.00	102400.0
76.00	8329.0
76.90	1370.0
77.90	1167.0
78.90	6374.0
79.90	2030.0
80.90	6246.0
81.90	1308.0
82.90	165.0
85.90	497.0
87.00	9004.0
87.90	8614.0
90.90	869.0
92.00	5964.0
93.00	8863.0
94.00	24824.0
95.00	204224.0
96.00	12920.0
97.10	293.0
103.90	887.0
104.90	261.0
105.90	871.0
106.70	241.0
109.90	165.0
110.70	128.0
112.90	155.0
114.90	298.0
115.90	722.0
116.90	1430.0
118.00	909.0
118.90	1381.0
123.90	110.0
127.80	786.0
128.80	311.0
129.80	759.0
130.90	420.0
133.90	104.0
134.90	327.0
136.00	114.0
136.80	356.0
139.80	211.0
140.90	1900.0
141.90	293.0
142.90	2526.0
144.00	305.0
144.90	728.0
145.80	389.0
146.90	106.0
147.90	405.0
149.00	169.0
150.10	275.0
151.80	119.0
153.00	161.0
153.90	126.0
154.90	641.0
155.70	144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB002

156.80	378.0
158.80	271.0
160.80	327.0
171.00	529.0
172.00	2516.0
173.00	2492.0
173.90	186944.0
174.90	14026.0
175.90	178560.0
176.90	10993.0
177.90	311.0

Instrument :
MSVOA_V
ClientSampleId :
BFB002

m/z	Abundance
36.00	1916.0
37.00	10445.0
38.00	9757.0
39.00	3981.0
40.00	1218.0
40.90	113.0
42.90	123.0
44.00	2171.0
45.00	1715.0
46.00	355.0
46.90	3140.0
48.00	1371.0
49.00	9274.0
50.00	42464.0
51.00	13296.0
52.00	536.0
52.90	261.0
54.20	118.0
55.00	522.0
56.00	3414.0
57.00	5942.0
58.00	290.0
60.00	2220.0
61.00	10164.0
62.00	9938.0
63.00	9345.0
64.00	1652.0
65.00	1787.0
65.90	212.0
67.00	483.0
68.00	22136.0
69.00	22064.0
70.00	1816.0
70.70	139.0
72.00	1289.0
73.00	9634.0
74.00	38280.0
75.00	109272.0
76.00	8928.0
76.90	1560.0
77.90	1200.0
78.90	6952.0
79.90	2201.0
80.90	6810.0
81.90	1476.0
82.90	168.0
85.90	452.0
87.00	9779.0
88.00	9402.0
90.90	975.0
92.00	6391.0
93.00	9425.0
94.00	26512.0
95.00	217088.0
96.00	14324.0
97.00	416.0
103.90	916.0
104.90	302.0
105.90	941.0
106.70	234.0
108.10	111.0
110.00	156.0
110.70	179.0
112.90	199.0
114.90	306.0
115.90	781.0
116.90	1606.0
118.00	899.0
118.90	1426.0
123.90	103.0
127.80	793.0
128.80	331.0
129.80	803.0
130.80	499.0
133.90	116.0
134.90	381.0
136.90	377.0
139.80	182.0
140.90	2034.0
141.90	280.0
142.90	2814.0
144.00	278.0
145.00	897.0
145.90	346.0
146.90	106.0
147.90	376.0
149.00	130.0
150.00	205.0
151.80	179.0
153.10	152.0
153.90	161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB002

154.90	707.0
155.80	118.0
156.80	416.0
158.80	265.0
160.80	298.0
171.00	564.0
172.00	2451.0
173.00	2634.0
173.90	194688.0
175.00	14673.0
175.90	186304.0
176.90	11881.0
177.90	359.0

Instrument :
MSVOA_V
ClientSampleId :
BFB002

m/z	Abundance
36.00	1938.0
37.00	10351.0
38.00	9507.0
39.00	3894.0
40.00	1100.0
40.90	132.0
42.90	125.0
44.00	1943.0
45.00	1764.0
45.90	258.0
46.30	275.0
46.90	2982.0
48.00	1321.0
49.00	8985.0
50.00	41408.0
51.00	12864.0
52.00	546.0
52.90	325.0
54.20	171.0
55.00	536.0
56.00	3161.0
57.00	5812.0
58.00	334.0
60.00	2202.0
61.00	9894.0
62.00	9717.0
63.00	8958.0
64.00	1633.0
65.00	1735.0
65.90	228.0
67.00	468.0
68.00	21712.0
69.00	21192.0
70.00	1826.0
72.00	1300.0
73.00	9595.0
74.00	36888.0
75.00	106176.0
76.00	8712.0
76.90	1493.0
77.90	1066.0
78.90	6883.0
79.90	2145.0
80.90	6965.0
81.90	1586.0
82.90	178.0
86.00	348.0
86.90	9411.0
88.00	9040.0
90.90	872.0
92.00	6234.0
93.00	9425.0
94.00	25384.0
95.00	209088.0
96.00	14285.0
97.00	529.0
103.90	924.0
104.90	315.0
105.90	896.0
106.80	179.0
108.00	124.0
110.10	146.0
110.80	172.0
112.00	109.0
112.90	196.0
114.90	293.0
115.90	826.0
116.90	1584.0
118.00	752.0
118.90	1334.0
127.90	722.0
128.80	356.0
129.90	742.0
130.80	469.0
135.00	368.0
136.90	367.0
139.70	146.0
140.90	1962.0
141.80	275.0
142.90	2932.0
144.10	203.0
145.00	957.0
145.90	303.0
146.90	103.0
148.00	351.0
149.00	107.0
150.00	151.0
151.80	192.0
153.10	141.0
153.90	164.0
154.90	662.0

Instrument :
MSVOA_V
ClientSampleId :
BFB002

155.90	121.0
156.80	409.0
158.80	240.0
160.80	253.0
171.00	480.0
171.90	2311.0
173.00	2473.0
173.90	181120.0
175.00	13848.0
175.90	174272.0
176.90	11852.0
177.90	310.0

Instrument :
MSVOA_V
ClientSampleId :
BFB002

Scan 2792 (10.068 min): VV012906.D
BFB41

m/z	Abundance
35.90	153.0
39.90	1224.0
44.00	874.0
74.80	104.0
77.10	115.0
207.20	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB002