




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091924\
 Data File : VV037388.D
 Acq On : 19 Sep 2024 17:27
 Operator : SY/MD
 Sample : P3986-20 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH8P0

Manual IntegrationsAPPROVED

Quant Time: Sep 20 01:59:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 20 01:54:17 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/20/2024
 Supervised By :Mahesh Dadoda 09/23/2024

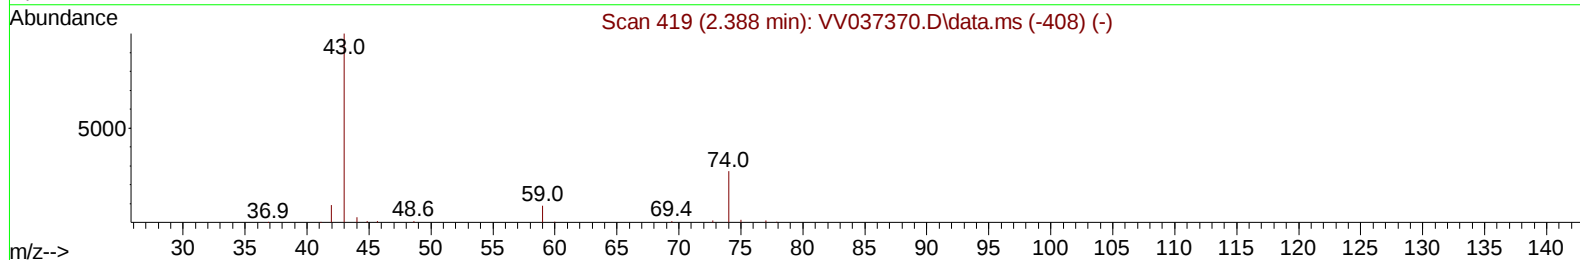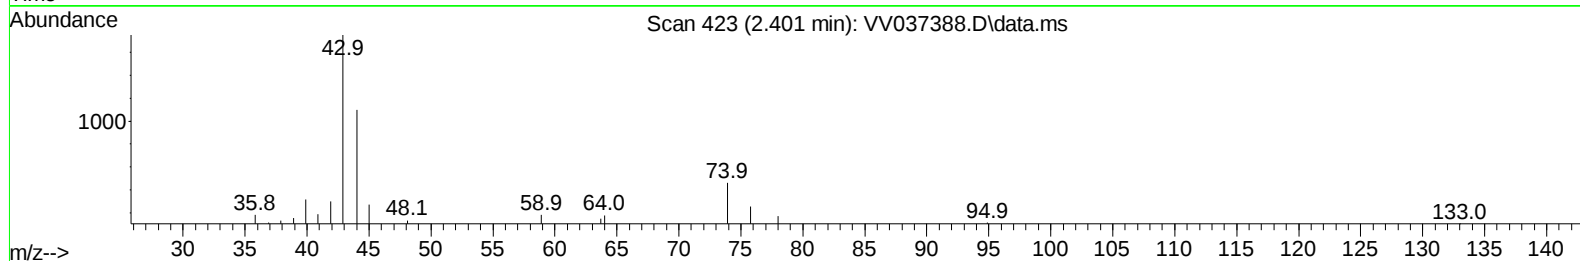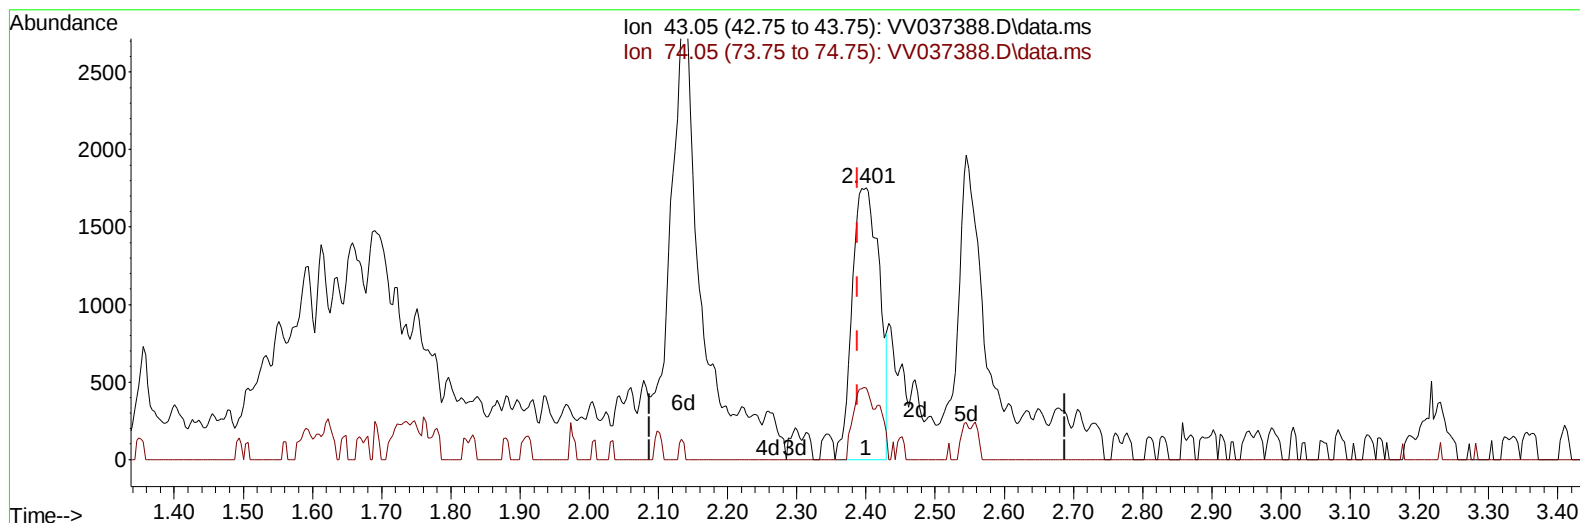

TIC: VV037388.D\data.ms

(15) Methyl Acetate (T)

2.401min (+ 0.013) 0.54 ug/L

response 4826

Ion	Exp%	Act%
43.05	100.00	100.00
74.05	26.20	18.88#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091924\
Data File : VV037388.D
Acq On : 19 Sep 2024 17:27
Operator : SY/MD
Sample : P3986-20 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH8P0

Manual IntegrationsAPPROVED

Quant Time: Sep 20 01:59:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 20 01:54:17 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/20/2024
Supervised By :Mahesh Dadoda 09/23/2024

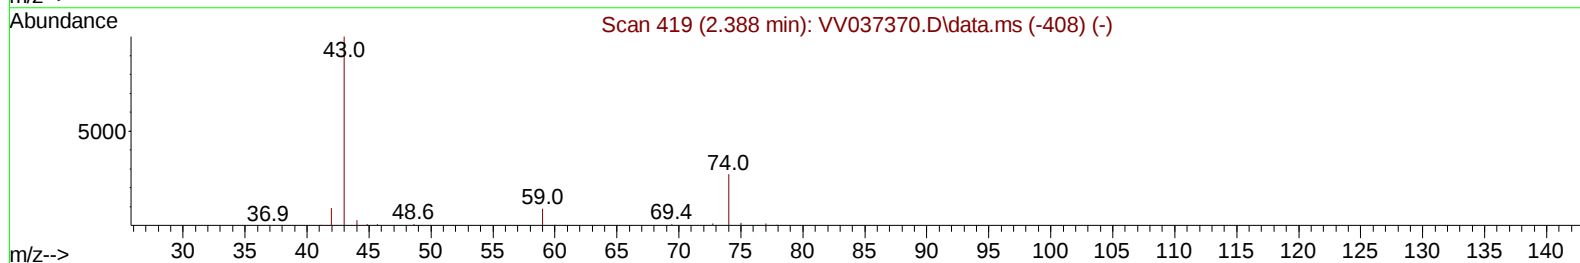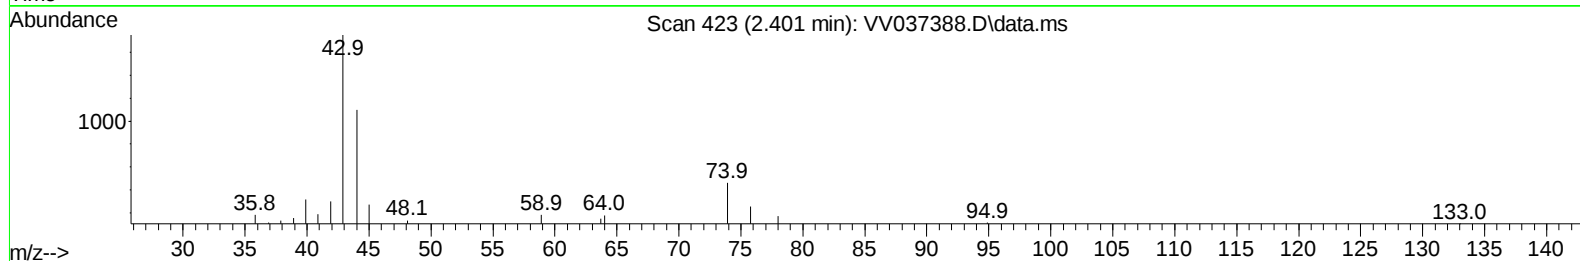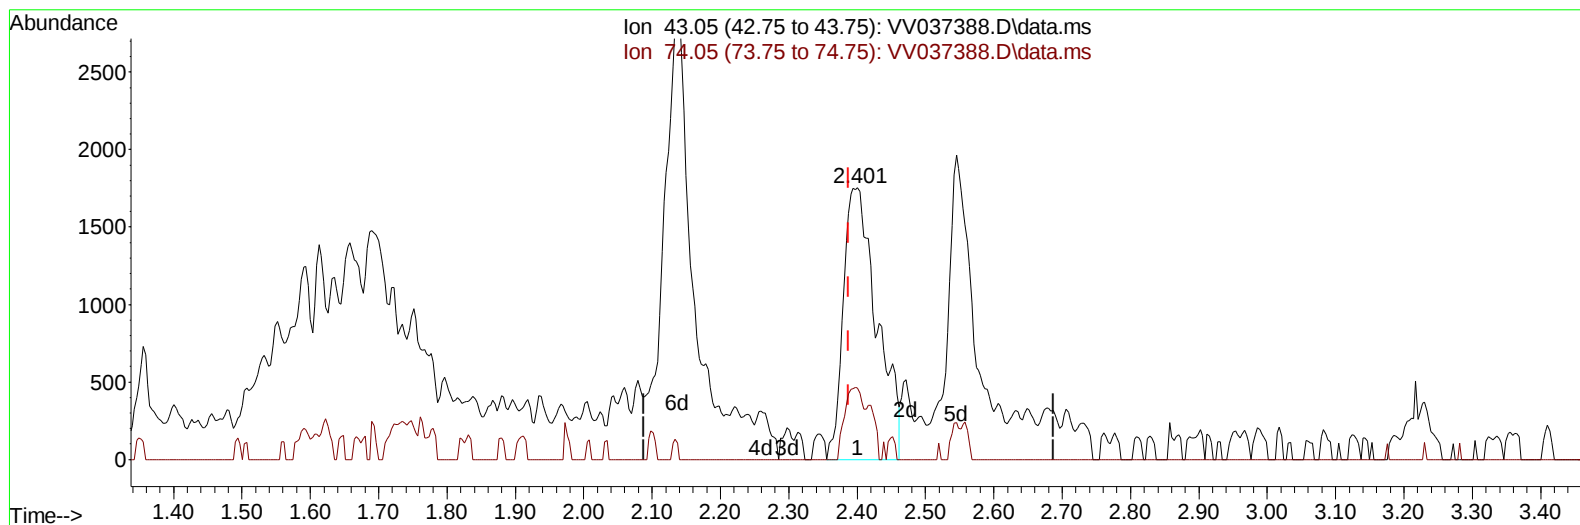

TIC: VV037388.D\data.ms

(15) Methyl Acetate (T)

2.401min (+ 0.013) 0.67 ug/L m

response 5995

Ion	Exp%	Act%
43.05	100.00	100.00
74.05	26.20	15.20#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091924\
 Data File : VV037388.D
 Acq On : 19 Sep 2024 17:27
 Operator : SY/MD
 Sample : P3986-20 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH8P0

Manual IntegrationsAPPROVED

Quant Time: Sep 20 01:59:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 20 01:54:17 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/20/2024
 Supervised By :Mahesh Dadoda 09/23/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	318783	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	333707	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.182	152	156667	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	66238	3.542	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	70.800%	
7) Chloroethane-d5	1.529	69	80794	4.143	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	82.800%	
11) 1,1-Dichloroethene-d2	2.047	65	37148	3.846	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	77.000%	
20) 2-Butanone-d5	3.809	46	293990	52.599	ug/L	-0.02
Spiked Amount 50.000	Range 40	- 130	Recovery	=	105.200%	
24) Chloroform-d	4.240	84	206430	4.546	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	91.000%	
26) 1,2-Dichloroethane-d4	4.937	65	100507	4.727	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	94.600%	
32) Benzene-d6	4.950	84	381671	4.266	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	85.400%	
36) 1,2-Dichloropropane-d6	5.982	67	131263	4.718	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	94.400%	
41) Toluene-d8	7.240	98	307682	3.817	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	76.400%	
43) trans-1,3-Dichloroprop...	7.561	79	33820	3.695	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	74.000%	
46) 2-Hexanone-d5	8.034	63	235842	52.741	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	105.480%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	115588	5.097	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	102.000%	
66) 1,2-Dichlorobenzene-d4	11.558	152	129529	4.650	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	93.000%	
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.278	62	57354	1.847	ug/L	86
12) 1,1-Dichloroethene	2.057	96	20843	0.933	ug/L #	1
15) Methyl Acetate	2.401	43	5995m	0.673	ug/L	
19) 1,1-Dichloroethane	3.105	63	81395	1.814	ug/L	99
22) cis-1,2-Dichloroethene	3.802	96	384964	15.151	ug/L	99
34) Trichloroethene	5.834	95	29271	1.080	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091924\
Data File : VV037388.D
Acq On : 19 Sep 2024 17:27
Operator : SY/MD
Sample : P3986-20 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH8P0

Manual IntegrationsAPPROVED

Quant Time: Sep 20 01:59:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 20 01:54:17 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/20/2024
Supervised By :Mahesh Dadoda 09/23/2024

