

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091924\
 Data File : VV037400.D
 Acq On : 19 Sep 2024 23:05
 Operator : SY/MD
 Sample : P3990-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS0

Quant Time: Sep 20 04:15:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 20 03:11:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	305215	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	315450	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	148063	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	62470	3.489	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	69.800%
7) Chloroethane-d5	1.529	69	77354	4.143	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.800%
11) 1,1-Dichloroethene-d2	2.053	65	34703	3.753	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.000%
20) 2-Butanone-d5	3.809	46	266318	49.766	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.540%
24) Chloroform-d	4.243	84	199512	4.589	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.800%
26) 1,2-Dichloroethane-d4	4.941	65	99868	4.906	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.200%
32) Benzene-d6	4.953	84	367316	4.343	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.800%
36) 1,2-Dichloropropane-d6	5.986	67	126472	4.808	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.200%
41) Toluene-d8	7.239	98	301111	3.951	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.000%
43) trans-1,3-Dichloroprop...	7.561	79	29746	3.438	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.800%
46) 2-Hexanone-d5	8.024	63	210682	49.841	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.680%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	110153	5.139	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.800%
66) 1,2-Dichlorobenzene-d4	11.558	152	127276	4.835	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.800%
Target Compounds						
					Qvalue	
13) Acetone	2.137	43	59340	15.926	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091924\
Data File : VV037400.D
Acq On : 19 Sep 2024 23:05
Operator : SY/MD
Sample : P3990-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS0

Quant Time: Sep 20 04:15:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 20 03:11:07 2024
Response via : Initial Calibration

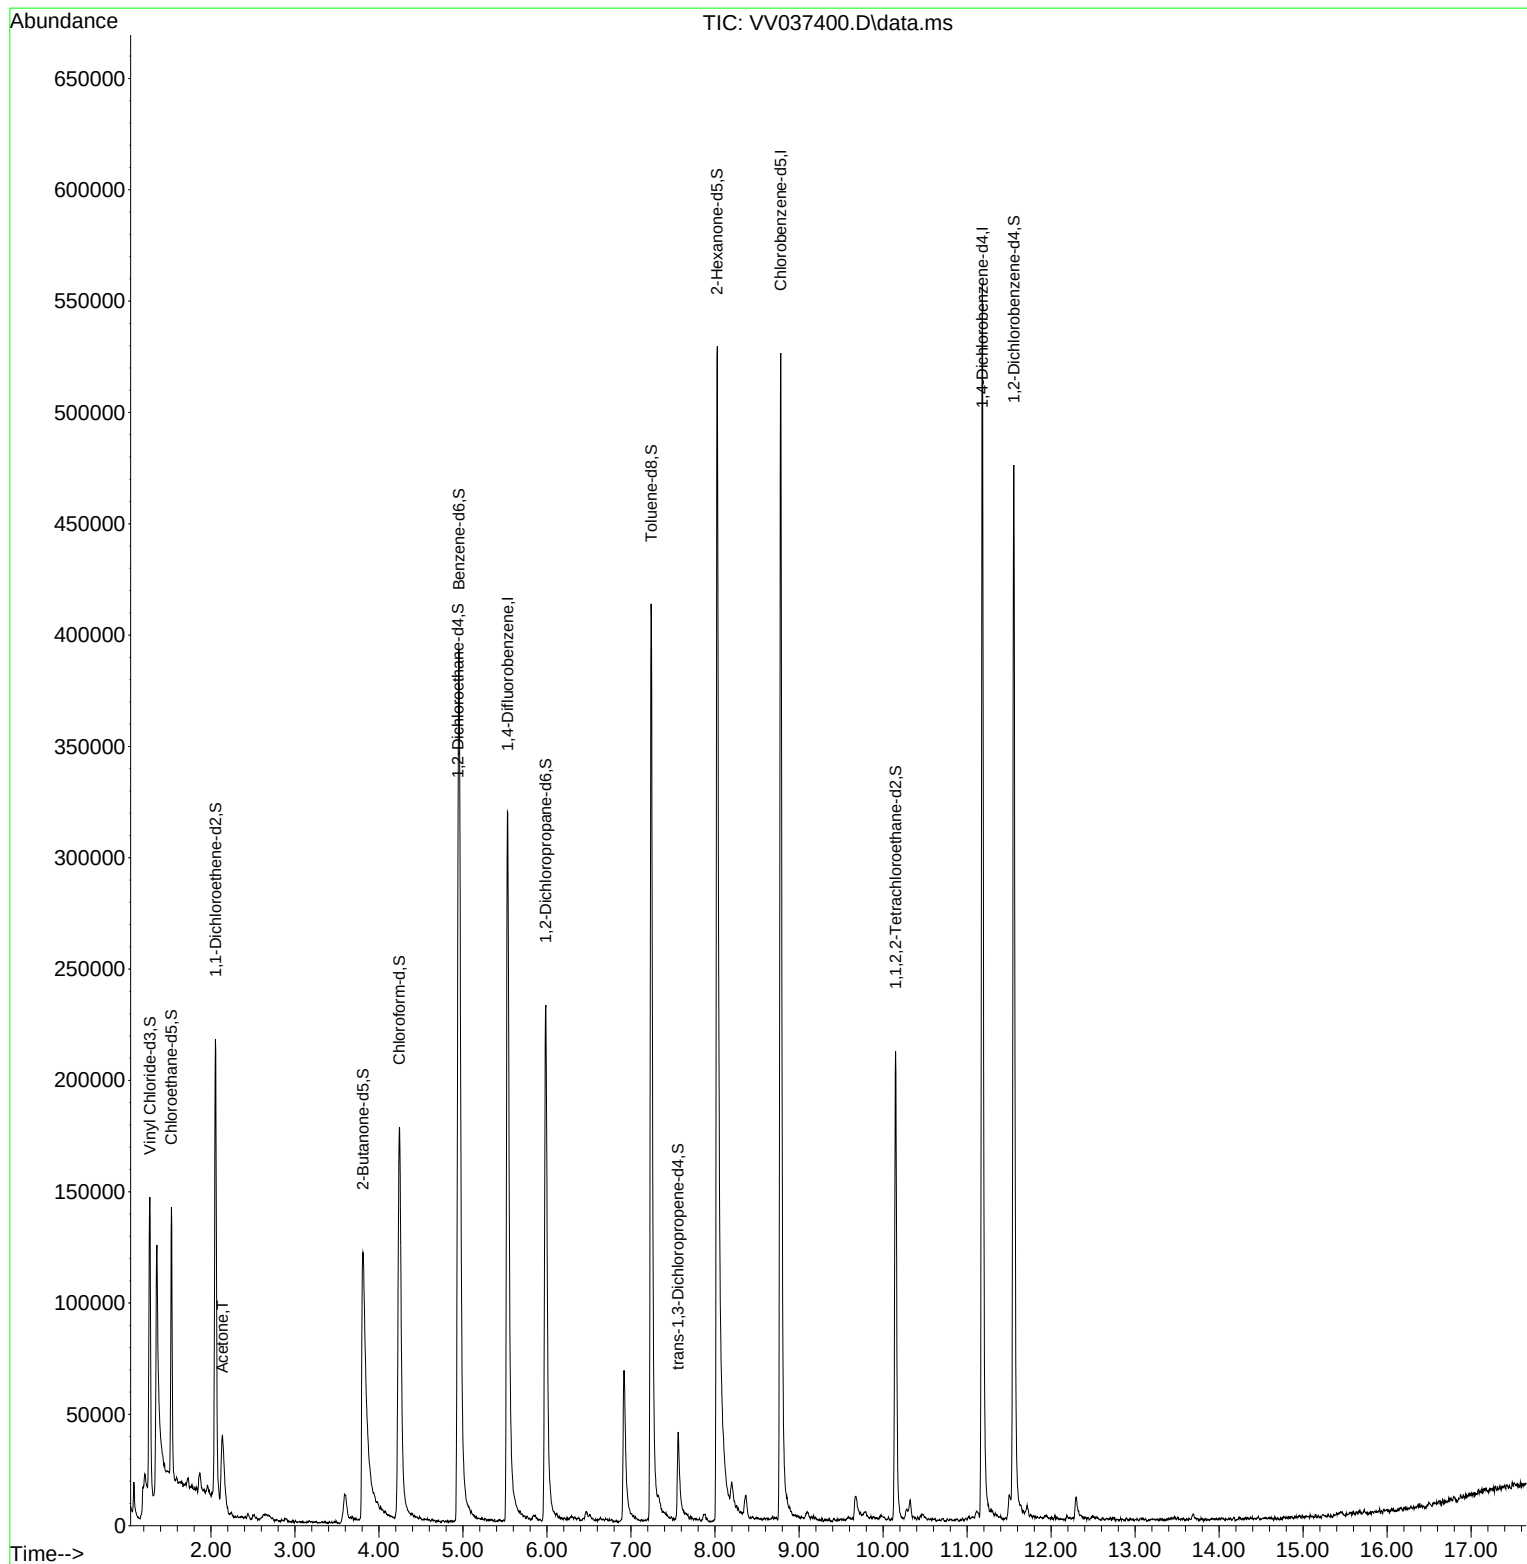

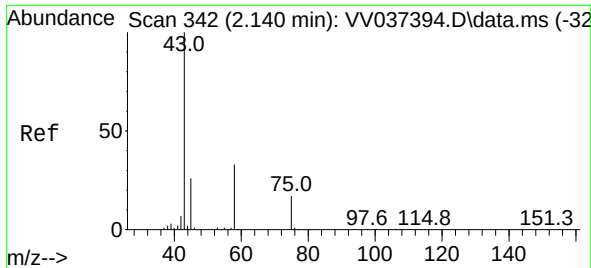

#13

Acetone

Concen: 15.926 ug/L

RT: 2.137 min Scan# 34

Delta R.T. -0.003 min

Lab File: VV037400.D


Acq: 19 Sep 2024 23:05

Instrument :

MSVOA_V

ClientSampleId :

C0AS0

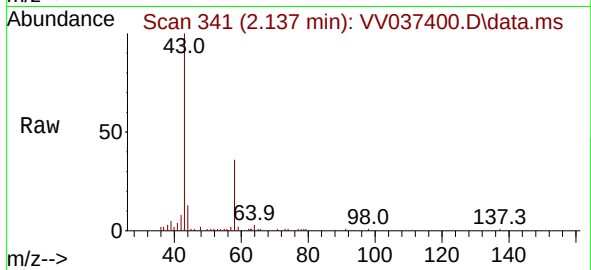

Tgt Ion: 43 Resp: 59340

Ion Ratio Lower Upper

43 100

58 34.2 0.0 69.2

