


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091924\
Data File : VV037369.D
Acq On : 19 Sep 2024 09:05
Operator : SY/MD
Sample : BFB276
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB276

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Sep 21 01:15:22 2024

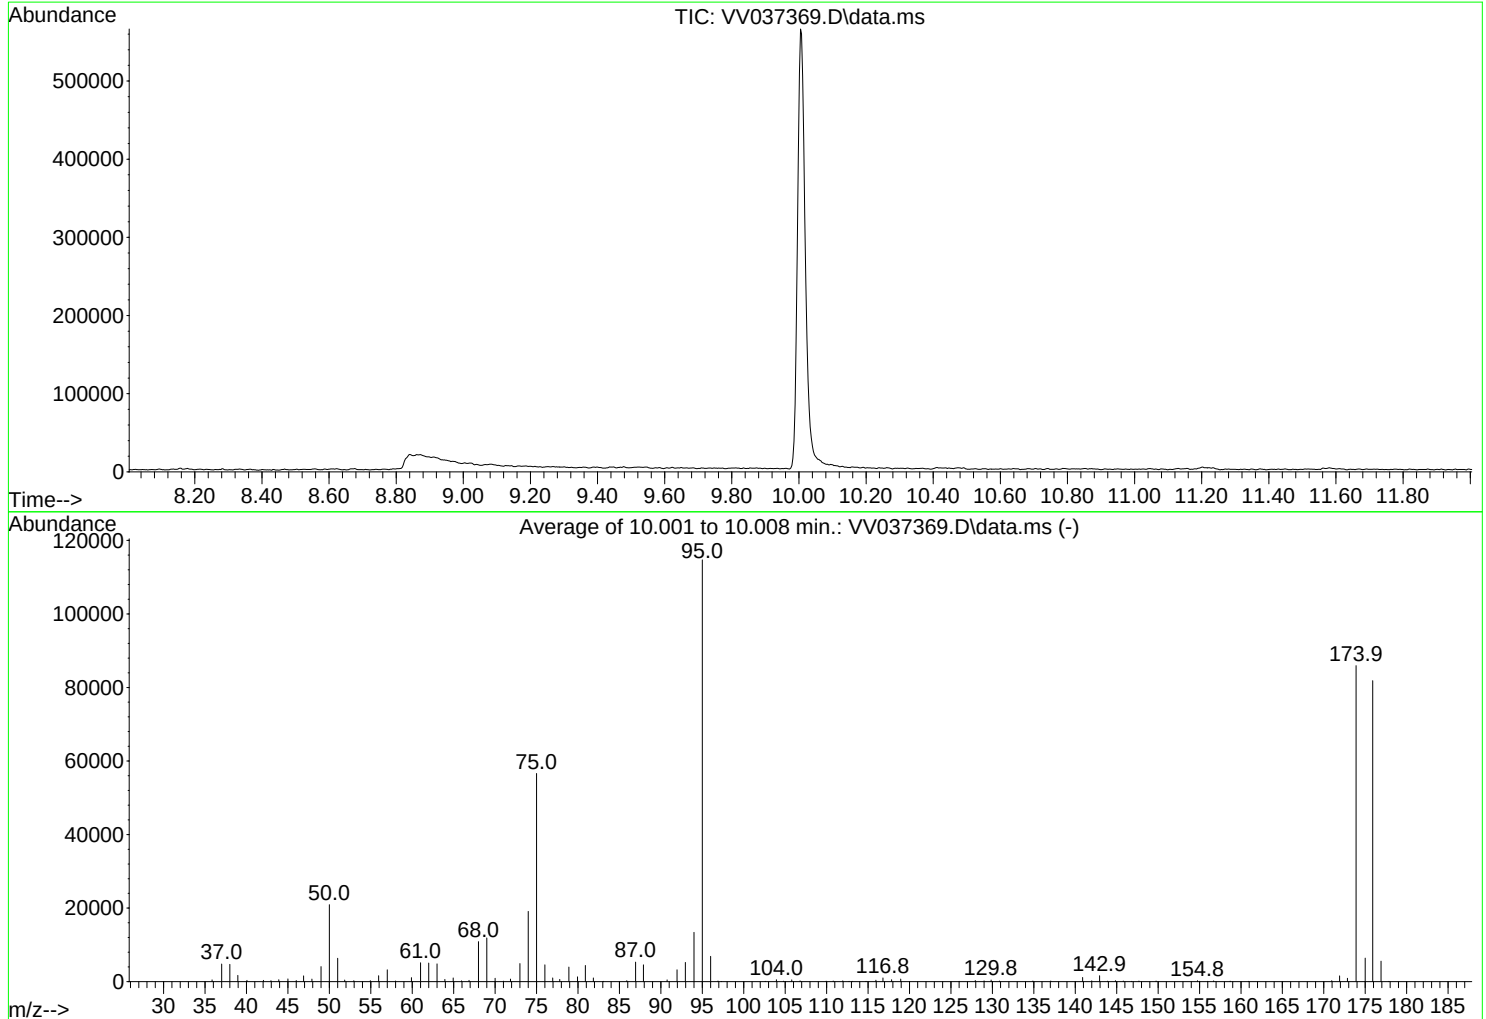

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	20915	PASS
75	95	30	80	49.4	56616	PASS
95	95	100	100	100.0	114715	PASS
96	95	5	9	6.0	6898	PASS
173	174	0.00	2	1.1	930	PASS
174	95	50	120	74.9	85963	PASS
175	174	5	9	7.5	6405	PASS
176	174	95	105	95.2	81853	PASS
177	176	5	10	6.8	5562	PASS

m/z	Abundance
35.90	157.0
37.00	155.0
38.90	364.0
39.80	396.0
41.00	265.0
41.80	328.0
42.70	129.0
43.90	838.0
44.80	147.0
45.00	147.0
54.00	116.0
55.10	150.0
59.90	638.0
64.00	129.0
72.80	256.0

Instrument :
MSVOA_V
ClientSampleId :
BFB276

m/z	Abundance
35.90	672.0
37.00	4660.0
38.00	4327.0
39.00	2140.0
40.00	403.0
41.00	223.0
42.10	326.0
42.90	285.0
43.90	1399.0
45.00	921.0
46.00	340.0
46.90	1702.0
47.90	532.0
49.00	3912.0
50.00	20048.0
51.00	5952.0
51.90	368.0
53.00	232.0
54.90	441.0
55.90	1394.0
57.00	3166.0
58.00	144.0
60.00	1523.0
61.00	4771.0
62.00	4978.0
63.00	4644.0
63.90	623.0
64.90	973.0
66.00	187.0
66.90	379.0
68.00	10303.0
69.00	11123.0
70.00	877.0
71.80	597.0
73.00	4821.0
74.00	18296.0
75.00	54616.0
76.00	4113.0
77.00	964.0
77.80	661.0
78.90	3653.0
80.00	1239.0
80.90	4073.0
81.80	956.0
85.90	216.0
87.00	4872.0
87.90	4343.0
90.80	592.0
91.90	2864.0
93.00	4906.0
94.00	12795.0
95.00	107312.0
96.00	6769.0
96.80	150.0
97.30	112.0
103.90	528.0
104.80	228.0
105.90	491.0
106.80	230.0
110.00	132.0
110.80	186.0
111.90	170.0
113.10	151.0
114.80	101.0
116.00	313.0
116.80	877.0
117.90	499.0
119.00	625.0
126.00	142.0
127.90	305.0
129.00	224.0
129.80	419.0
130.80	175.0
134.90	164.0
137.00	141.0
140.90	1168.0
142.00	196.0
142.90	1505.0
144.00	108.0
144.80	272.0
145.80	211.0
147.70	161.0
149.70	170.0
154.80	205.0
156.70	151.0
160.90	176.0
171.00	200.0
171.90	1540.0
172.80	818.0
173.90	78504.0
175.00	5945.0
175.90	74512.0

Instrument :
MSVOA_V
ClientSampleId :
BFB276

176.904935.0

177.90118.0

Instrument :

MSVOA_V

ClientSampleId :

BFB276

m/z	Abundance
35.90	657.0
37.00	5186.0
38.00	4926.0
39.00	2091.0
40.00	346.0
40.90	214.0
42.00	392.0
43.00	253.0
44.00	1355.0
45.10	869.0
46.00	345.0
46.90	1630.0
47.90	709.0
49.00	4213.0
50.00	21768.0
51.00	6626.0
51.90	437.0
53.00	299.0
54.90	442.0
55.90	1590.0
57.00	3436.0
58.00	155.0
60.00	1771.0
61.00	5330.0
62.00	5227.0
63.00	5000.0
64.00	750.0
64.90	1007.0
65.90	230.0
66.80	378.0
68.00	11314.0
69.00	12438.0
70.00	984.0
71.00	153.0
71.80	689.0
73.00	5095.0
74.00	19704.0
75.00	58312.0
76.00	4770.0
76.90	1049.0
77.80	630.0
78.90	4082.0
79.90	1339.0
80.90	4615.0
81.80	1019.0
83.00	127.0
85.90	300.0
86.90	5503.0
87.90	4721.0
90.70	542.0
92.00	3369.0
92.90	5453.0
94.00	14039.0
95.00	119264.0
96.00	7040.0
96.90	170.0
102.60	128.0
103.90	536.0
104.80	207.0
105.80	515.0
106.80	229.0
109.90	149.0
110.80	196.0
111.90	231.0
112.70	115.0
113.10	130.0
114.70	120.0
115.90	390.0
116.80	1036.0
117.80	522.0
118.90	697.0
126.00	129.0
128.00	309.0
129.00	246.0
129.80	454.0
130.90	165.0
134.90	201.0
137.10	204.0
140.90	1182.0
142.00	242.0
143.00	1674.0
143.90	139.0
144.90	271.0
145.80	193.0
146.80	117.0
147.70	198.0
149.70	174.0
154.70	251.0
155.00	251.0
156.00	141.0
156.70	243.0
158.70	178.0

Instrument :
MSVOA_V
ClientSampleId :
BFB276

160.90	135.0
170.90	259.0
171.90	1634.0
172.90	969.0
173.90	89288.0
175.00	6655.0
175.90	85160.0
176.90	5767.0
177.80	138.0

Instrument :
MSVOA_V
ClientSampleId :
BFB276

m/z	Abundance
35.90	620.0
37.00	4976.0
38.00	4881.0
39.00	2010.0
40.10	356.0
40.90	231.0
42.00	365.0
43.00	231.0
44.00	1304.0
45.10	833.0
46.00	275.0
46.90	1395.0
47.90	847.0
49.00	4168.0
50.00	20928.0
51.00	6504.0
51.80	497.0
52.90	293.0
54.90	412.0
56.00	1804.0
57.00	3069.0
58.00	189.0
59.90	1826.0
61.00	5307.0
62.00	4975.0
63.00	4865.0
64.00	862.0
65.00	1071.0
65.90	211.0
66.80	308.0
68.00	11066.0
69.00	12122.0
70.00	888.0
71.00	186.0
71.90	800.0
73.00	4889.0
74.00	19352.0
75.00	56920.0
76.00	4886.0
76.90	1015.0
77.80	540.0
78.90	4095.0
79.90	1296.0
80.90	4527.0
81.90	987.0
83.10	167.0
85.90	319.0
86.90	5610.0
87.90	4690.0
90.70	366.0
92.00	3482.0
92.90	5299.0
94.00	13423.0
95.00	117568.0
96.00	6885.0
97.00	211.0
102.60	133.0
104.00	522.0
105.00	162.0
105.70	468.0
106.80	191.0
109.90	169.0
110.80	140.0
112.00	222.0
112.70	114.0
114.70	112.0
115.90	441.0
116.80	1041.0
117.80	514.0
118.90	714.0
127.90	332.0
129.00	255.0
129.90	471.0
130.90	159.0
134.90	201.0
137.10	228.0
140.90	1018.0
142.00	265.0
143.00	1667.0
143.80	175.0
144.90	283.0
145.80	177.0
146.80	165.0
147.70	229.0
149.80	128.0
154.70	312.0
156.00	164.0
156.70	257.0
158.70	221.0
170.90	287.0
171.90	1585.0
172.90	1002.0

Instrument :
MSVOA_V
ClientSampleId :
BFB276

173.90	90096.0
175.00	6615.0
175.90	85888.0
176.90	5984.0

Instrument :
MSVOA_V
ClientSampleId :
BFB276