

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092018\
 Data File : VV007656.D
 Acq On : 20 Sep 2018 15:26
 Operator : SY/MD
 Sample : J4900-14
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A3ZA9

Quant Time: Sep 21 02:24:41 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 21 01:37:43 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	98225	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	91193	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	48586	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	20093	4.98	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.60%
7) Chloroethane-d5	1.59	69	20022	5.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.60%
11) 1,1-Dichloroethene-d2	2.13	63	37405	3.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.80%
20) 2-Butanone-d5	3.97	46	56560	54.92	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.84%
24) Chloroform-d	4.41	84	49573	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.00%
26) 1,2-Dichloroethane-d4	5.09	65	25449	5.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.00%
32) Benzene-d6	5.10	84	94791	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.80%
36) 1,2-Dichloropropane-d6	6.12	67	27841	5.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.40%
41) Toluene-d8	7.36	98	93962	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.80%
43) trans-1,3-Dichloropropene-	7.67	79	10568	4.93	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.60%
46) 2-Hexanone-d5	8.14	63	40822	48.85	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.70%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22413	5.07	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	43311	5.40	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.00%


Target Compounds					Ovalue
13) Acetone	2.22	43	3101	3.126 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092018\
Data File : VV007656.D
Acq On : 20 Sep 2018 15:26
Operator : SY/MD
Sample : J4900-14
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A3ZA9

Quant Time: Sep 21 02:24:41 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 21 01:37:43 2018
Response via : Initial Calibration

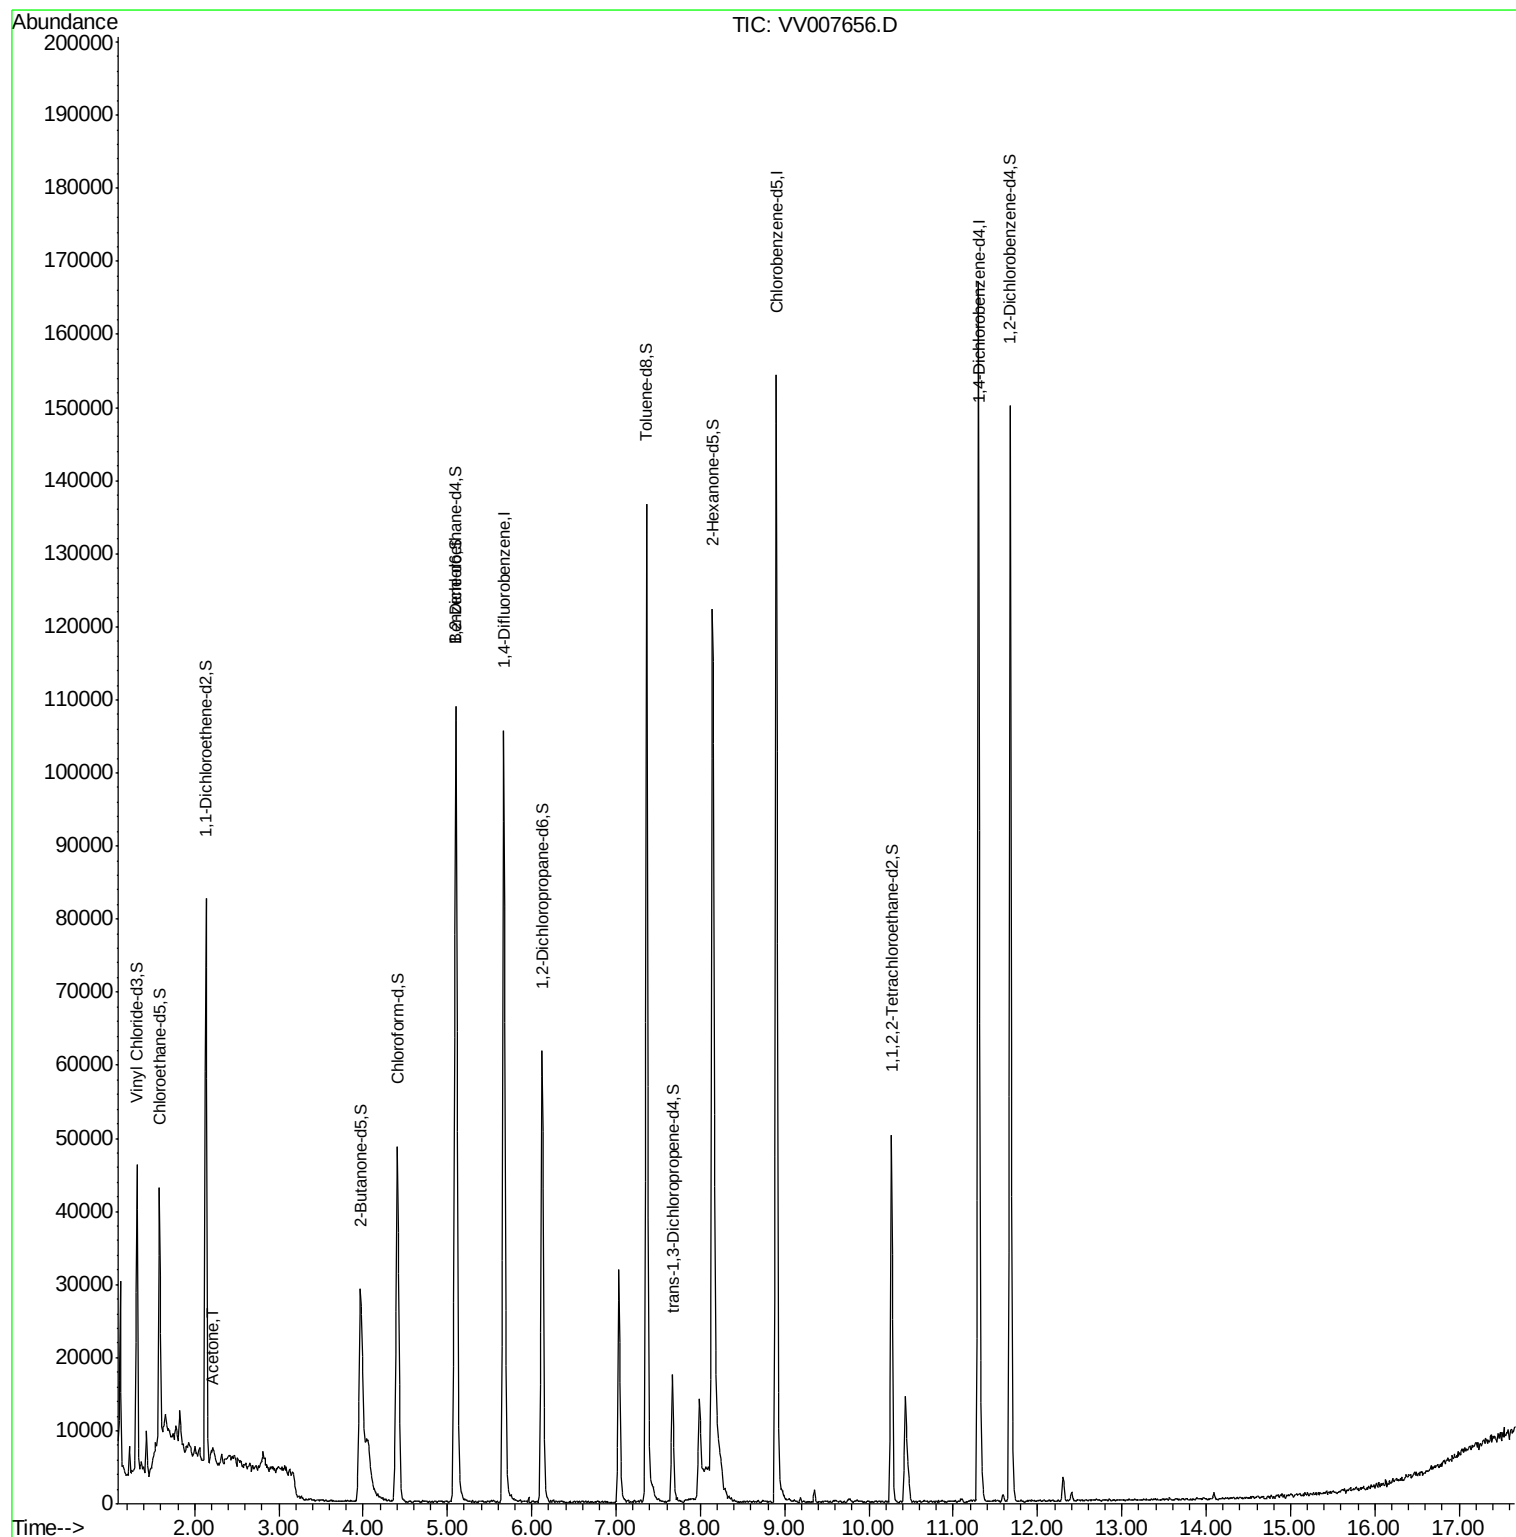

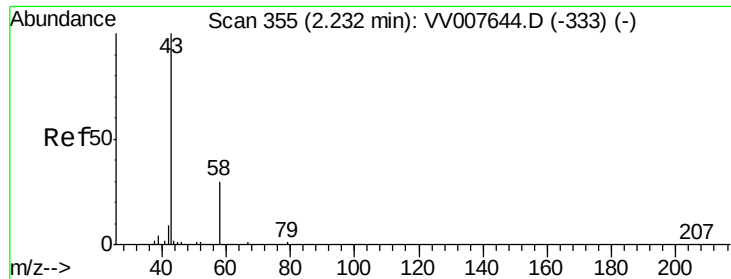

#13

Acetone

Concen: 3.126 ug/L

RT: 2.22 min Scan# 350

Delta R.T. -0.02 min

Lab File: VV007656.D

Acq: 20 Sep 2018 15:26

Instrument :
MSVOA_V
ClientSampleId :
A3ZA9

Tot Ion: 43 Resp: 3101

Ion Ratio Lower Upper

43 100

58 35.3 0.0 63.6

