

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092018\
 Data File : VV007658.D
 Acq On : 20 Sep 2018 16:21
 Operator : SY/MD
 Sample : J4900-16
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A3ZE1

Quant Time: Sep 21 02:29:35 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 21 01:37:43 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	105222	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	99173	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	52809	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	19060	4.41	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.20%
7) Chloroethane-d5	1.59	69	20268	4.99	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.80%
11) 1,1-Dichloroethene-d2	2.14	63	37100	3.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.60%
20) 2-Butanone-d5	3.97	46	52678	47.75	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.50%
24) Chloroform-d	4.41	84	47910	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.80%
26) 1,2-Dichloroethane-d4	5.09	65	25154	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.80%
32) Benzene-d6	5.10	84	92382	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
36) 1,2-Dichloropropane-d6	6.12	67	28059	4.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.80%
41) Toluene-d8	7.36	98	93057	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.80%
43) trans-1,3-Dichloropropene-	7.67	79	10015	4.29	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.80%
46) 2-Hexanone-d5	8.14	63	36608	40.28	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.56%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21352	4.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	41796	4.79	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.80%


Target Compounds					Ovalue
9) Trichlorofluoromethane	1.77	101	6643	0.415 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092018\
Data File : VV007658.D
Acq On : 20 Sep 2018 16:21
Operator : SY/MD
Sample : J4900-16
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A3ZE1

Quant Time: Sep 21 02:29:35 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 21 01:37:43 2018
Response via : Initial Calibration

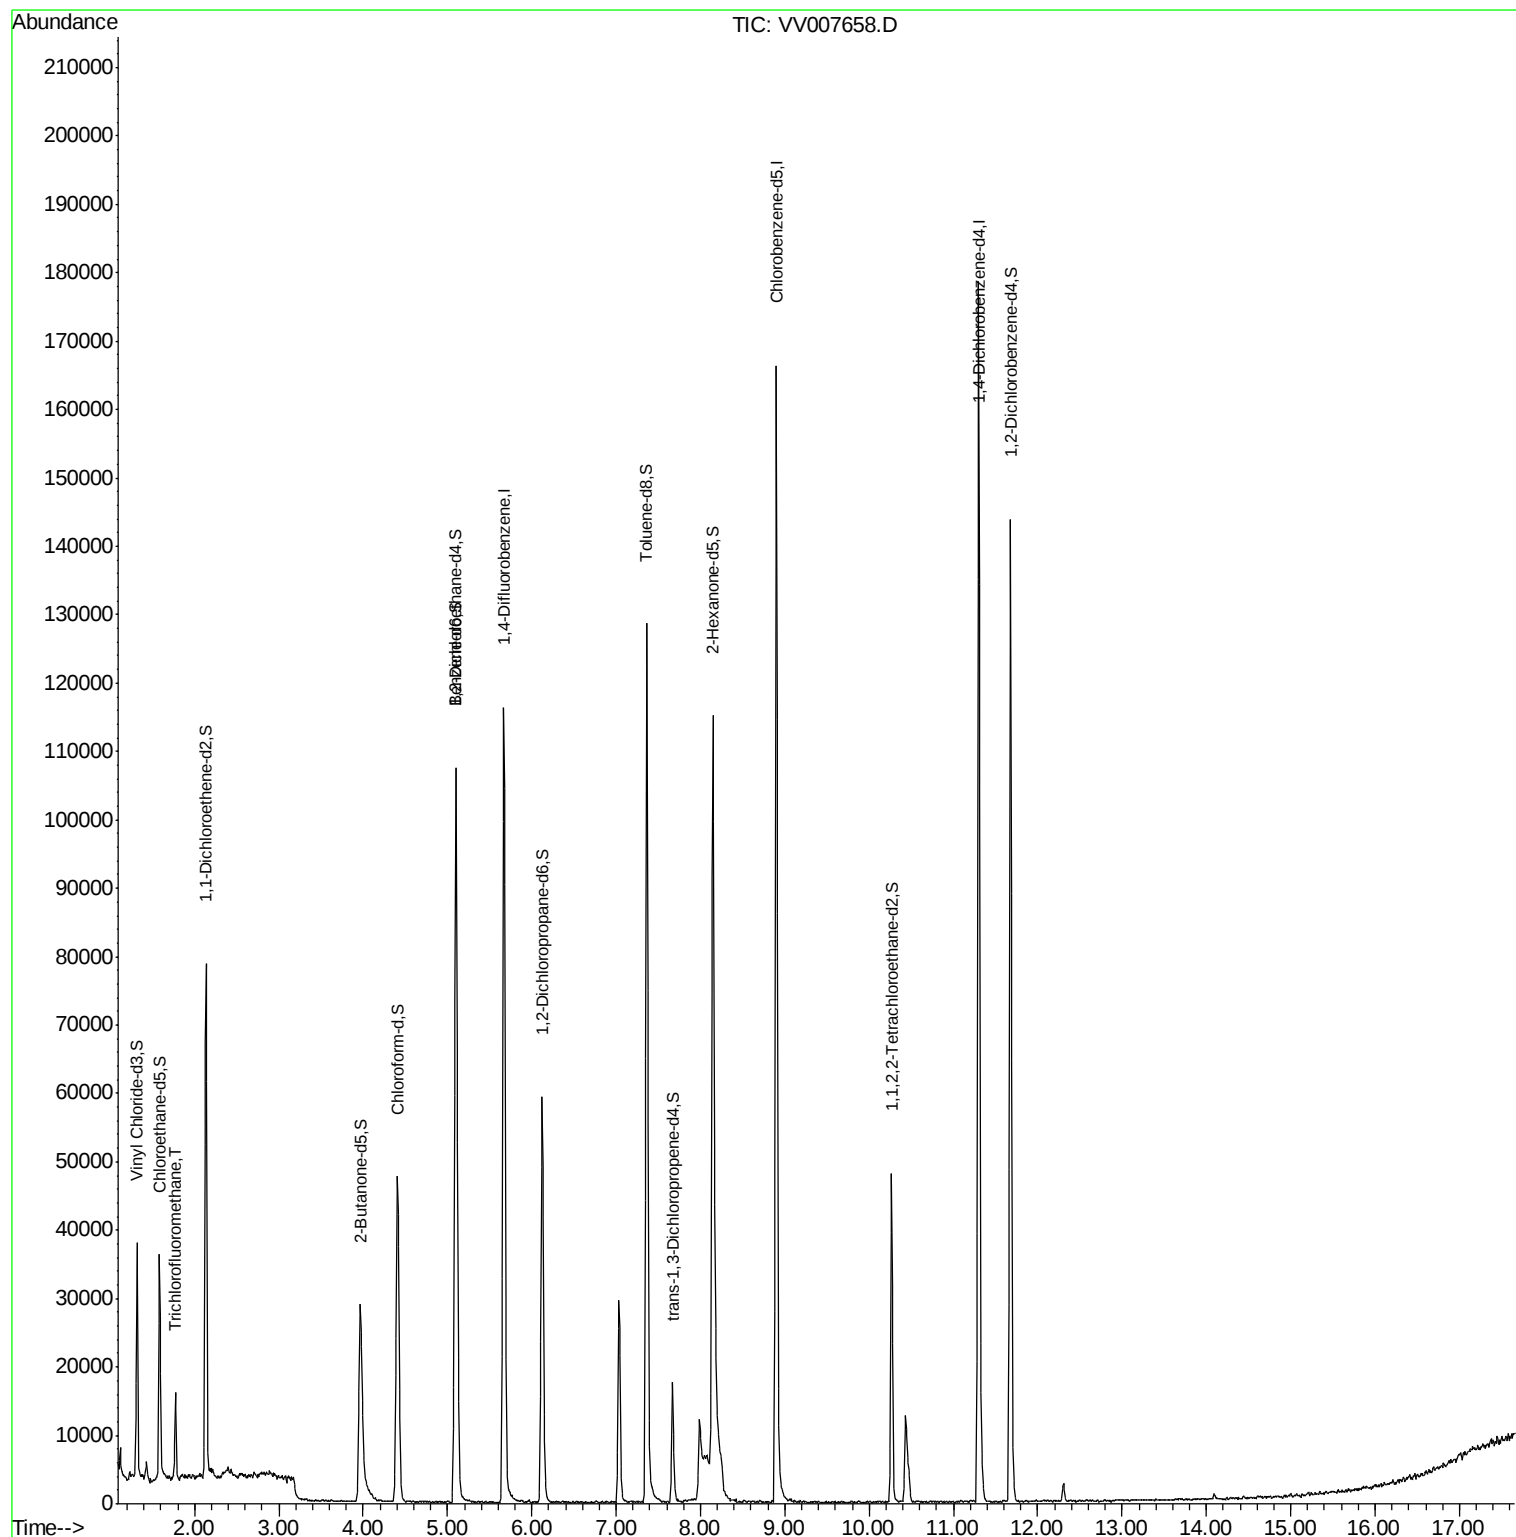

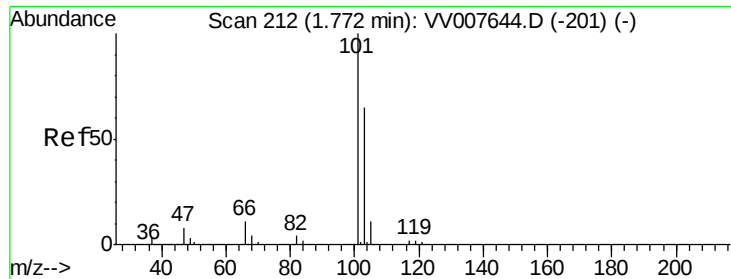

#9

Trichlorofluoromethane
 Concen: 0.415 ug/L
 RT: 1.77 min Scan# 212
 Delta R.T. -0.00 min
 Lab File: VV007658.D
 Acq: 20 Sep 2018 16:21

Instrument :
 MSVOA_V
 ClientSampleId :
 A3ZE1

Tot Ion:101 Resp: 6643
 Ion Ratio Lower Upper
 101 100
 103 64.9 51.9 77.9

