

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092018\
 Data File : VV007672.D
 Acq On : 20 Sep 2018 23:15
 Operator : SY/MD
 Sample : J4989-10
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ET0S2

Quant Time: Sep 21 03:50:01 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 21 03:27:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	111510	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	102268	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	54702	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	19053	4.16	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.20%
7) Chloroethane-d5	1.58	69	19446	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.40%
11) 1,1-Dichloroethene-d2	2.13	63	35877	2.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.00%#
20) 2-Butanone-d5	3.97	46	53403	45.68	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.36%
24) Chloroform-d	4.41	84	46229	4.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.60%
26) 1,2-Dichloroethane-d4	5.09	65	25195	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.20%
32) Benzene-d6	5.10	84	91309	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.00%
36) 1,2-Dichloropropane-d6	6.12	67	27240	4.55	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.00%
41) Toluene-d8	7.36	98	89913	4.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.00%
43) trans-1,3-Dichloropropene-	7.67	79	9394	3.90	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.00%
46) 2-Hexanone-d5	8.14	63	37527	40.04	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.08%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21142	4.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	40652	4.50	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.00%


Target Compounds					Ovalue
13) Acetone	2.22	43	18991	16.862 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092018\
Data File : VV007672.D
Acq On : 20 Sep 2018 23:15
Operator : SY/MD
Sample : J4989-10
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ET0S2

Quant Time: Sep 21 03:50:01 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 21 03:27:29 2018
Response via : Initial Calibration

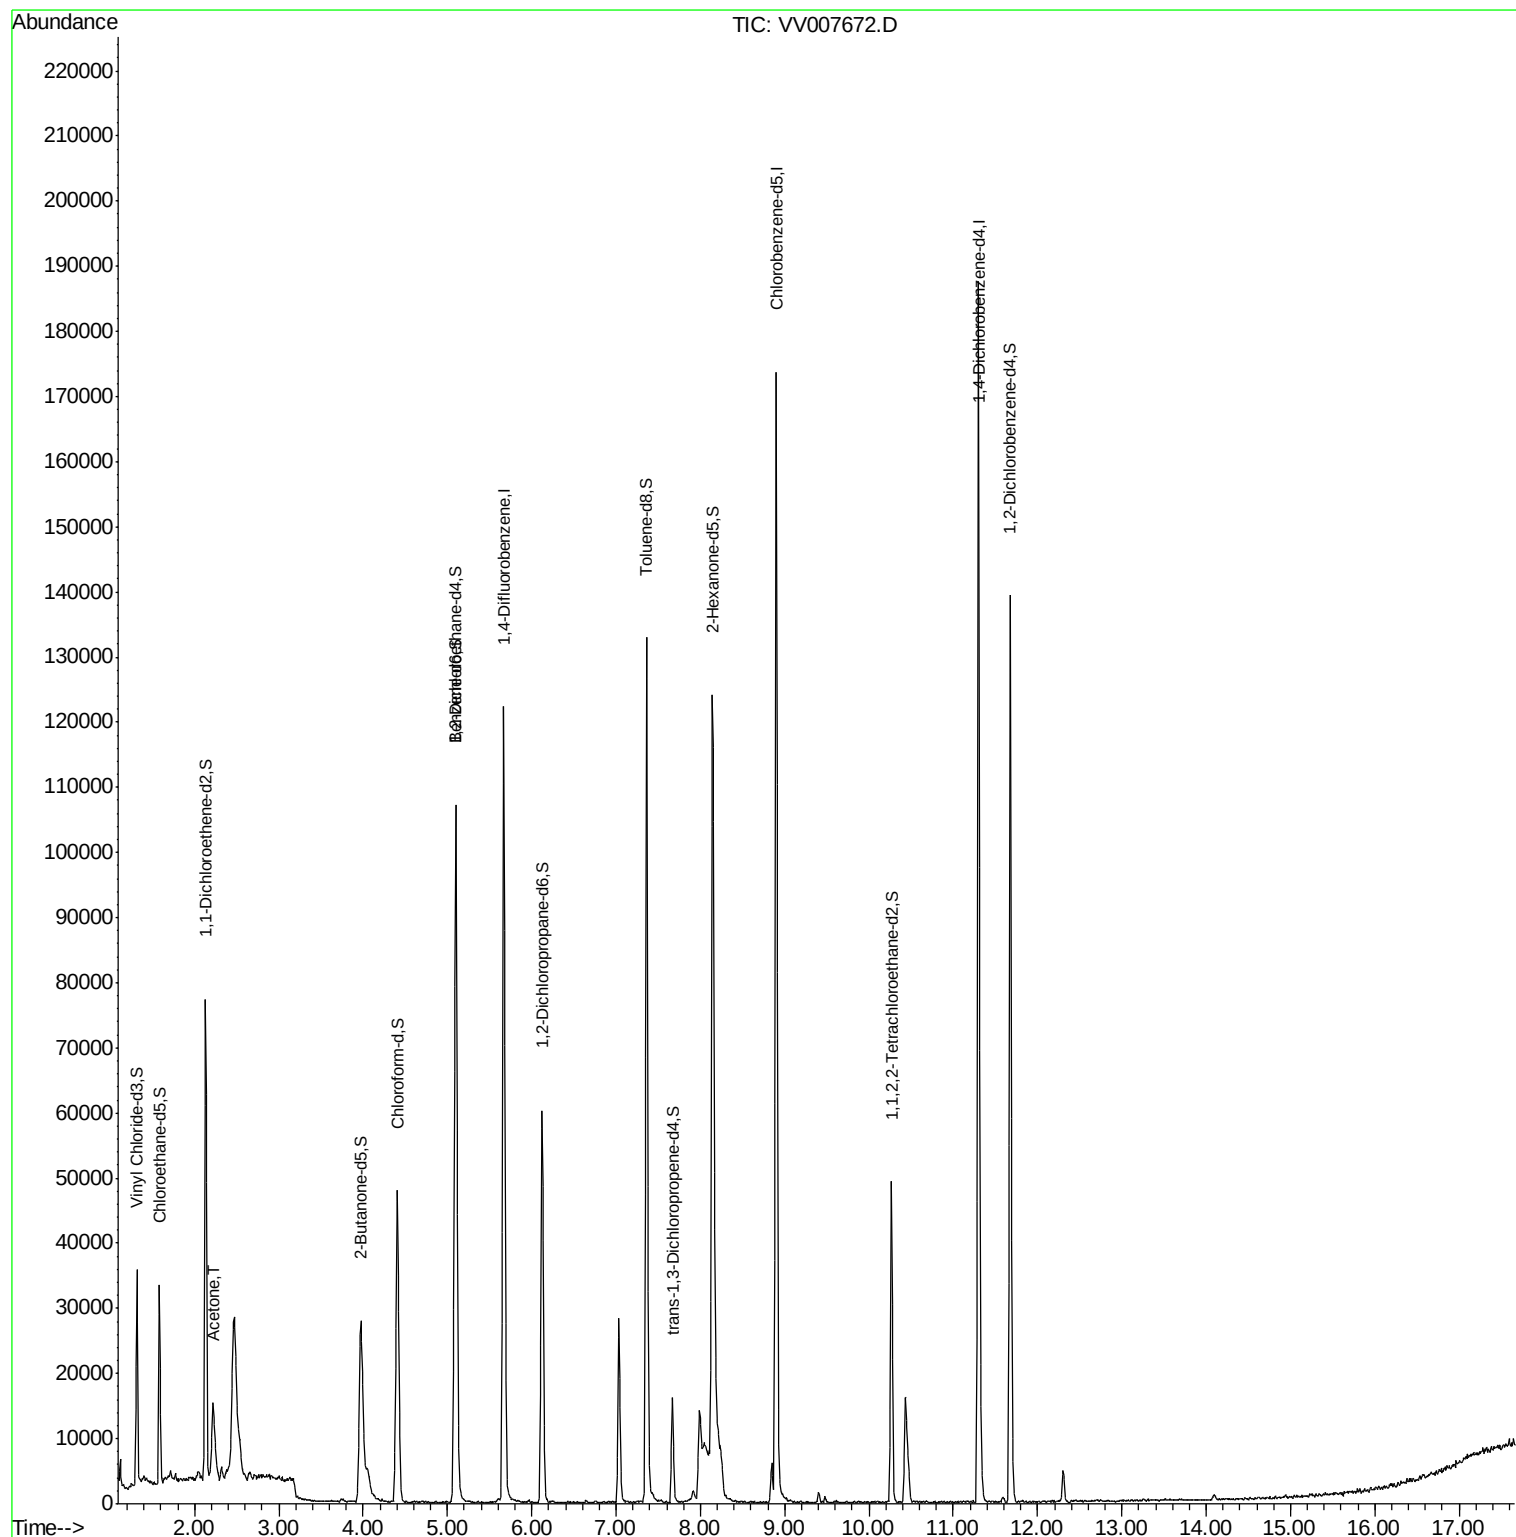

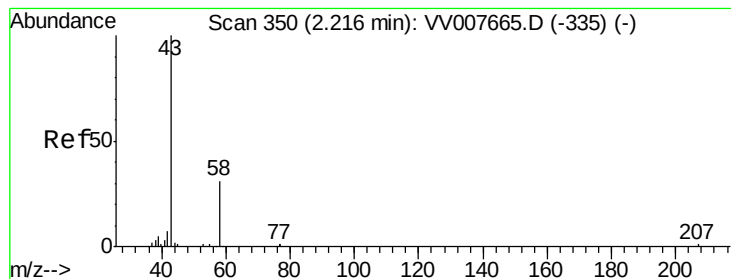

#13

Acetone

Concen: 16.862 ug/L

RT: 2.22 min Scan# 351

Delta R.T. 0.00 min

Lab File: VV007672.D

Acq: 20 Sep 2018 23:15

Instrument :
MSVOA_V
ClientSampleId :
ET0S2

Tot Ion: 43 Resp: 18991

Ion Ratio Lower Upper

43 100

58 31.9 0.0 63.6

