

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092018\
 Data File : VV007673.D
 Acq On : 20 Sep 2018 23:42
 Operator : SY/MD
 Sample : J4990-01
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0T02

Quant Time: Sep 21 03:52:43 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 21 03:27:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	105048	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	96538	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	51244	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	17531	4.06	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.20%
7) Chloroethane-d5	1.59	69	18755	4.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.40%
11) 1,1-Dichloroethene-d2	2.13	63	33890	2.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.20%#
20) 2-Butanone-d5	3.97	46	52244	47.43	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.86%
24) Chloroform-d	4.41	84	45206	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.80%
26) 1,2-Dichloroethane-d4	5.09	65	24514	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.40%
32) Benzene-d6	5.10	84	86399	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.20%
36) 1,2-Dichloropropane-d6	6.12	67	26372	4.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.40%
41) Toluene-d8	7.36	98	86914	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.00%
43) trans-1,3-Dichloropropene-	7.67	79	8920	3.93	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.60%
46) 2-Hexanone-d5	8.14	63	35727	40.38	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.76%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21097	4.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	39495	4.67	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.40%


Target Compounds					Ovalue
13) Acetone	2.22	43	15326	14.445 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092018\
Data File : VV007673.D
Acq On : 20 Sep 2018 23:42
Operator : SY/MD
Sample : J4990-01
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0T02

Quant Time: Sep 21 03:52:43 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 21 03:27:29 2018
Response via : Initial Calibration

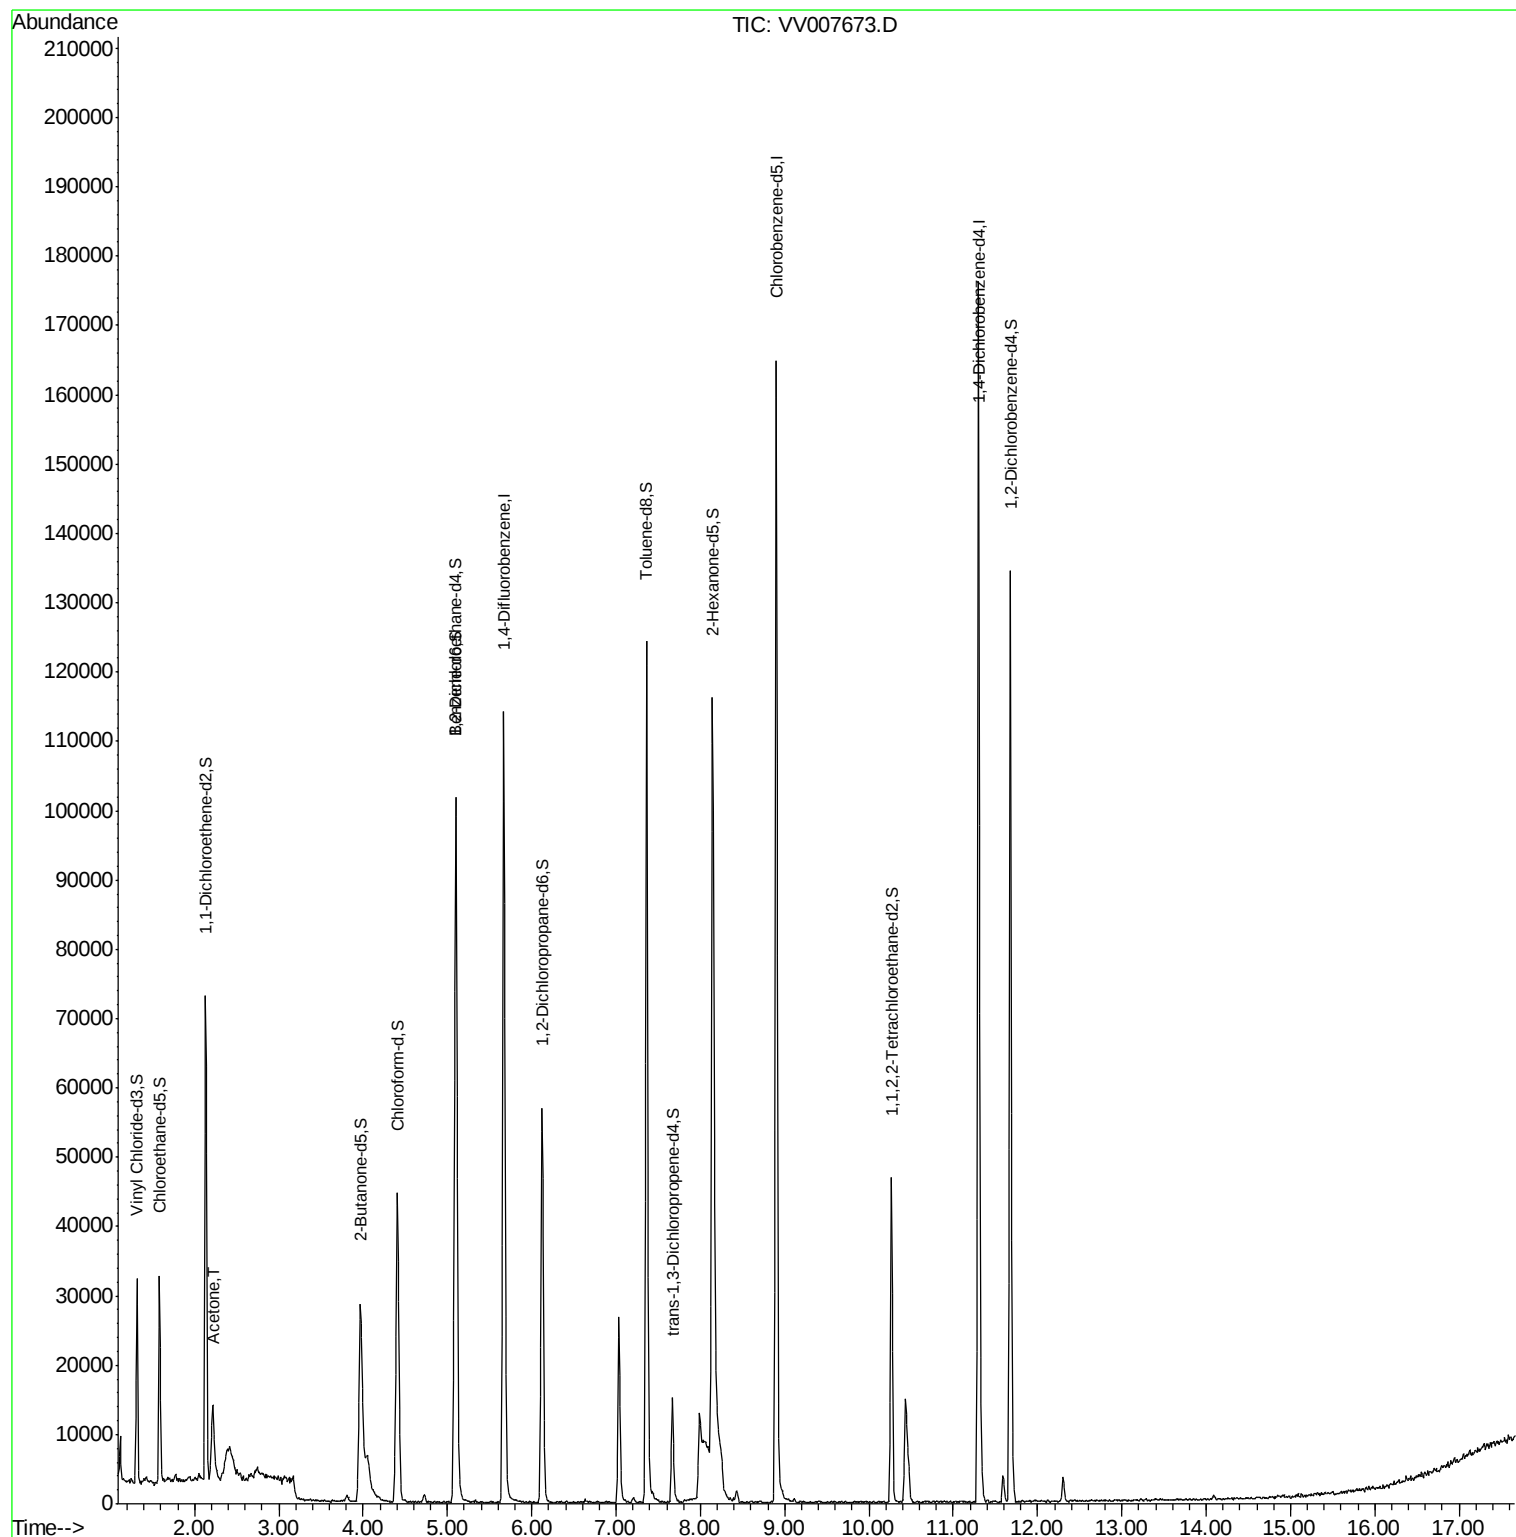

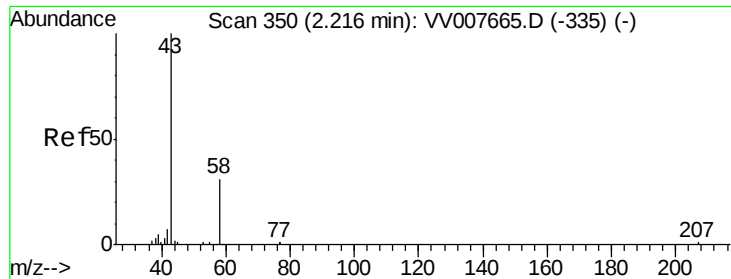

#13

Acetone

Concen: 14.445 ug/L

RT: 2.22 min Scan# 350

Delta R.T. 0.00 min

Lab File: VV007673.D

Acq: 20 Sep 2018 23:42

Instrument :

MSVOA_V

ClientSampleId :

C0T02

Tot Ion: 43 Resp: 15326

Ion Ratio Lower Upper

43 100

58 32.7 0.0 63.6

