

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092018\
 Data File : VV007675.D
 Acq On : 21 Sep 2018 00:37
 Operator : SY/MD
 Sample : J4990-03
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0T05

Quant Time: Sep 21 03:57:52 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 21 03:27:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	108883	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	98976	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	51443	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	18201	4.07	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.40%
7) Chloroethane-d5	1.58	69	19294	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.80%
11) 1,1-Dichloroethene-d2	2.13	63	33850	2.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.00%#
20) 2-Butanone-d5	3.96	46	52047	45.59	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.18%
24) Chloroform-d	4.41	84	46616	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.40%
26) 1,2-Dichloroethane-d4	5.09	65	23682	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.80%
32) Benzene-d6	5.10	84	88842	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.60%
36) 1,2-Dichloropropane-d6	6.12	67	25779	4.45	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.00%
41) Toluene-d8	7.36	98	87396	4.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.40%
43) trans-1,3-Dichloropropene-	7.67	79	9029	3.88	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.60%
46) 2-Hexanone-d5	8.14	63	37432	41.27	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.54%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	20518	4.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	39241	4.62	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	11499	10.456 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092018\
Data File : VV007675.D
Acq On : 21 Sep 2018 00:37
Operator : SY/MD
Sample : J4990-03
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0T05

Quant Time: Sep 21 03:57:52 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 21 03:27:29 2018
Response via : Initial Calibration

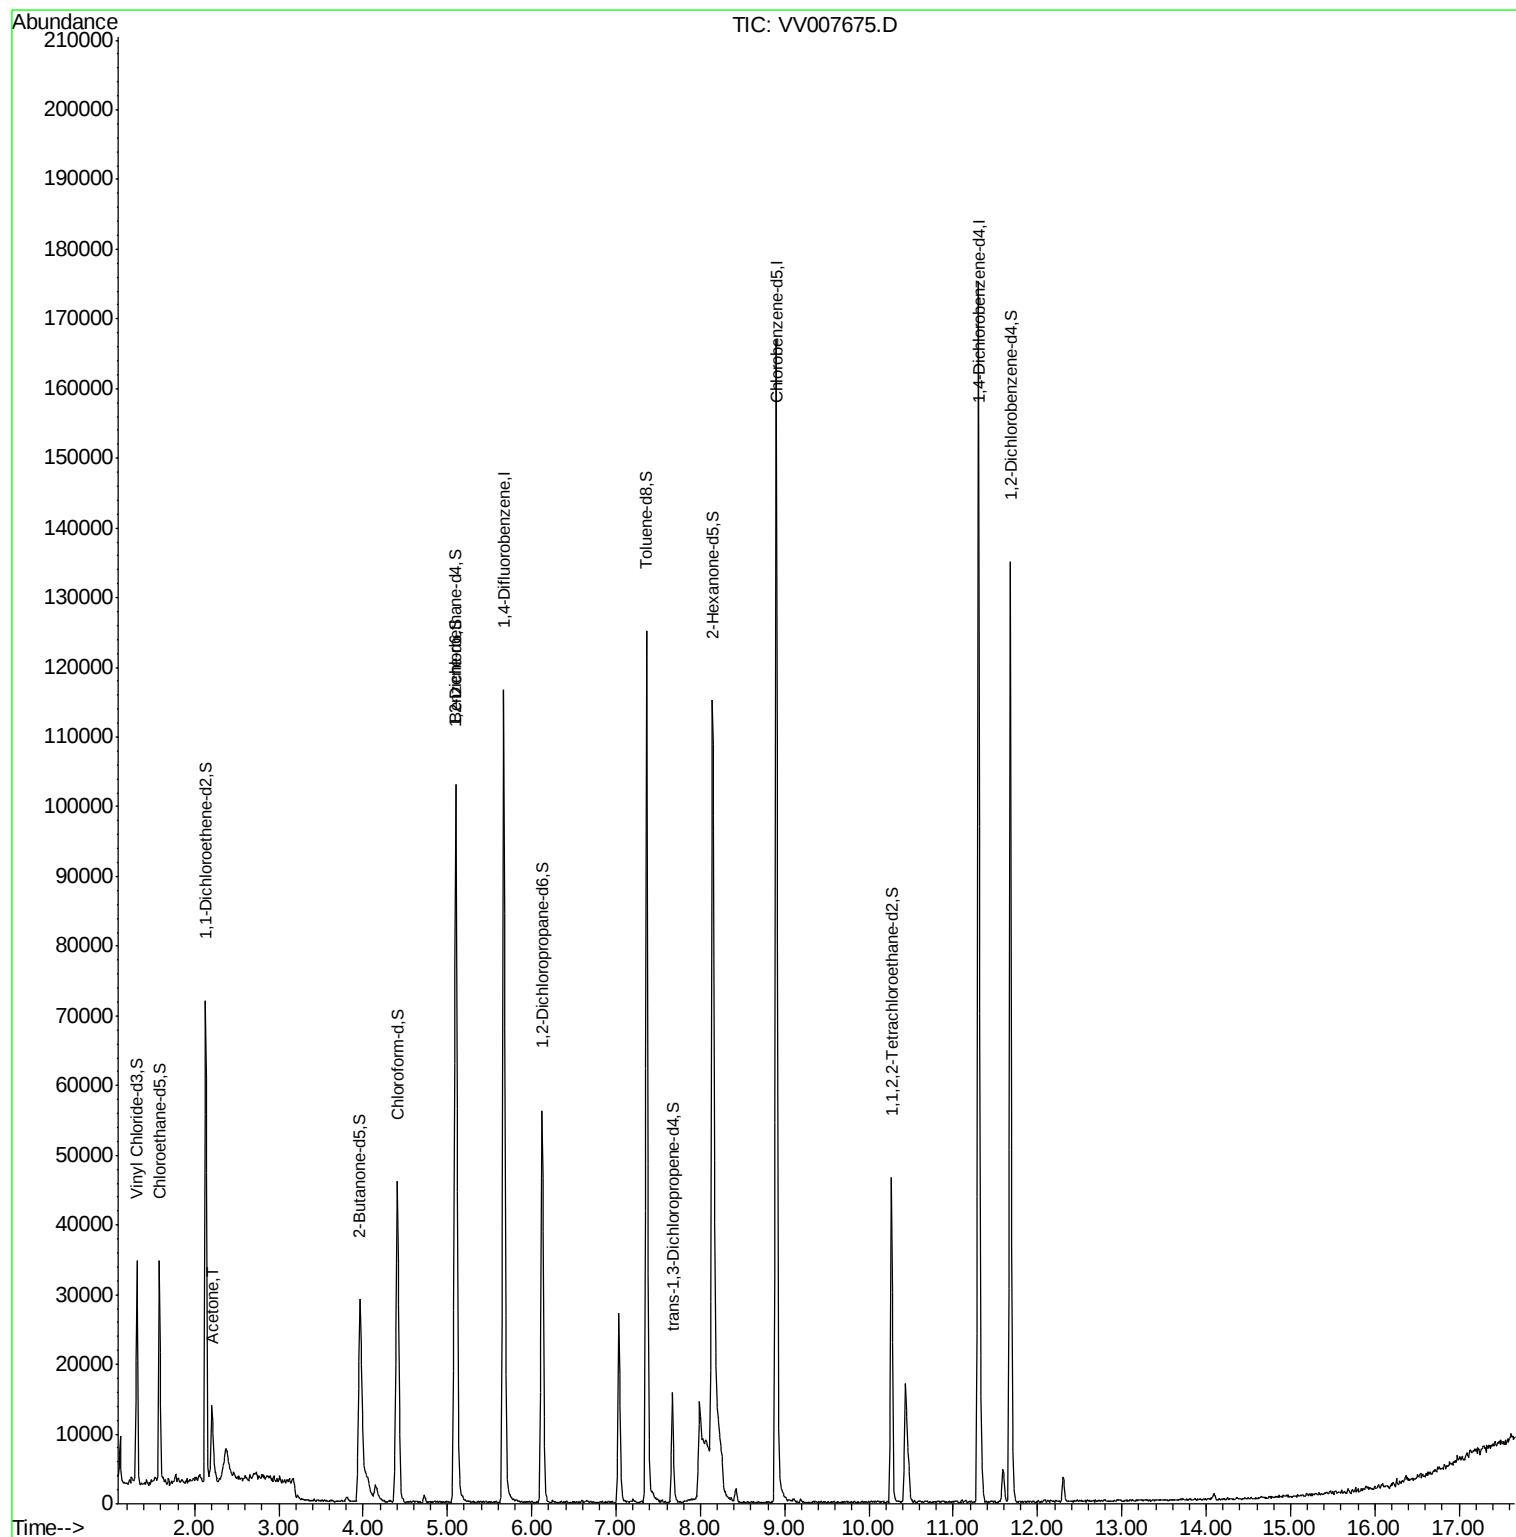

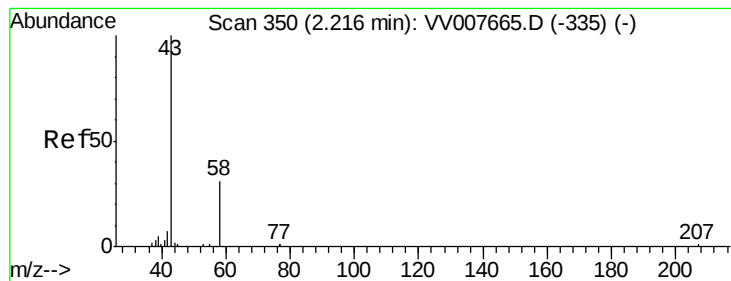

#13
 Acetone
 Concen: 10.456 ug/L
 RT: 2.21 min Scan# 347
 Delta R.T. -0.01 min
 Lab File: VV007675.D
 Acq: 21 Sep 2018 00:37

Instrument :
 MSVOA_V
 ClientSampleId :
 C0T05

Tot Ion: 43 Resp: 11499
 Ion Ratio Lower Upper
 43 100
 58 35.4 0.0 63.6

