

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092018\
 Data File : VV007677.D
 Acq On : 21 Sep 2018 01:32
 Operator : SY/MD
 Sample : J4990-05
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0T07

Quant Time: Sep 21 04:03:35 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 21 03:27:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	101975	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	94731	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	51664	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	17897	4.27	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.40%
7) Chloroethane-d5	1.58	69	18921	4.81	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.20%
11) 1,1-Dichloroethene-d2	2.13	63	33533	3.02	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.40%
20) 2-Butanone-d5	3.96	46	51680	48.34	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.68%
24) Chloroform-d	4.41	84	44878	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.80%
26) 1,2-Dichloroethane-d4	5.09	65	23976	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.00%
32) Benzene-d6	5.10	84	85155	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.60%
36) 1,2-Dichloropropane-d6	6.12	67	25659	4.63	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.60%
41) Toluene-d8	7.36	98	84695	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.40%
43) trans-1,3-Dichloropropene-	7.67	79	8434	3.78	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.60%
46) 2-Hexanone-d5	8.14	63	36885	42.49	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.98%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	19890	4.33	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	39115	4.59	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.80%


Target Compounds					Ovalue
13) Acetone	2.21	43	25473	24.732 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092018\
Data File : VV007677.D
Acq On : 21 Sep 2018 01:32
Operator : SY/MD
Sample : J4990-05
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0T07

Quant Time: Sep 21 04:03:35 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 21 03:27:29 2018
Response via : Initial Calibration

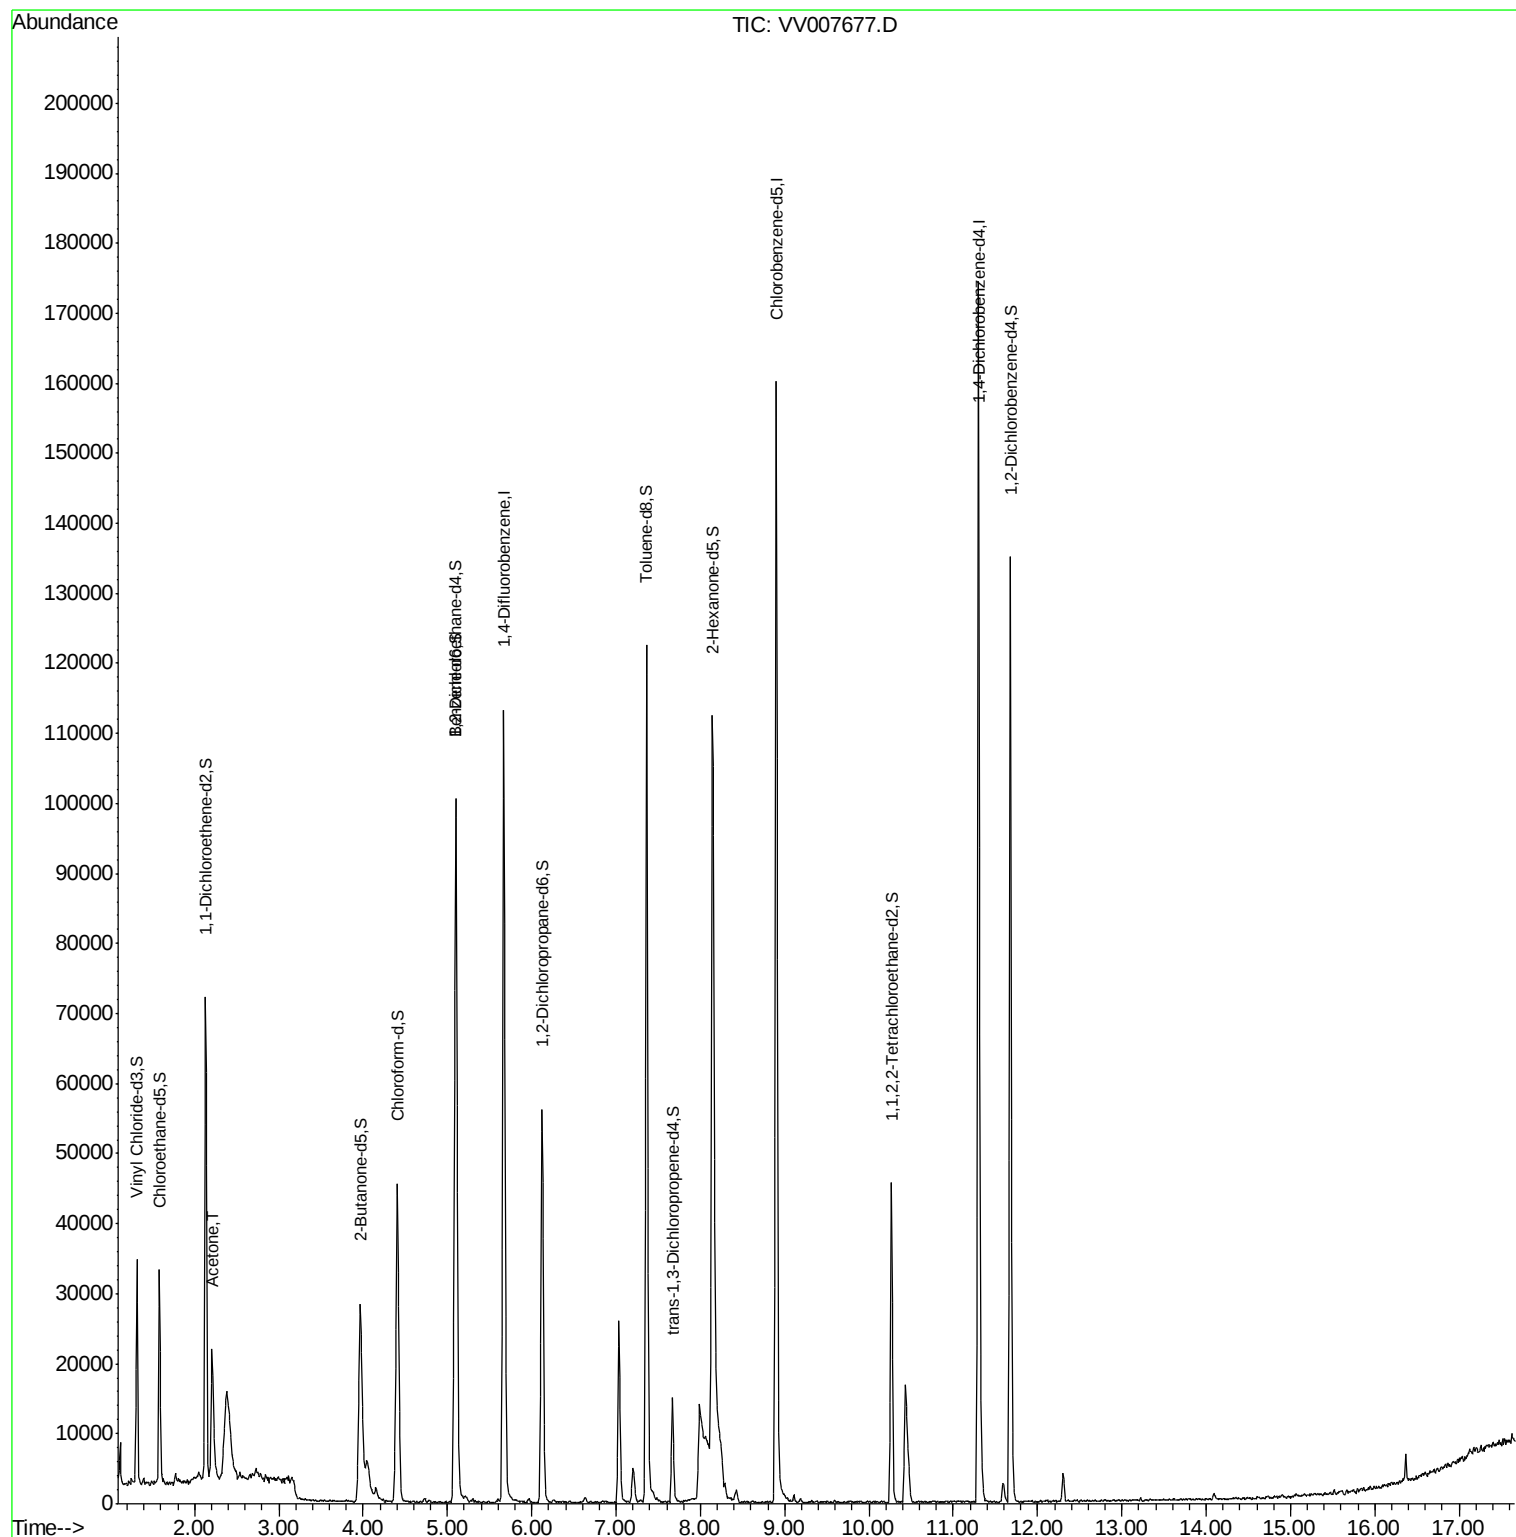

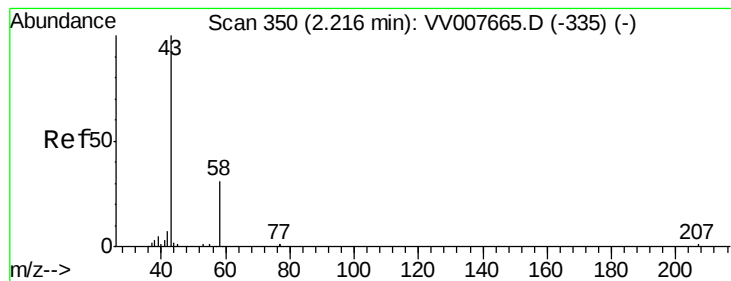

#13
 Acetone
 Concen: 24.732 ug/L
 RT: 2.21 min Scan# 348
 Delta R.T. -0.01 min
 Lab File: VV007677.D
 Acq: 21 Sep 2018 01:32

Instrument :
 MSVOA_V
 ClientSampleId :
 C0T07

Tot Ion: 43 Resp: 25473
 Ion Ratio Lower Upper
 43 100
 58 29.9 0.0 63.6

