

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092018\
 Data File : VV007678.D
 Acq On : 21 Sep 2018 02:00
 Operator : SY/MD
 Sample : J4990-06
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0T08

Quant Time: Sep 21 04:05:25 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 21 03:27:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	102751	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	93896	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	50662	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	18040	4.27	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.40%
7) Chloroethane-d5	1.59	69	19886	5.01	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.20%
11) 1,1-Dichloroethene-d2	2.13	63	34166	3.05	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.00%
20) 2-Butanone-d5	3.96	46	53260	49.44	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.88%
24) Chloroform-d	4.41	84	46893	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.00%
26) 1,2-Dichloroethane-d4	5.09	65	24371	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.00%
32) Benzene-d6	5.10	84	87944	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
36) 1,2-Dichloropropane-d6	6.12	67	27289	4.97	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.40%
41) Toluene-d8	7.36	98	88236	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.00%
43) trans-1,3-Dichloropropene-	7.67	79	8343	3.78	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.60%
46) 2-Hexanone-d5	8.14	63	38417	44.65	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.30%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22112	4.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	40804	4.88	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.60%


Target Compounds					Ovalue
13) Acetone	2.21	43	16927	16.310 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092018\
Data File : VV007678.D
Acq On : 21 Sep 2018 02:00
Operator : SY/MD
Sample : J4990-06
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0T08

Quant Time: Sep 21 04:05:25 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 21 03:27:29 2018
Response via : Initial Calibration

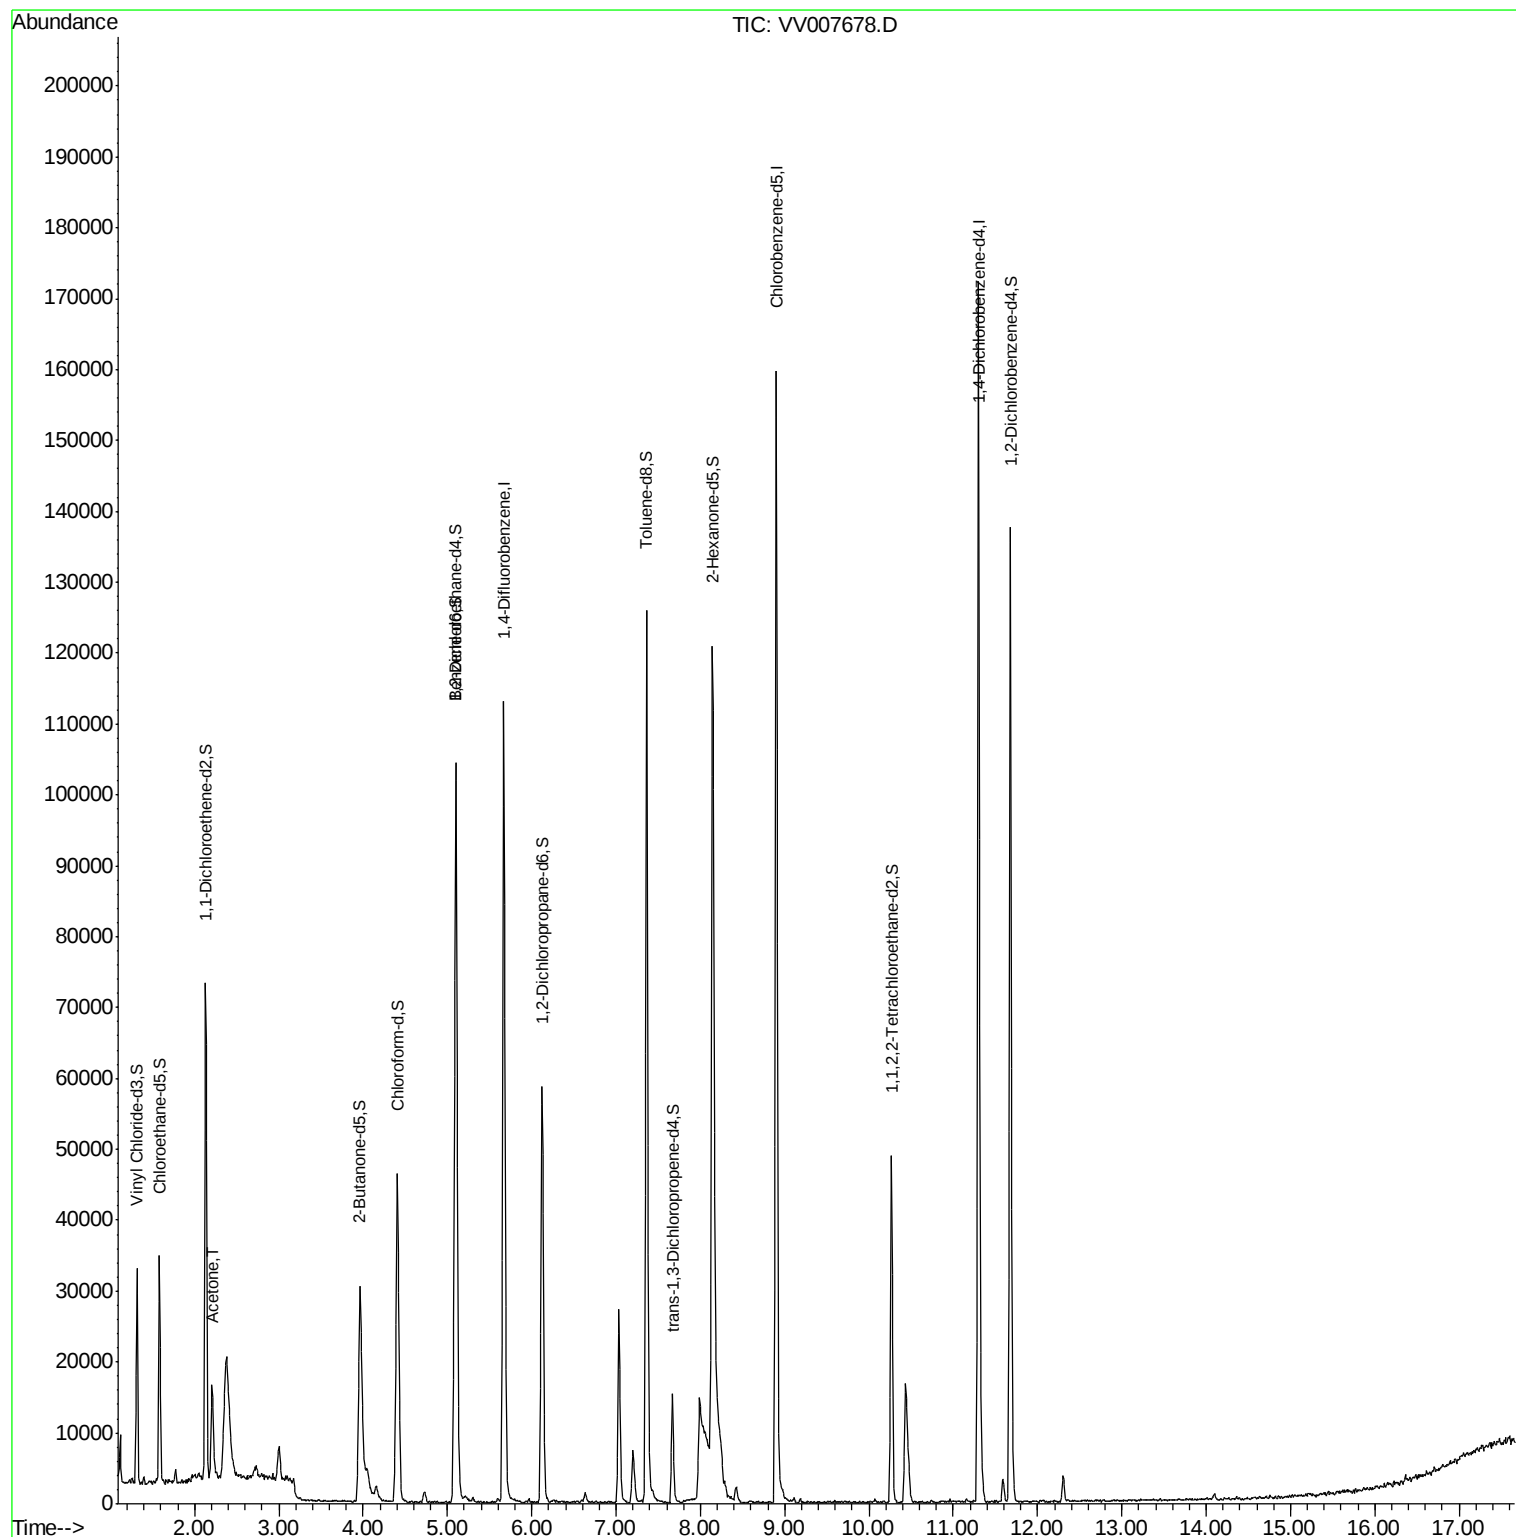

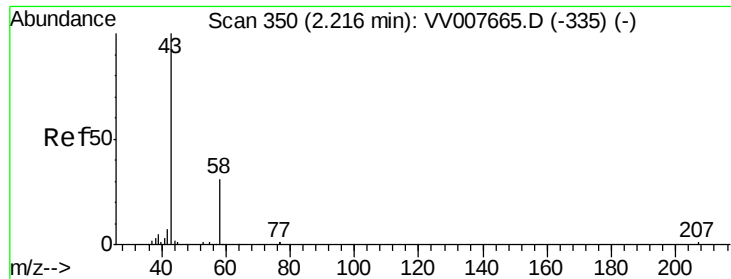

#13

Acetone

Concen: 16.310 ug/L

RT: 2.21 min Scan# 348

Delta R.T. -0.01 min

Lab File: VV007678.D

Acq: 21 Sep 2018 02:00

Instrument :
MSVOA_V
ClientSampleId :
C0T08

Tot Ion: 43 Resp: 16927

Ion Ratio Lower Upper

43 100

58 30.8 0.0 63.6

