

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092018\
 Data File : VV007679.D
 Acq On : 21 Sep 2018 02:27
 Operator : SY/MD
 Sample : J4990-07
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0T09

Quant Time: Sep 21 04:07:11 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 21 03:27:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	110504	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	101843	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	53379	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	18017	3.97	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.40%
7) Chloroethane-d5	1.59	69	20276	4.75	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.00%
11) 1,1-Dichloroethene-d2	2.13	63	34757	2.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.60%#
20) 2-Butanone-d5	3.96	46	53870	46.49	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.98%
24) Chloroform-d	4.41	84	47125	4.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.00%
26) 1,2-Dichloroethane-d4	5.09	65	24540	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
32) Benzene-d6	5.10	84	89209	4.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.40%
36) 1,2-Dichloropropane-d6	6.12	67	27050	4.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.80%
41) Toluene-d8	7.36	98	89451	4.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.00%
43) trans-1,3-Dichloropropene-	7.67	79	9248	3.86	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.20%
46) 2-Hexanone-d5	8.14	63	38399	41.14	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.28%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21505	4.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	40152	4.56	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	13001	11.648 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092018\
Data File : VV007679.D
Acq On : 21 Sep 2018 02:27
Operator : SY/MD
Sample : J4990-07
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0T09

Quant Time: Sep 21 04:07:11 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 21 03:27:29 2018
Response via : Initial Calibration

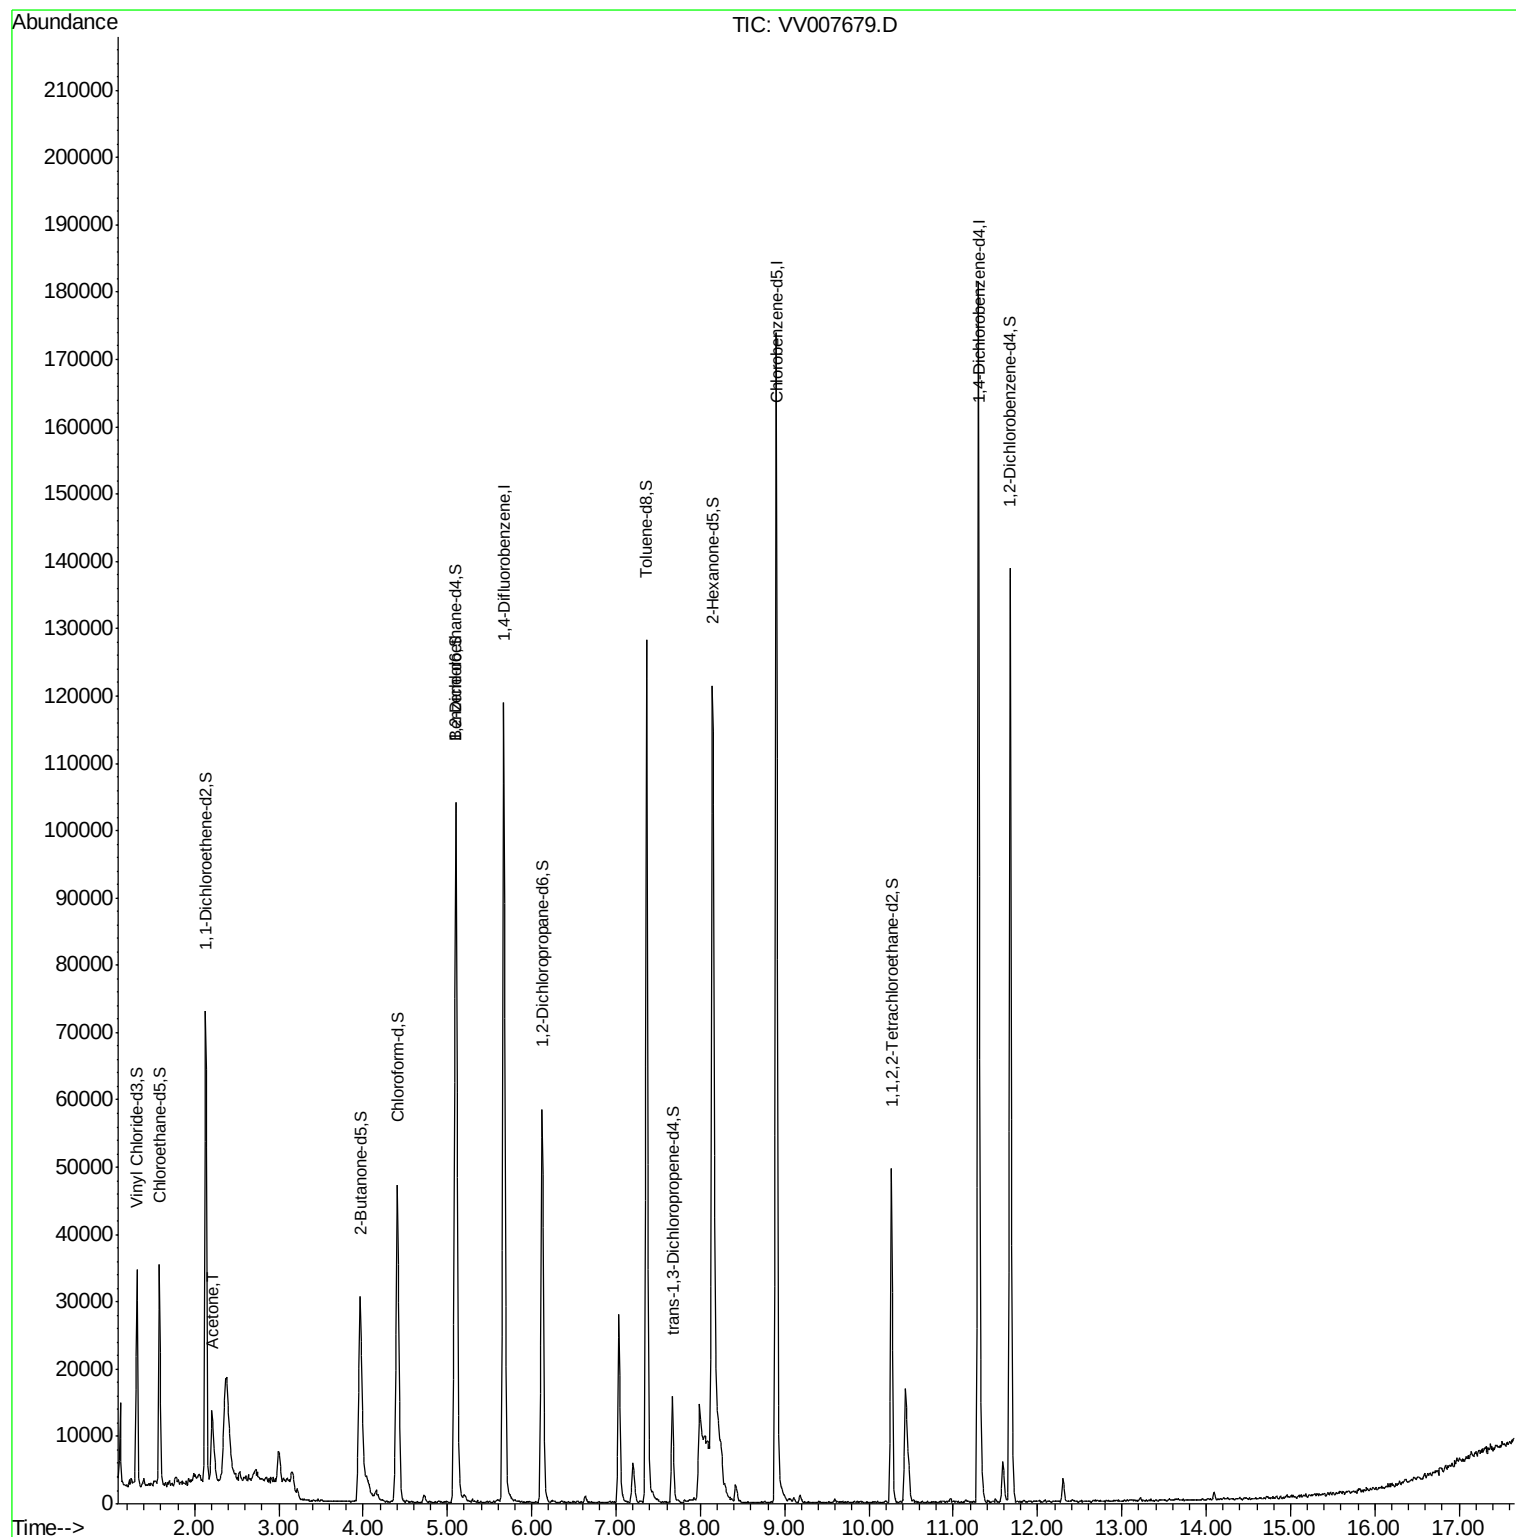

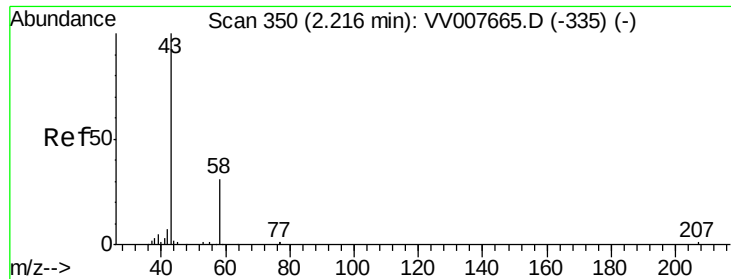

#13

Acetone

Concen: 11.648 ug/L

RT: 2.21 min Scan# 348

Delta R.T. -0.01 min

Lab File: VV007679.D

Acq: 21 Sep 2018 02:27

Instrument :

MSVOA_V

ClientSampleId :

C0T09

Tot Ion: 43 Resp: 13001

Ion Ratio Lower Upper

43 100

58 29.1 0.0 63.6

