

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092018\
 Data File : VV007680.D
 Acq On : 21 Sep 2018 02:55
 Operator : SY/MD
 Sample : J4990-08
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COT10

Quant Time: Sep 21 04:09:11 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 21 03:27:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	106777	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	98157	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	52193	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	17924	4.08	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.60%
7) Chloroethane-d5	1.59	69	20284	4.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.40%
11) 1,1-Dichloroethene-d2	2.13	63	34511	2.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.20%#
20) 2-Butanone-d5	3.96	46	53688	47.96	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.92%
24) Chloroform-d	4.41	84	47027	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.80%
26) 1,2-Dichloroethane-d4	5.09	65	24445	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
32) Benzene-d6	5.10	84	87949	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.40%
36) 1,2-Dichloropropane-d6	6.12	67	27024	4.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.20%
41) Toluene-d8	7.36	98	87196	4.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.00%
43) trans-1,3-Dichloropropene-	7.67	79	8921	3.86	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.20%
46) 2-Hexanone-d5	8.14	63	37819	42.04	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.08%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21513	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	40226	4.67	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	15185	14.080 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092018\
Data File : VV007680.D
Acq On : 21 Sep 2018 02:55
Operator : SY/MD
Sample : J4990-08
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0T10

Quant Time: Sep 21 04:09:11 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 21 03:27:29 2018
Response via : Initial Calibration

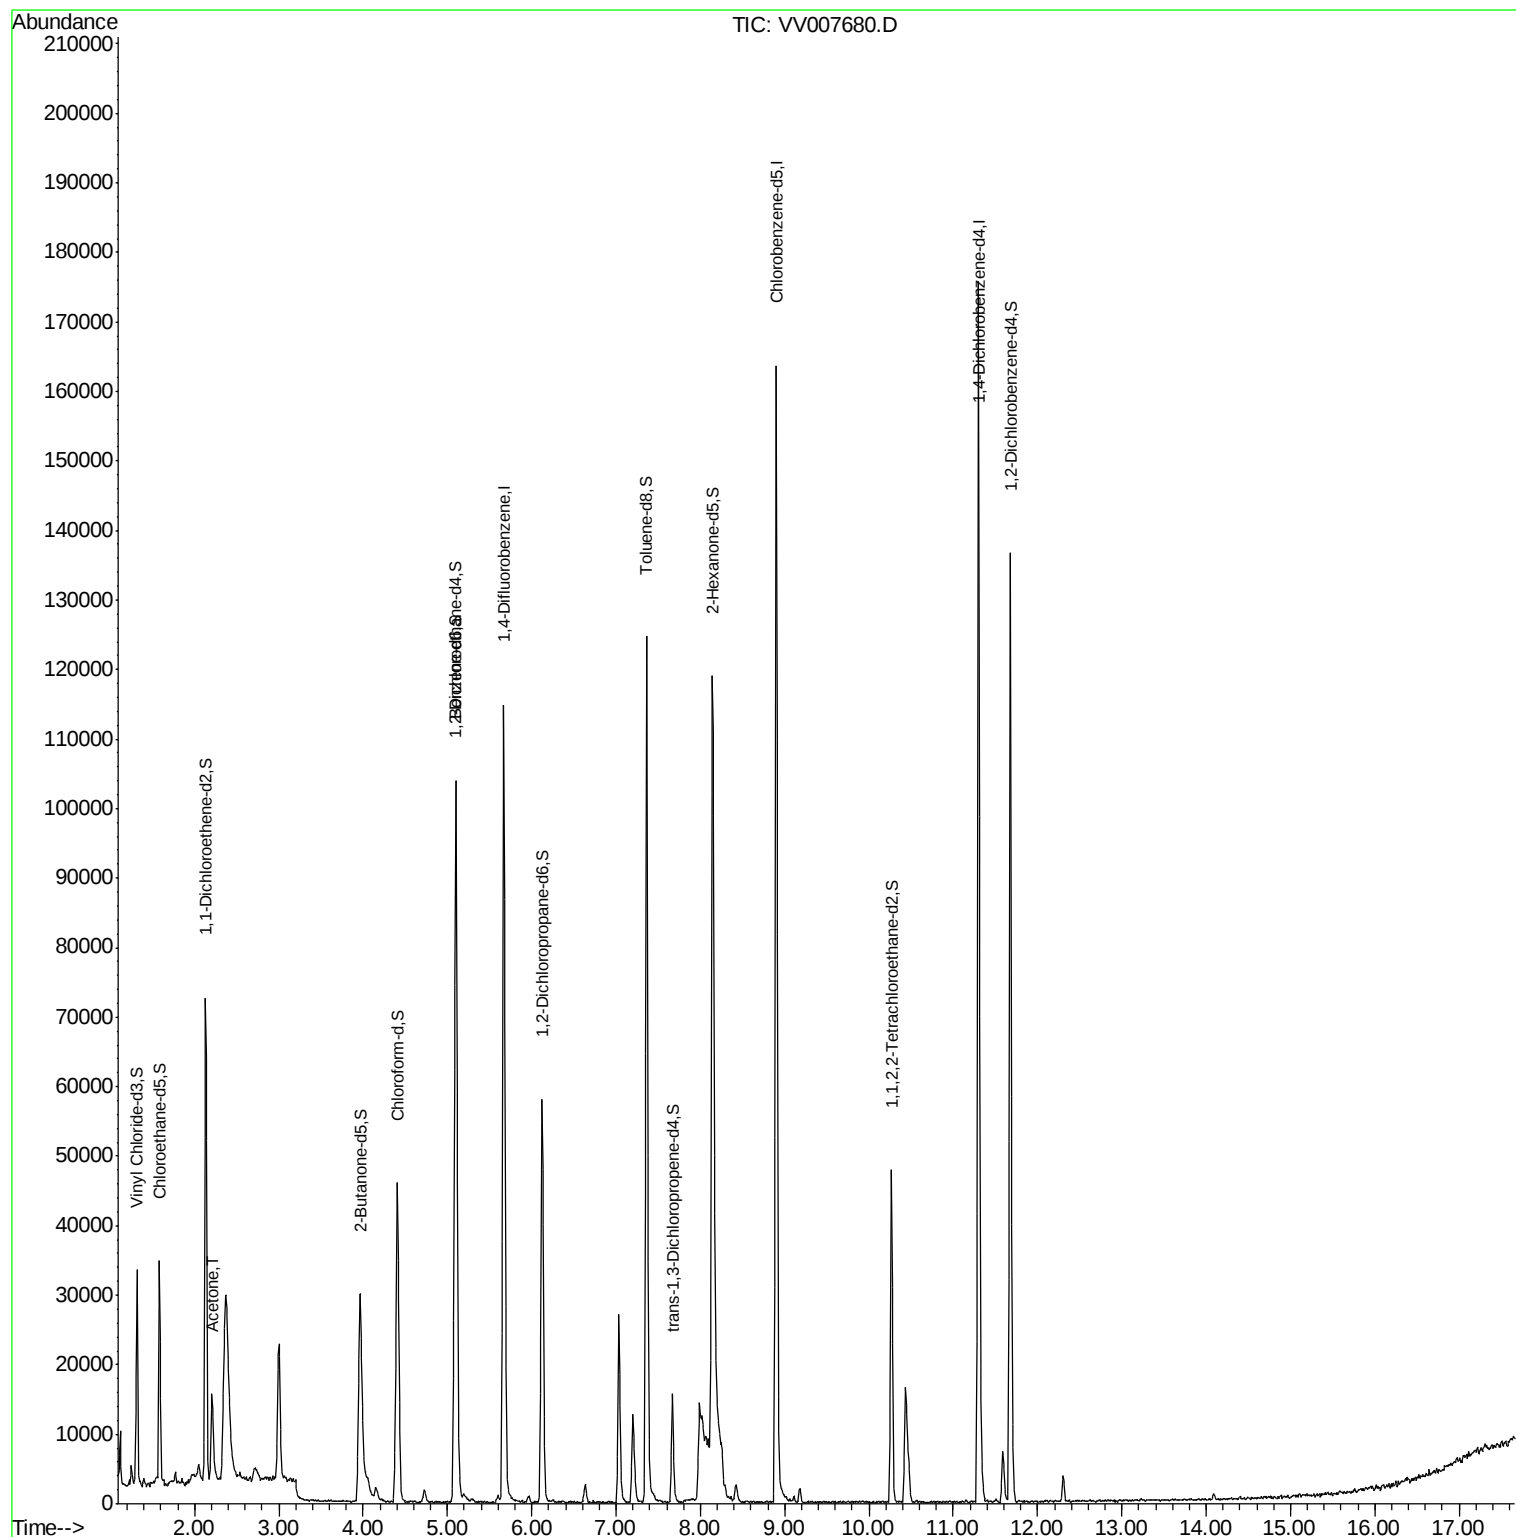

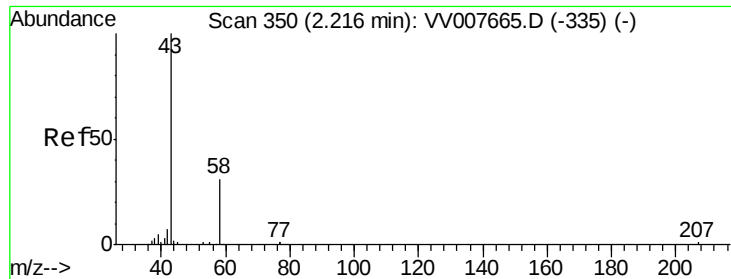

#13

Acetone

Concen: 14.080 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.01 min

Lab File: VV007680.D

Acq: 21 Sep 2018 02:55

Instrument :
MSVOA_V
ClientSampleId :
COT10

Tot Ion: 43 Resp: 15185

Ion Ratio Lower Upper

43 100

58 33.2 0.0 63.6

