


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV092018\
Data File : VV007643.D
Acq On : 20 Sep 2018 08:29
Operator : SY/MD
Sample : BFB61
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB61

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091918WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Sep 21 03:27:29 2018

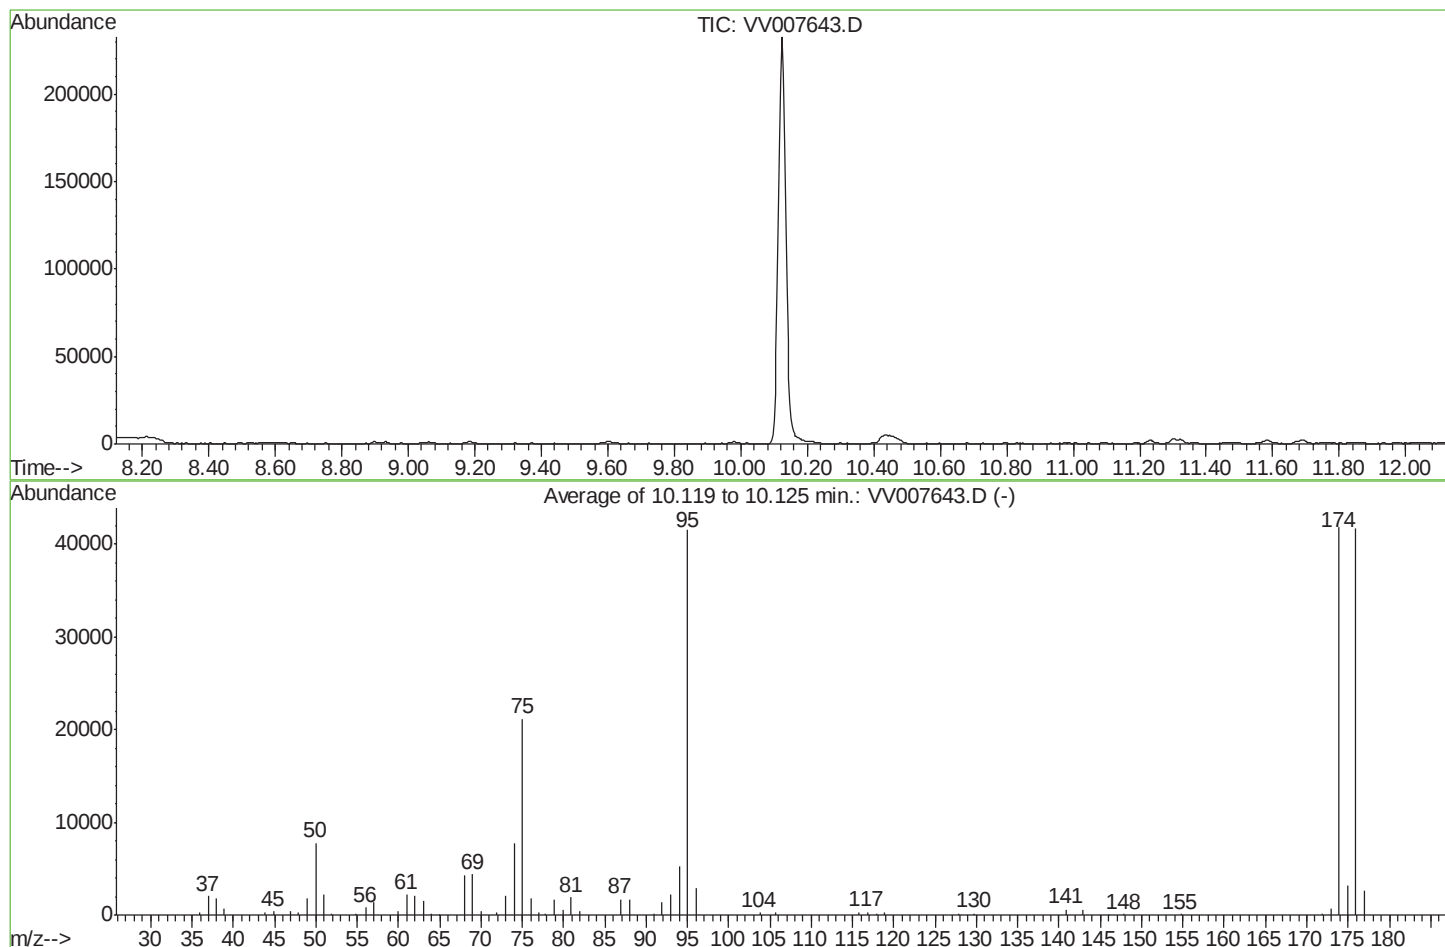

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	7788	PASS
75	95	30	80	51.0	21173	PASS
95	95	100	100	100.0	41546	PASS
96	95	5	9	6.9	2864	PASS
173	174	0.00	2	1.5	629	PASS
174	95	50	120	100.7	41837	PASS
175	174	5	9	7.6	3190	PASS
176	174	95	101	99.9	41778	PASS
177	176	5	9	6.1	2568	PASS

m/z	Abundance
43.90	264.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
35.90	368.0
36.90	2060.0
38.00	1739.0
38.90	672.0
44.00	483.0
44.90	361.0
46.90	328.0
47.90	344.0
49.00	1728.0
50.00	7133.0
51.00	2148.0
51.90	104.0
54.90	165.0
56.00	757.0
57.00	1329.0
60.00	380.0
61.00	2024.0
62.00	2037.0
63.00	1511.0
64.00	191.0
67.90	4113.0
69.00	4212.0
70.00	360.0
71.90	205.0
73.00	1910.0
74.00	7379.0
75.00	20024.0
76.00	1821.0
76.90	247.0
77.70	147.0
78.90	1556.0
79.90	535.0
80.90	1776.0
81.90	422.0
86.90	1684.0
88.00	1396.0
91.00	192.0
92.00	1366.0
92.90	1943.0
94.00	5021.0
95.00	38624.0
96.00	2745.0
103.80	215.0
105.70	230.0
115.80	216.0
116.80	292.0
117.90	155.0
118.90	263.0
127.80	144.0
129.80	195.0
140.90	578.0
142.90	529.0
147.90	119.0
154.80	103.0
171.90	169.0
173.00	603.0
173.90	37856.0
174.90	3006.0
175.90	38384.0
176.90	2518.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
35.90	342.0
37.00	2096.0
38.00	1788.0
38.90	662.0
44.00	495.0
44.90	408.0
46.90	408.0
47.90	322.0
49.00	1845.0
50.00	8127.0
51.00	2261.0
52.00	119.0
54.90	163.0
56.00	840.0
57.00	1469.0
60.00	395.0
61.00	2213.0
61.90	2191.0
63.00	1580.0
64.00	175.0
64.90	100.0
68.00	4476.0
69.00	4546.0
70.00	387.0
71.90	236.0
73.00	2106.0
74.00	7954.0
75.00	21832.0
76.00	1846.0
77.00	289.0
77.80	168.0
78.90	1704.0
79.90	557.0
80.90	1972.0
81.90	414.0
86.90	1727.0
87.90	1699.0
90.90	196.0
92.00	1512.0
93.00	2265.0
94.00	5435.0
95.00	43008.0
96.00	2982.0
103.80	247.0
105.70	242.0
115.80	244.0
116.80	356.0
117.80	189.0
118.90	293.0
127.80	196.0
129.70	206.0
140.90	640.0
142.90	602.0
147.90	116.0
154.80	147.0
171.90	206.0
173.00	635.0
173.90	43032.0
174.90	3292.0
175.90	43208.0
176.90	2615.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
35.90	307.0
37.00	1920.0
38.00	1740.0
38.90	666.0
43.90	493.0
44.90	391.0
46.90	414.0
47.90	284.0
49.00	1749.0
50.00	8105.0
51.00	2188.0
54.90	160.0
56.00	817.0
57.00	1410.0
60.00	429.0
61.00	2217.0
61.90	2127.0
63.00	1468.0
63.90	155.0
64.90	108.0
68.00	4394.0
69.00	4504.0
70.00	375.0
71.90	251.0
73.00	2120.0
74.00	7862.0
75.00	21664.0
76.00	1776.0
77.00	248.0
77.90	167.0
78.90	1759.0
79.90	496.0
80.90	1940.0
81.90	387.0
86.90	1600.0
87.90	1821.0
90.80	211.0
91.90	1452.0
93.00	2386.0
94.00	5401.0
95.00	43008.0
96.00	2866.0
103.80	240.0
105.80	229.0
115.80	237.0
116.80	376.0
117.80	199.0
118.90	290.0
127.90	215.0
129.80	206.0
140.90	631.0
142.90	608.0
145.90	107.0
147.90	107.0
154.80	158.0
171.90	250.0
173.00	649.0
173.90	44624.0
174.90	3272.0
175.90	43744.0
176.90	2572.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61