

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW092021\
 Data File : VW022251.D
 Acq On : 20 Sep 2021 23:03
 Operator : SY/MD
 Sample : M3788-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :


Quant Time: Sep 21 06:23:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Sep 21 06:08:34 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	311039	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	293443	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	126013	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	102547	47.608	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	95.220%	

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022251.D
Acq On : 20 Sep 2021 23:03
Operator : SY/MD
Sample : M3788-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Sep 21 06:23:19 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 21 06:08:34 2021
Response via : Initial Calibration




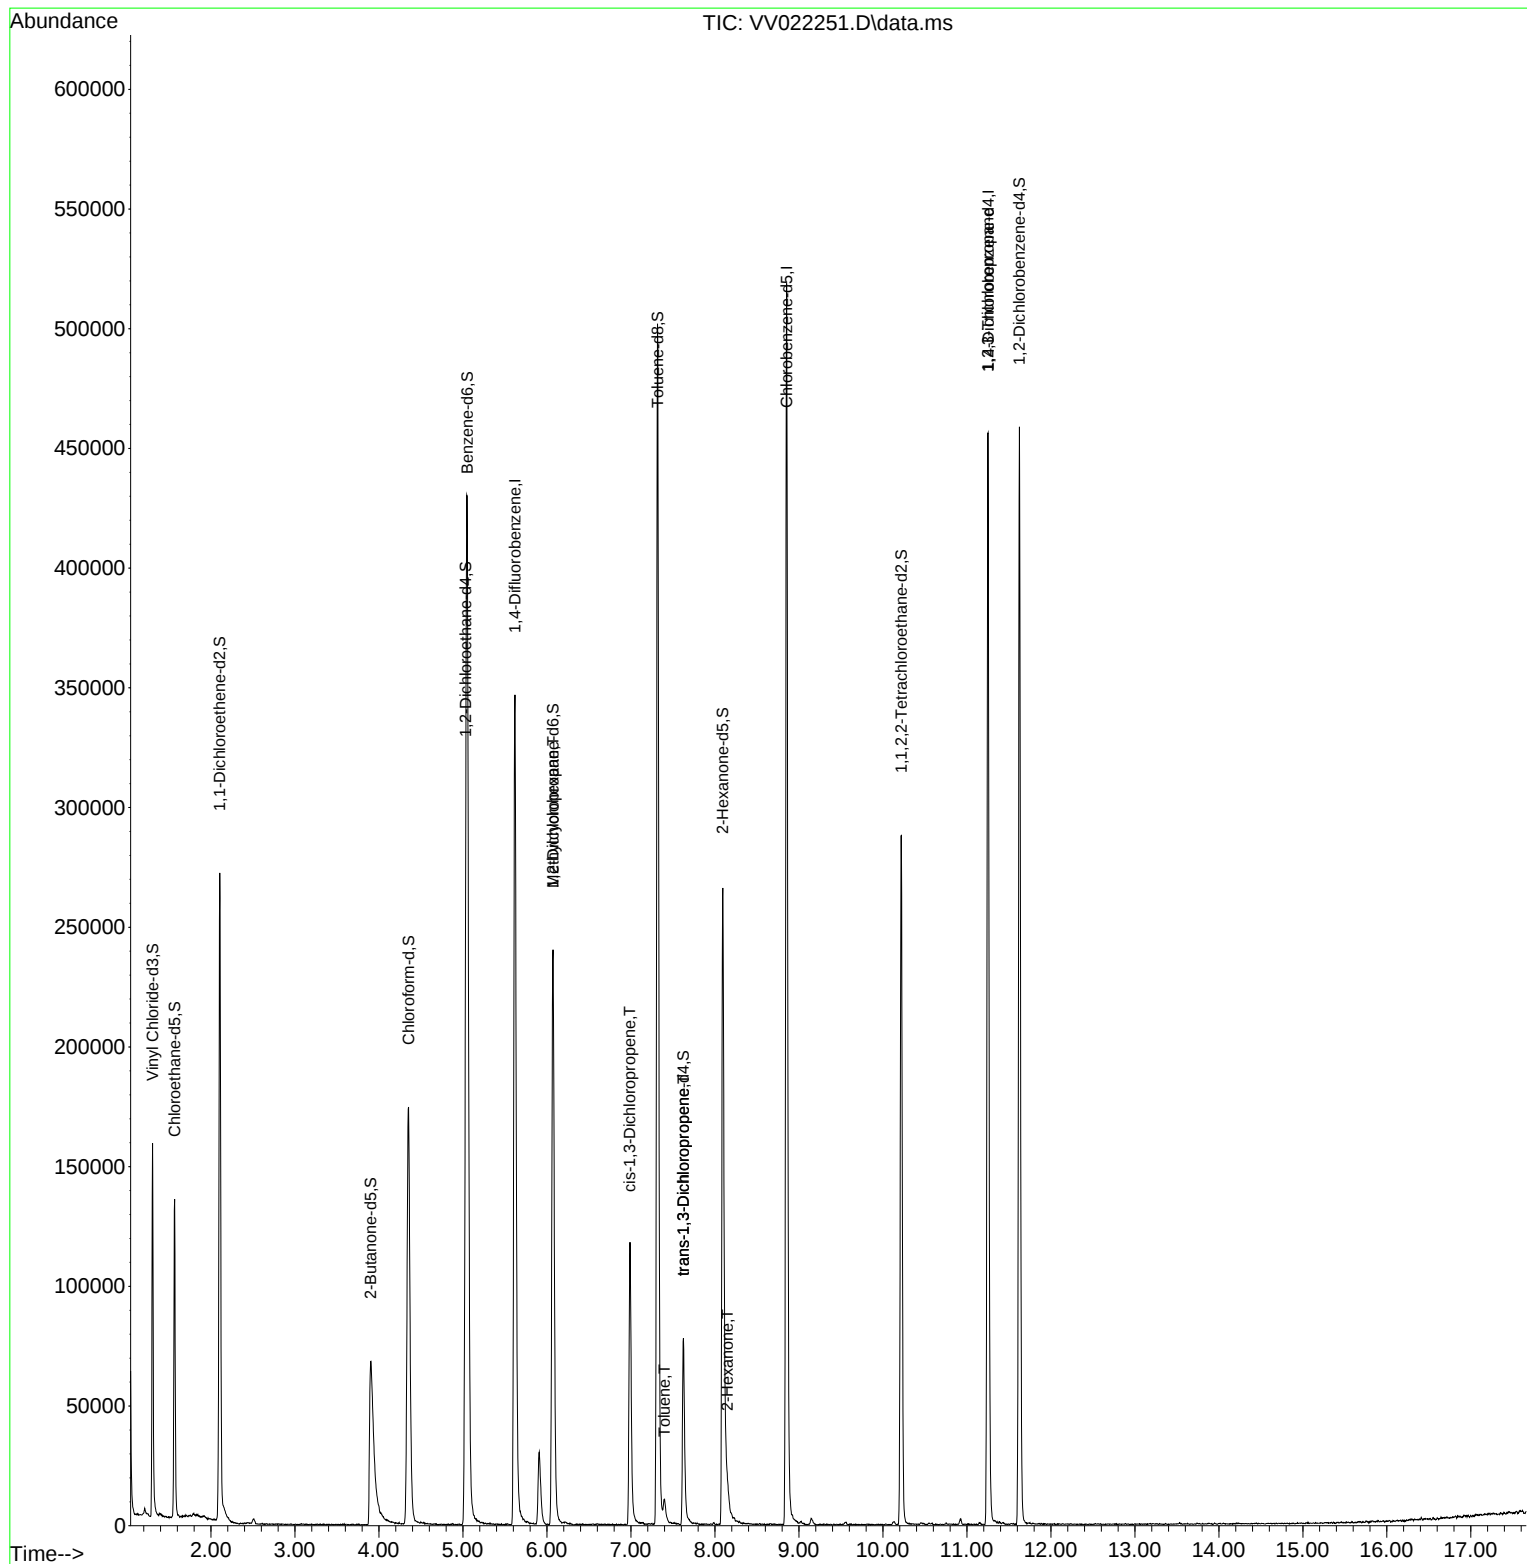


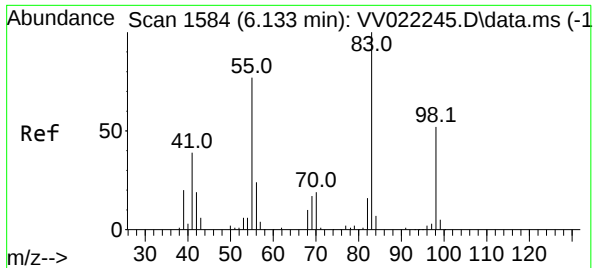


#35
Methylcyclohexane
Concen: 7.973 ug/L
RT: 6.072 min Scan# 1565
Delta R.T. -0.061 min
Lab File: VV022251.D
Acq: 20 Sep 2021 23:03

Instrument :
MSVOA_V
ClientSampled :

Tgt Ion	Ratio	Lower	Upper
83	100		
55	0.1	56.8	85.2#
98	1.8	39.9	59.9#

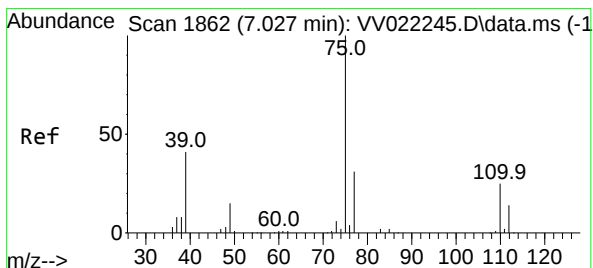
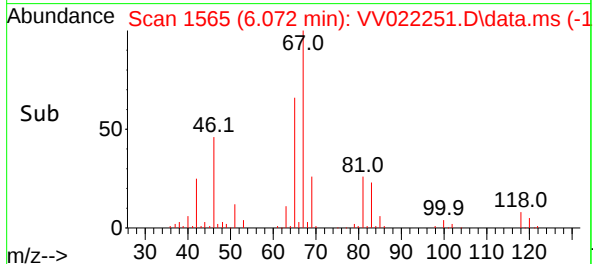
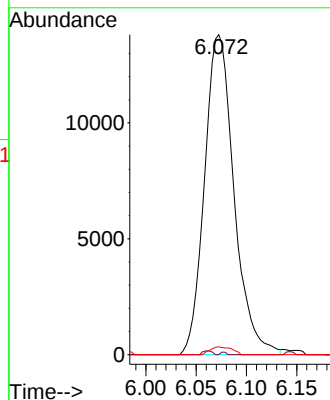
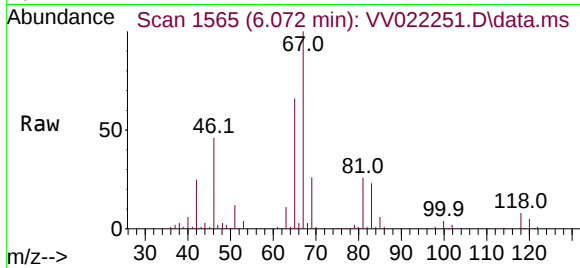


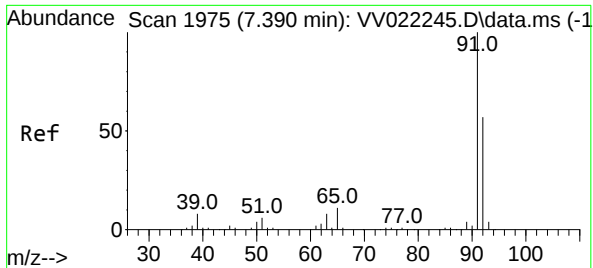


#42
Toluene
Concen: 0.793 ug/L
RT: 7.397 min Scan# 1977
Delta R.T. 0.007 min
Lab File: VV022251.D
Acq: 20 Sep 2021 23:03

Instrument :
MSVOA_V
ClientSampled :

Tgt Ion: 91 Resp: 7304
Ion Ratio Lower Upper
91 100
92 59.3 40.3 74.8

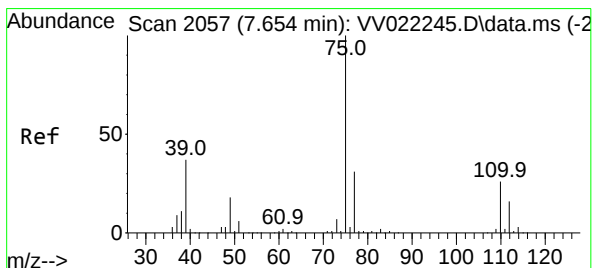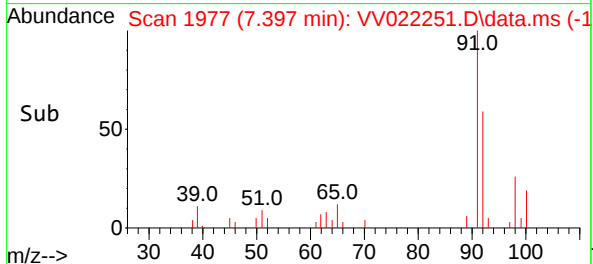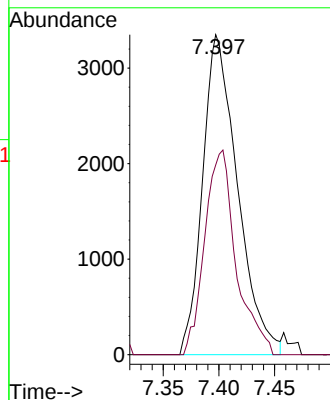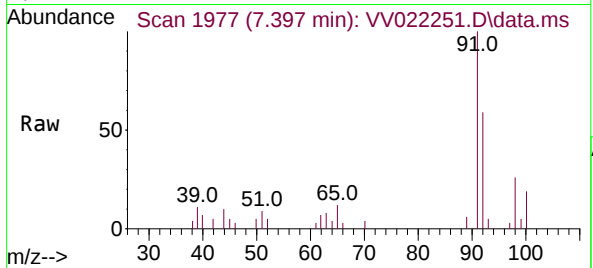

#44

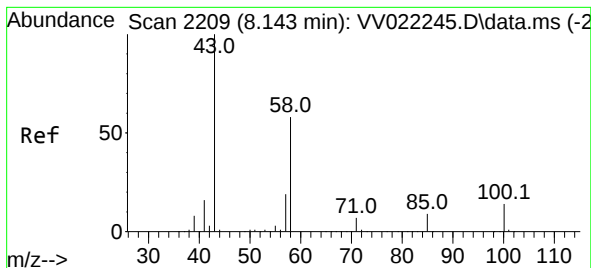

#48

2-Hexanone

Concen: 3.413 ug/L

RT: 8.146 min Scan# 2210

Delta R.T. 0.003 min

Lab File: VV022251.D

Acq: 20 Sep 2021 23:03

Tgt Ion: 43 Resp: 7944

Ion Ratio Lower Upper

43 100

58 50.4 47.5 71.3

57 1.3 15.9 23.9#

100 2.3 11.4 17.2#

