

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022226.D
 Acq On : 20 Sep 2021 12:40
 Operator : SY/MD
 Sample : M3787-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022226.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	103	rVB	165072	173184	15.00%	2.011%
2	1.568	156	164	179	rBV	138725	157698	13.66%	1.832%
3	2.105	321	331	346	rBV	286739	415398	35.97%	4.824%
4	2.400	421	423	427	rBV2	518	371	0.03%	0.004%
5	2.497	450	453	455	rBV2	575	417	0.04%	0.005%
6	2.642	496	498	501	rVB2	348	158	0.01%	0.002%
7	2.690	510	513	515	rBV	227	137	0.01%	0.002%
8	2.751	529	532	535	rBV2	361	279	0.02%	0.003%
9	2.963	595	598	601	rBV2	280	193	0.02%	0.002%
10	2.982	601	604	609	rVB2	430	327	0.03%	0.004%
11	3.008	609	612	614	rBV2	242	126	0.01%	0.001%
12	3.143	651	654	658	rBV	459	353	0.03%	0.004%
13	3.256	683	689	691	rBV3	305	367	0.03%	0.004%
14	3.372	722	725	727	rBV	244	145	0.01%	0.002%
15	3.490	760	762	768	rVB4	330	243	0.02%	0.003%
16	3.716	829	832	836	rBV	273	207	0.02%	0.002%
17	3.806	858	860	864	rVB	256	124	0.01%	0.001%
18	3.828	864	867	871	rBV2	483	222	0.02%	0.003%
19	3.867	876	879	880	rBV	330	132	0.01%	0.002%
20	3.905	880	891	938	rBV	69574	255827	22.15%	2.971%
21	4.240	993	995	996	rBV	417	147	0.01%	0.002%
22	4.352	1016	1030	1057	rVB	178864	438584	37.98%	5.094%
23	4.716	1140	1143	1145	rBV2	246	147	0.01%	0.002%
24	4.809	1171	1172	1176	rBV2	255	128	0.01%	0.001%
25	4.912	1201	1204	1210	rVB	420	304	0.03%	0.004%
26	4.947	1210	1215	1217	rBV2	258	201	0.02%	0.002%
27	5.050	1227	1247	1289	rBV2	457489	1154848	100.00%	13.412%
28	5.301	1323	1325	1329	rBV2	368	185	0.02%	0.002%
29	5.452	1371	1372	1374	rBV	309	169	0.01%	0.002%
30	5.529	1393	1396	1397	rBV2	328	199	0.02%	0.002%
31	5.619	1412	1424	1450	rBV	351534	709767	61.46%	8.243%
32	5.912	1502	1515	1540	rBV6	40742	98540	8.53%	1.144%
33	6.072	1552	1565	1591	rBV	243243	506601	43.87%	5.884%
34	6.301	1633	1636	1639	rBV2	389	299	0.03%	0.003%
35	6.330	1643	1645	1647	rVB2	381	153	0.01%	0.002%
36	6.342	1647	1649	1651	rBV2	339	156	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022226.D
 Acq On : 20 Sep 2021 12:40
 Operator : SY/MD
 Sample : M3787-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.359	1651	1654	1656	rBV2	353	178	0.02%	0.002%
38	6.371	1656	1658	1663	rVB2	250	162	0.01%	0.002%
39	6.397	1663	1666	1670	rVB2	411	295	0.03%	0.003%
40	6.503	1695	1699	1702	rBV	218	173	0.01%	0.002%
41	6.529	1702	1707	1708	rBV3	225	173	0.01%	0.002%
42	6.641	1739	1742	1746	rBV3	249	163	0.01%	0.002%
43	6.667	1747	1750	1751	rBV3	496	203	0.02%	0.002%
44	6.693	1756	1758	1763	rBV2	471	335	0.03%	0.004%
45	6.757	1775	1778	1780	rBV	254	146	0.01%	0.002%
46	6.773	1781	1783	1789	rVB2	247	125	0.01%	0.001%
47	6.889	1815	1819	1822	rBV2	275	234	0.02%	0.003%
48	6.989	1836	1850	1872	rBV	130189	238520	20.65%	2.770%
49	7.207	1916	1918	1920	rBV2	507	251	0.02%	0.003%
50	7.265	1933	1936	1938	rBV	478	317	0.03%	0.004%
51	7.317	1940	1952	1972	rBV	527237	913978	79.14%	10.615%
52	7.625	2037	2048	2069	rBV	88912	158722	13.74%	1.843%
53	7.821	2107	2109	2112	rVB3	329	136	0.01%	0.002%
54	7.921	2137	2140	2142	rBV2	441	257	0.02%	0.003%
55	7.944	2144	2147	2148	rBV	549	253	0.02%	0.003%
56	7.985	2157	2160	2165	rVB4	780	586	0.05%	0.007%
57	8.018	2168	2170	2175	rVB2	381	241	0.02%	0.003%
58	8.095	2183	2194	2231	rBV	267255	538172	46.60%	6.250%
59	8.555	2334	2337	2340	rBV3	363	294	0.03%	0.003%
60	8.625	2356	2359	2360	rBV2	430	212	0.02%	0.002%
61	8.722	2387	2389	2391	rBV	296	123	0.01%	0.001%
62	8.741	2391	2395	2397	rVV2	322	250	0.02%	0.003%
63	8.854	2418	2430	2457	rBV	521589	848250	73.45%	9.852%
64	9.137	2515	2518	2522	rBV2	924	841	0.07%	0.010%
65	9.201	2535	2538	2539	rBV	263	171	0.01%	0.002%
66	9.275	2558	2561	2563	rBV	205	174	0.02%	0.002%
67	9.542	2639	2644	2645	rBV	352	257	0.02%	0.003%
68	9.558	2647	2649	2652	rVB2	292	137	0.01%	0.002%
69	9.596	2659	2661	2665	rBV	225	192	0.02%	0.002%
70	9.706	2693	2695	2698	rVB3	328	186	0.02%	0.002%
71	10.030	2789	2796	2800	rBV4	1599	2031	0.18%	0.024%
72	10.088	2811	2814	2818	rBV2	318	303	0.03%	0.004%
73	10.130	2819	2827	2828	rBV4	2209	2277	0.20%	0.026%
74	10.217	2840	2854	2876	rBV	307664	487970	42.25%	5.667%
75	10.339	2890	2892	2893	rBV2	445	146	0.01%	0.002%
76	10.464	2929	2931	2935	rBV	254	217	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022226.D
 Acq On : 20 Sep 2021 12:40
 Operator : SY/MD
 Sample : M3787-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.542	2948	2955	2957	rBV2	558	519	0.04%	0.006%
78	10.571	2957	2964	2965	rBV2	744	548	0.05%	0.006%
79	10.606	2972	2975	2983	rVB3	601	569	0.05%	0.007%
80	10.664	2990	2993	2996	rBV2	294	228	0.02%	0.003%
81	10.722	3006	3011	3013	rBV2	142	133	0.01%	0.002%
82	10.854	3050	3052	3057	rBV2	338	229	0.02%	0.003%
83	10.889	3060	3063	3064	rVV2	298	148	0.01%	0.002%
84	10.921	3067	3073	3082	rVV5	1743	2163	0.19%	0.025%
85	11.027	3104	3106	3108	rBV2	239	117	0.01%	0.001%
86	11.252	3164	3176	3195	rBV	467163	734737	63.62%	8.533%
87	11.394	3213	3220	3223	rBV6	1314	1596	0.14%	0.019%
88	11.625	3280	3292	3311	rBV	484755	752317	65.14%	8.737%
89	11.780	3337	3340	3341	rBV2	808	412	0.04%	0.005%
90	11.850	3358	3362	3364	rBV2	450	290	0.03%	0.003%
91	12.336	3510	3513	3515	rBV	262	141	0.01%	0.002%
92	12.394	3529	3531	3535	rVB2	290	154	0.01%	0.002%
93	12.416	3535	3538	3539	rBV	289	153	0.01%	0.002%
94	12.529	3571	3573	3575	rVB	341	152	0.01%	0.002%
95	12.545	3575	3578	3581	rBV2	362	215	0.02%	0.002%
96	12.632	3602	3605	3607	rBV	180	129	0.01%	0.001%
97	12.734	3633	3637	3640	rBV3	351	375	0.03%	0.004%
98	12.895	3685	3687	3689	rBV	428	132	0.01%	0.002%
99	13.622	3911	3913	3917	rVB	352	243	0.02%	0.003%
100	14.632	4224	4227	4231	rBV2	587	607	0.05%	0.007%




Sum of corrected areas: 8610294

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022226.D
Acq On : 20 Sep 2021 12:40
Operator : SY/MD
Sample : M3787-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

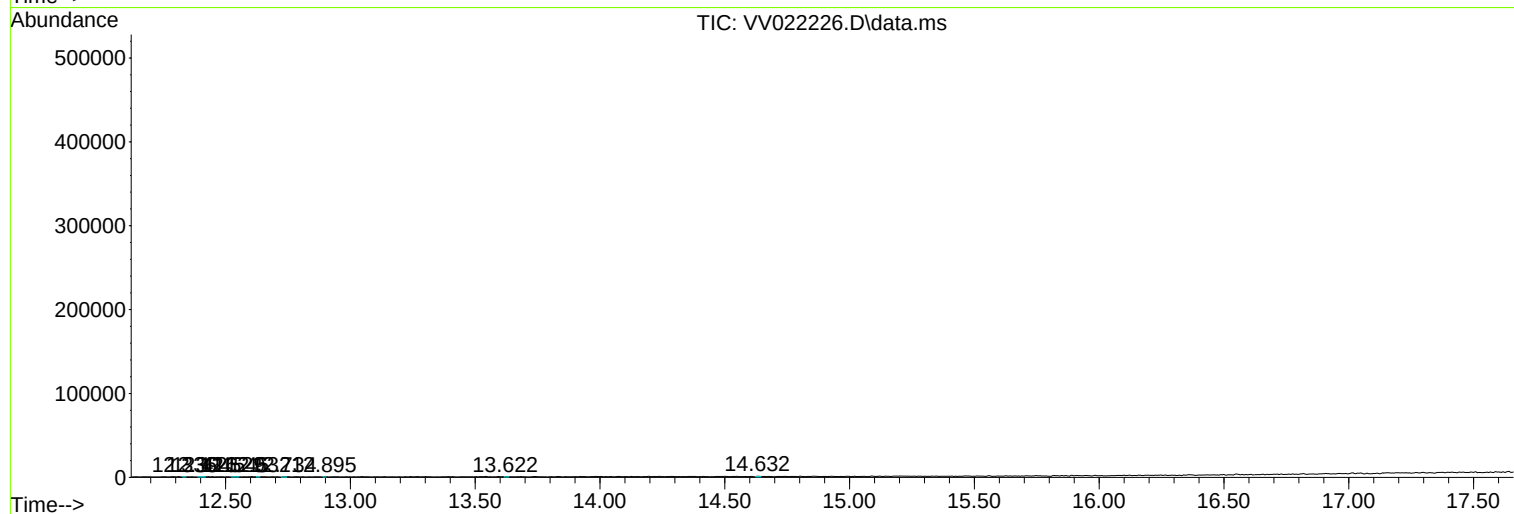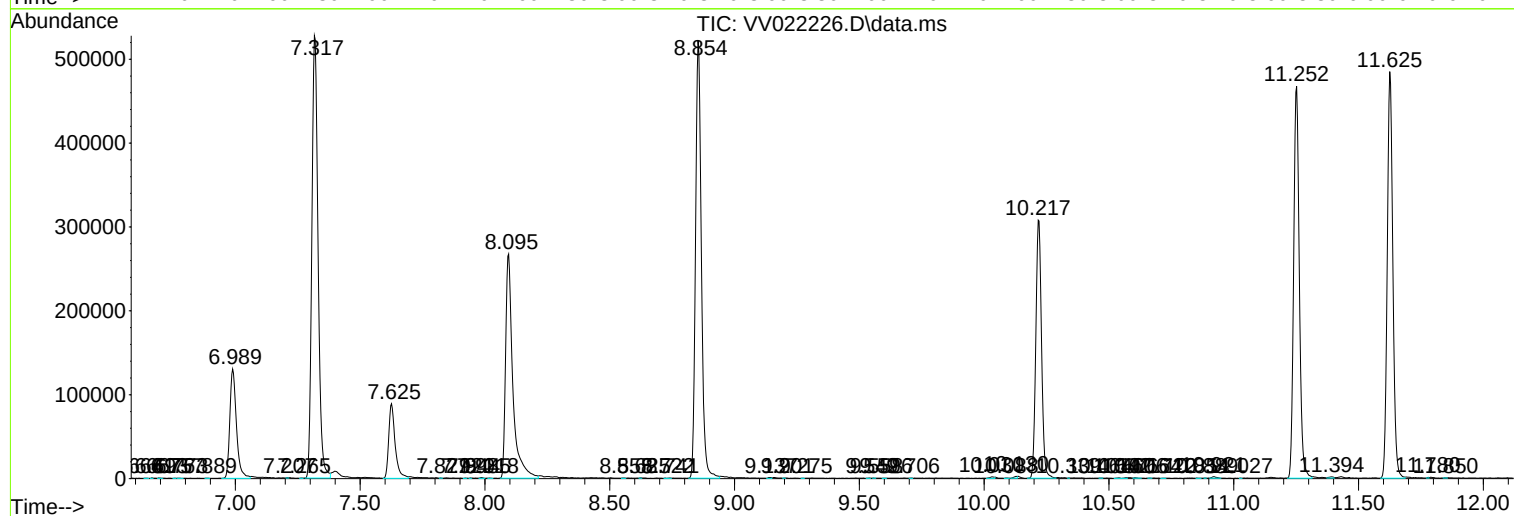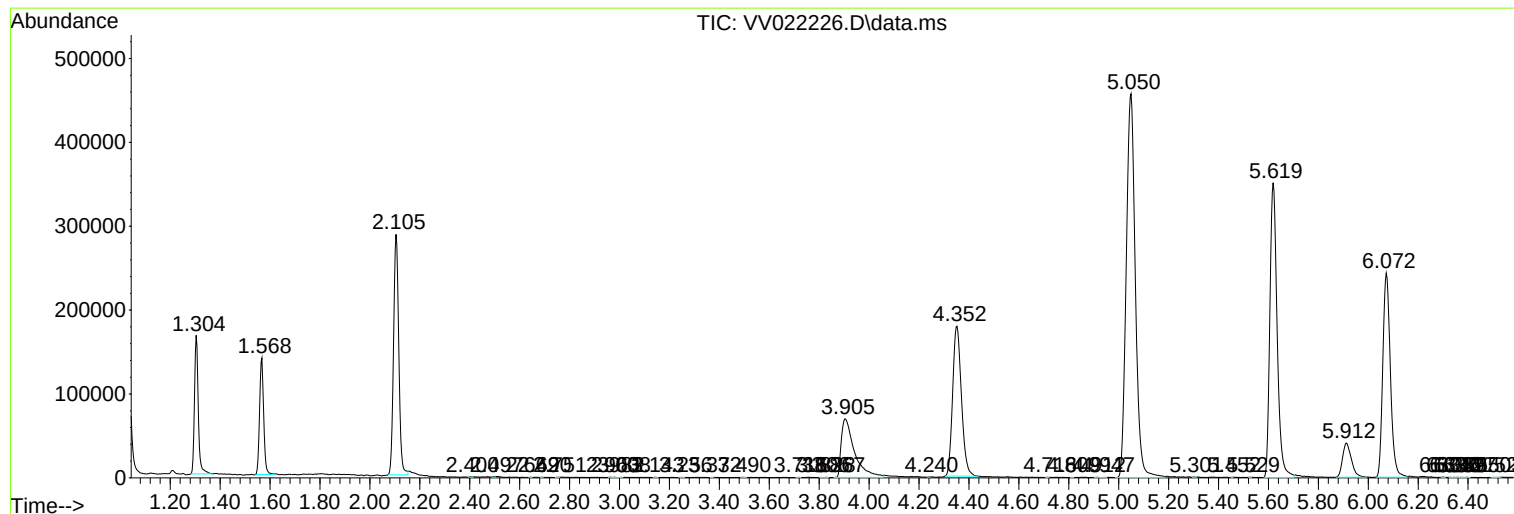

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022226.D
Acq On : 20 Sep 2021 12:40
Operator : SY/MD
Sample : M3787-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022226.D
Acq On : 20 Sep 2021 12:40
Operator : SY/MD
Sample : M3787-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------