

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022227.D
 Acq On : 20 Sep 2021 13:04
 Operator : SY/MD
 Sample : M3787-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022227.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rBV	166228	174901	15.42%	2.024%
2	1.561	155	162	181	rVB	133463	156144	13.77%	1.807%
3	2.105	321	331	354	rVB	290667	435900	38.43%	5.044%
4	2.732	523	526	532	rVB3	680	439	0.04%	0.005%
5	2.764	532	536	537	rBV	395	192	0.02%	0.002%
6	2.883	569	573	577	rBV2	444	301	0.03%	0.003%
7	3.060	625	628	630	rBV	229	133	0.01%	0.002%
8	3.134	649	651	654	rVB2	304	174	0.02%	0.002%
9	3.153	654	657	661	rBV2	249	141	0.01%	0.002%
10	3.458	750	752	759	rVB3	272	272	0.02%	0.003%
11	3.568	784	786	792	rVB3	356	257	0.02%	0.003%
12	3.732	833	837	839	rBV2	253	186	0.02%	0.002%
13	3.777	848	851	853	rBV	175	134	0.01%	0.002%
14	3.806	858	860	865	rVV2	212	184	0.02%	0.002%
15	3.876	872	882	912	rBV	92876	257672	22.72%	2.982%
16	4.349	1012	1029	1056	rBV	178918	445557	39.28%	5.156%
17	4.677	1128	1131	1133	rBV2	340	222	0.02%	0.003%
18	4.738	1148	1150	1152	rBV	261	153	0.01%	0.002%
19	4.822	1171	1176	1181	rVB3	523	427	0.04%	0.005%
20	4.905	1201	1202	1206	rBV2	377	230	0.02%	0.003%
21	4.953	1215	1217	1218	rBV2	342	133	0.01%	0.002%
22	4.986	1225	1227	1228	rBV	282	134	0.01%	0.002%
23	5.047	1229	1246	1277	rVV2	441088	1134264	100.00%	13.126%
24	5.420	1358	1362	1366	rBV3	583	552	0.05%	0.006%
25	5.510	1387	1390	1395	rVB4	440	399	0.04%	0.005%
26	5.535	1395	1398	1400	rBV	351	216	0.02%	0.002%
27	5.619	1411	1424	1454	rBV	362120	723667	63.80%	8.374%
28	5.915	1503	1516	1535	rBV8	47760	112901	9.95%	1.306%
29	6.072	1551	1565	1588	rBV	247145	508906	44.87%	5.889%
30	6.320	1639	1642	1647	rBV2	226	199	0.02%	0.002%
31	6.346	1647	1650	1652	rBV2	358	174	0.02%	0.002%
32	6.452	1679	1683	1686	rBV3	388	239	0.02%	0.003%
33	6.494	1693	1696	1698	rBV	289	186	0.02%	0.002%
34	6.535	1706	1709	1712	rBV	476	353	0.03%	0.004%
35	6.658	1743	1747	1751	rBV2	318	244	0.02%	0.003%
36	6.677	1751	1753	1755	rBV	375	184	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022227.D
 Acq On : 20 Sep 2021 13:04
 Operator : SY/MD
 Sample : M3787-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.738	1767	1772	1775	rBV	272	221	0.02%	0.003%
38	6.892	1817	1820	1829	rVB	346	377	0.03%	0.004%
39	6.944	1829	1836	1839	rBV2	322	350	0.03%	0.004%
40	6.989	1839	1850	1870	rBV	128797	236583	20.86%	2.738%
41	7.185	1909	1911	1914	rBV	411	187	0.02%	0.002%
42	7.249	1927	1931	1932	rBV	245	166	0.01%	0.002%
43	7.268	1934	1937	1940	rVB	392	257	0.02%	0.003%
44	7.317	1940	1952	1971	rBV	517927	898512	79.22%	10.397%
45	7.584	2032	2035	2038	rBV	208	135	0.01%	0.002%
46	7.625	2038	2048	2070	rBV	88821	155498	13.71%	1.799%
47	7.838	2110	2114	2120	rBV4	585	510	0.04%	0.006%
48	7.863	2120	2122	2124	rBV2	409	186	0.02%	0.002%
49	7.982	2154	2159	2164	rBV2	650	737	0.06%	0.009%
50	8.053	2178	2181	2182	rBV2	257	181	0.02%	0.002%
51	8.092	2182	2193	2228	rBV2	265885	520811	45.92%	6.027%
52	8.452	2303	2305	2308	rVB2	523	279	0.02%	0.003%
53	8.519	2323	2326	2328	rBV2	353	242	0.02%	0.003%
54	8.580	2343	2345	2349	rVB2	328	167	0.01%	0.002%
55	8.603	2349	2352	2357	rBV3	360	391	0.03%	0.005%
56	8.629	2357	2360	2361	rBV2	562	259	0.02%	0.003%
57	8.690	2376	2379	2382	rBV2	154	140	0.01%	0.002%
58	8.776	2400	2406	2408	rBV	249	257	0.02%	0.003%
59	8.854	2418	2430	2456	rBV	539325	868718	76.59%	10.053%
60	9.117	2510	2512	2515	rVB2	372	185	0.02%	0.002%
61	9.137	2515	2518	2519	rBV	276	142	0.01%	0.002%
62	9.275	2560	2561	2569	rVB2	500	359	0.03%	0.004%
63	9.310	2569	2572	2576	rBV2	294	206	0.02%	0.002%
64	9.355	2583	2586	2590	rBV2	347	281	0.02%	0.003%
65	9.465	2616	2620	2621	rBV	300	207	0.02%	0.002%
66	9.497	2627	2630	2633	rVB	296	186	0.02%	0.002%
67	9.551	2643	2647	2651	rBV	312	243	0.02%	0.003%
68	9.751	2705	2709	2714	rVB2	341	308	0.03%	0.004%
69	9.947	2768	2770	2779	rBV2	278	202	0.02%	0.002%
70	10.133	2820	2828	2834	rBV5	1973	2850	0.25%	0.033%
71	10.217	2841	2854	2876	rBV	307970	483473	42.62%	5.595%
72	10.429	2918	2920	2923	rVB	314	170	0.01%	0.002%
73	10.474	2930	2934	2939	rBV2	493	320	0.03%	0.004%
74	10.497	2939	2941	2943	rBV2	271	136	0.01%	0.002%
75	10.513	2943	2946	2947	rBV	246	143	0.01%	0.002%
76	10.554	2956	2959	2961	rVB2	363	203	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022227.D
 Acq On : 20 Sep 2021 13:04
 Operator : SY/MD
 Sample : M3787-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.622	2978	2980	2983	rBV	352	222	0.02%	0.003%
78	10.661	2989	2992	2994	rVB	543	249	0.02%	0.003%
79	10.773	3022	3027	3028	rBV2	303	246	0.02%	0.003%
80	10.792	3031	3033	3036	rBV	202	157	0.01%	0.002%
81	10.834	3043	3046	3048	rVB2	311	172	0.02%	0.002%
82	10.860	3051	3054	3056	rBV	330	178	0.02%	0.002%
83	10.924	3067	3074	3082	rVB5	1836	2634	0.23%	0.030%
84	11.146	3139	3143	3146	rBV3	789	610	0.05%	0.007%
85	11.252	3164	3176	3197	rBV	478821	755044	66.57%	8.737%
86	11.497	3248	3252	3254	rBV	358	282	0.02%	0.003%
87	11.545	3263	3267	3269	rBV2	362	241	0.02%	0.003%
88	11.571	3273	3275	3278	rBV2	336	195	0.02%	0.002%
89	11.625	3280	3292	3317	rVV	468663	747804	65.93%	8.654%
90	11.841	3356	3359	3360	rBV	373	247	0.02%	0.003%
91	12.024	3414	3416	3421	rBV2	448	386	0.03%	0.004%
92	12.046	3421	3423	3425	rBV	340	147	0.01%	0.002%
93	12.159	3456	3458	3461	rBV	305	194	0.02%	0.002%
94	12.358	3518	3520	3522	rBV2	411	201	0.02%	0.002%
95	12.677	3615	3619	3620	rBV	363	247	0.02%	0.003%
96	12.773	3647	3649	3652	rBV	255	180	0.02%	0.002%
97	12.892	3683	3686	3688	rBV2	268	217	0.02%	0.003%
98	12.927	3694	3697	3700	rBV2	344	172	0.02%	0.002%
99	13.394	3839	3842	3844	rBV	429	220	0.02%	0.003%
100	13.995	4027	4029	4031	rBV	458	241	0.02%	0.003%




Sum of corrected areas: 8641634

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022227.D
Acq On : 20 Sep 2021 13:04
Operator : SY/MD
Sample : M3787-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

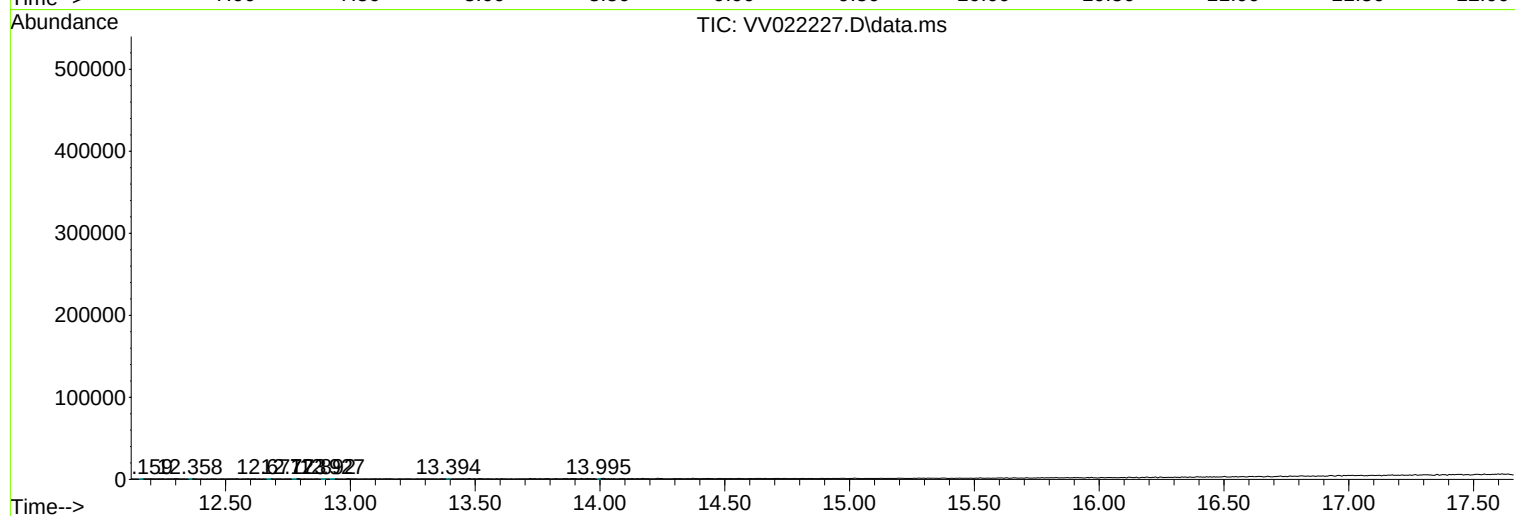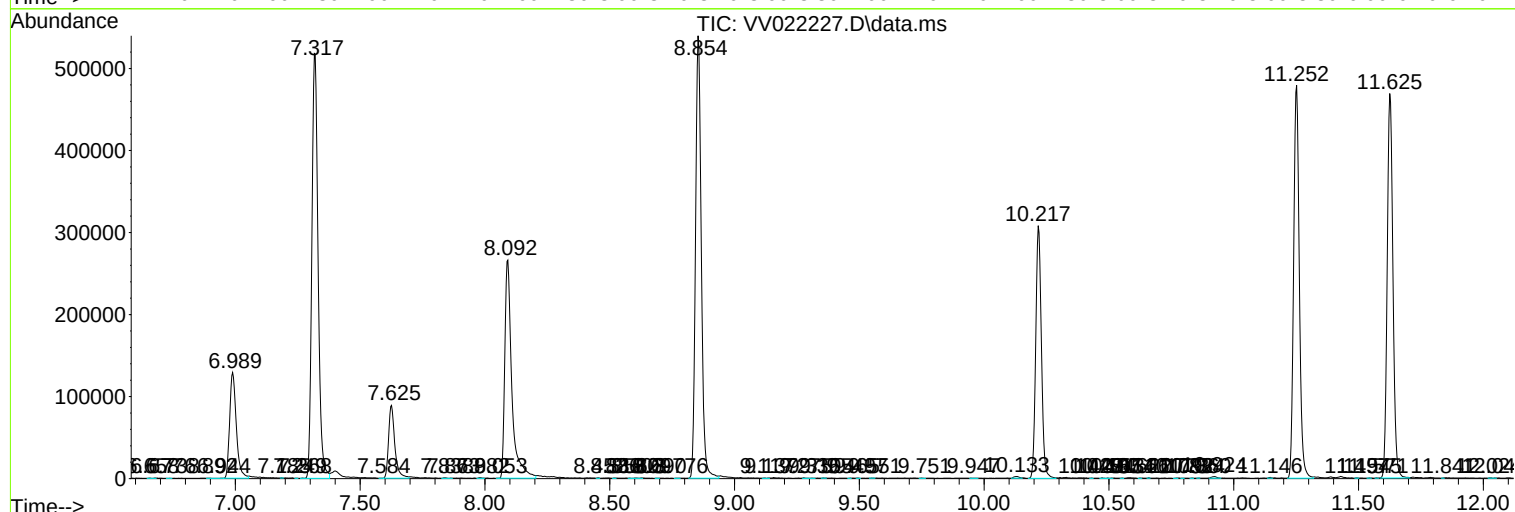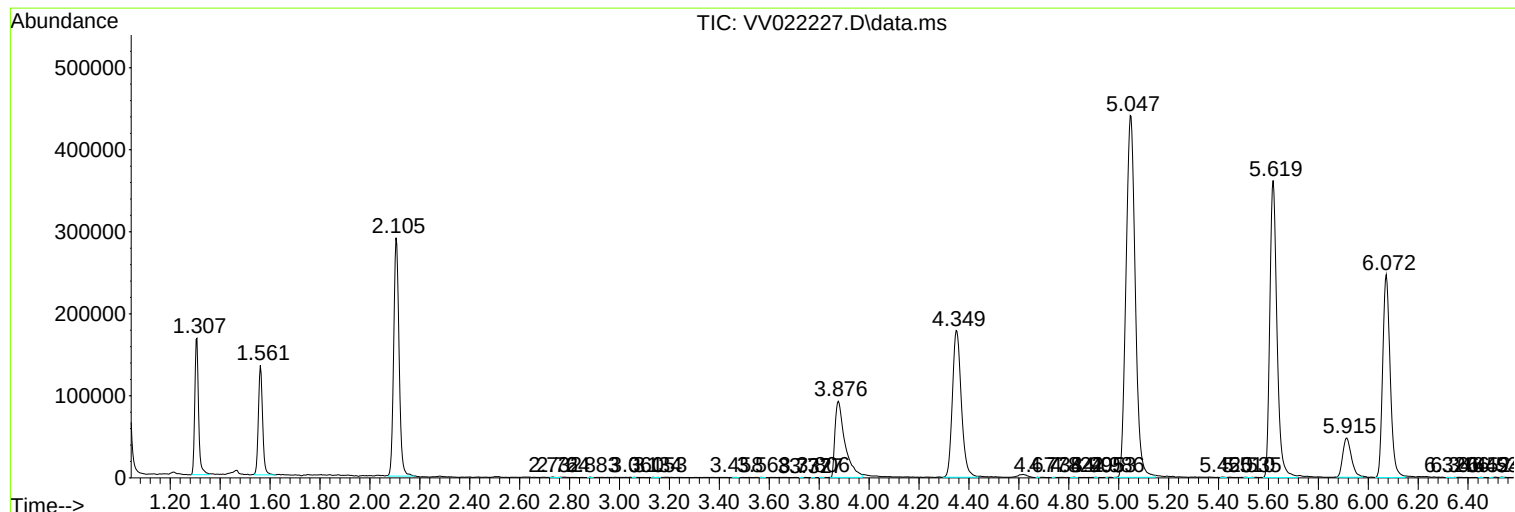

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022227.D
Acq On : 20 Sep 2021 13:04
Operator : SY/MD
Sample : M3787-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022227.D
Acq On : 20 Sep 2021 13:04
Operator : SY/MD
Sample : M3787-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------