

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022235.D
 Acq On : 20 Sep 2021 16:15
 Operator : SY/MD
 Sample : M3788-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022235.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	102	rBV	142276	150995	12.82%	1.578%
2	1.568	156	164	177	rBV	123826	145620	12.37%	1.522%
3	2.108	321	332	365	rVB2	283889	456670	38.78%	4.773%
4	2.323	397	399	401	rBV2	547	310	0.03%	0.003%
5	2.561	472	473	478	rVB2	415	229	0.02%	0.002%
6	2.690	512	513	518	rVB	441	233	0.02%	0.002%
7	2.902	576	579	582	rVV2	260	191	0.02%	0.002%
8	3.002	607	610	612	rBV2	298	192	0.02%	0.002%
9	3.256	687	689	692	rBV2	270	153	0.01%	0.002%
10	3.275	692	695	701	rVB2	216	168	0.01%	0.002%
11	3.310	701	706	709	rBV2	359	215	0.02%	0.002%
12	3.339	712	715	719	rVB3	258	170	0.01%	0.002%
13	3.433	741	744	747	rVB3	221	156	0.01%	0.002%
14	3.905	878	891	929	rBV2	93588	320194	27.19%	3.347%
15	4.230	990	992	994	rBV2	371	154	0.01%	0.002%
16	4.352	1015	1030	1060	rVB	173226	423683	35.98%	4.428%
17	4.616	1099	1112	1126	rBV3	15177	35826	3.04%	0.374%
18	4.754	1153	1155	1160	rVB	274	197	0.02%	0.002%
19	4.970	1219	1222	1226	rBV3	242	191	0.02%	0.002%
20	4.992	1226	1229	1230	rBV	313	176	0.01%	0.002%
21	5.050	1231	1247	1272	rBV2	425210	1074874	91.28%	11.235%
22	5.310	1325	1328	1332	rBV3	388	398	0.03%	0.004%
23	5.478	1375	1380	1384	rBV4	538	435	0.04%	0.005%
24	5.500	1384	1387	1390	rVB	304	157	0.01%	0.002%
25	5.552	1401	1403	1408	rVB	443	279	0.02%	0.003%
26	5.619	1412	1424	1452	rBV	358377	720003	61.14%	7.526%
27	5.915	1502	1516	1550	rBV	594094	1177619	100.00%	12.309%
28	6.072	1553	1565	1588	rVV	235404	481819	40.91%	5.036%
29	6.346	1647	1650	1653	rBV2	191	160	0.01%	0.002%
30	6.410	1665	1670	1673	rBV	374	395	0.03%	0.004%
31	6.458	1684	1685	1687	rBV	464	213	0.02%	0.002%
32	6.503	1697	1699	1703	rBV2	319	145	0.01%	0.002%
33	6.532	1704	1708	1710	rBV2	319	248	0.02%	0.003%
34	6.687	1753	1756	1759	rVV3	549	414	0.04%	0.004%
35	6.703	1759	1761	1766	rVB	329	162	0.01%	0.002%
36	6.793	1785	1789	1790	rBV2	432	243	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022235.D
 Acq On : 20 Sep 2021 16:15
 Operator : SY/MD
 Sample : M3788-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.818	1795	1797	1802	rVB2	338	258	0.02%	0.003%
38	6.854	1805	1808	1811	rVB2	413	202	0.02%	0.002%
39	6.870	1811	1813	1816	rVB	275	147	0.01%	0.002%
40	6.905	1821	1824	1827	rBV2	299	197	0.02%	0.002%
41	6.989	1839	1850	1877	rBV	123196	227956	19.36%	2.383%
42	7.211	1915	1919	1921	rBV2	562	423	0.04%	0.004%
43	7.249	1927	1931	1932	rBV2	375	213	0.02%	0.002%
44	7.320	1941	1953	1972	rBV	494025	855163	72.62%	8.938%
45	7.513	2011	2013	2022	rVB3	564	551	0.05%	0.006%
46	7.625	2039	2048	2075	rBV	82768	145926	12.39%	1.525%
47	7.812	2100	2106	2110	rBV5	475	559	0.05%	0.006%
48	7.854	2117	2119	2123	rBV2	482	313	0.03%	0.003%
49	7.905	2132	2135	2137	rBV	336	241	0.02%	0.003%
50	7.982	2154	2159	2167	rVB4	1922	2613	0.22%	0.027%
51	8.095	2183	2194	2229	rBV2	263919	535523	45.48%	5.597%
52	8.400	2287	2289	2291	rBV	322	187	0.02%	0.002%
53	8.503	2319	2321	2325	rBV2	441	304	0.03%	0.003%
54	8.622	2355	2358	2362	rBV2	354	251	0.02%	0.003%
55	8.661	2367	2370	2373	rBV3	402	292	0.02%	0.003%
56	8.748	2395	2397	2402	rBV2	237	220	0.02%	0.002%
57	8.802	2410	2414	2419	rBV2	299	257	0.02%	0.003%
58	8.854	2419	2430	2463	rBV	522022	866578	73.59%	9.058%
59	9.056	2491	2493	2497	rVB3	456	281	0.02%	0.003%
60	9.075	2497	2499	2503	rVB3	538	281	0.02%	0.003%
61	9.101	2503	2507	2508	rBV2	293	194	0.02%	0.002%
62	9.111	2508	2510	2513	rBV3	431	183	0.02%	0.002%
63	9.146	2518	2521	2522	rBV3	603	287	0.02%	0.003%
64	9.207	2538	2540	2542	rBV	301	153	0.01%	0.002%
65	9.378	2588	2593	2596	rBV3	293	251	0.02%	0.003%
66	9.394	2596	2598	2602	rVB2	480	204	0.02%	0.002%
67	9.500	2625	2631	2632	rBV	350	238	0.02%	0.002%
68	9.593	2657	2660	2662	rBV	317	193	0.02%	0.002%
69	9.796	2718	2723	2724	rBV2	225	164	0.01%	0.002%
70	9.892	2749	2753	2754	rBV	242	156	0.01%	0.002%
71	10.047	2796	2801	2802	rBV	472	356	0.03%	0.004%
72	10.056	2802	2804	2810	rVB2	489	313	0.03%	0.003%
73	10.124	2820	2825	2826	rBV4	1488	1074	0.09%	0.011%
74	10.217	2843	2854	2880	rBV	295976	467757	39.72%	4.889%
75	10.387	2904	2907	2908	rBV	270	153	0.01%	0.002%
76	10.416	2913	2916	2921	rVB3	292	238	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022235.D
 Acq On : 20 Sep 2021 16:15
 Operator : SY/MD
 Sample : M3788-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.538	2948	2954	2956	rBV2	245	272	0.02%	0.003%
78	10.664	2989	2993	2998	rBV	283	252	0.02%	0.003%
79	10.918	3064	3072	3075	rBV6	1708	1882	0.16%	0.020%
80	11.056	3113	3115	3120	rBV2	237	197	0.02%	0.002%
81	11.149	3139	3144	3147	rBV5	983	1025	0.09%	0.011%
82	11.252	3164	3176	3200	rBV	470960	744777	63.24%	7.785%
83	11.625	3280	3292	3313	rBV	447298	710850	60.36%	7.430%
84	11.837	3356	3358	3360	rBV	389	161	0.01%	0.002%
85	11.863	3363	3366	3369	rBV2	313	200	0.02%	0.002%
86	11.979	3399	3402	3404	rBV2	275	164	0.01%	0.002%
87	12.024	3413	3416	3422	rBV	301	243	0.02%	0.003%
88	12.053	3422	3425	3428	rBV2	577	366	0.03%	0.004%
89	12.165	3458	3460	3464	rVB2	448	246	0.02%	0.003%
90	12.349	3515	3517	3520	rVB2	408	218	0.02%	0.002%
91	12.365	3520	3522	3525	rBV	303	176	0.01%	0.002%
92	12.432	3539	3543	3544	rBV2	287	182	0.02%	0.002%
93	12.516	3565	3569	3572	rBV3	240	212	0.02%	0.002%
94	12.612	3597	3599	3603	rBV	365	237	0.02%	0.002%
95	12.661	3612	3614	3618	rBV2	386	176	0.01%	0.002%
96	12.866	3675	3678	3679	rBV	283	153	0.01%	0.002%
97	12.921	3691	3695	3697	rBV2	420	325	0.03%	0.003%
98	13.037	3729	3731	3736	rBV2	266	226	0.02%	0.002%
99	13.095	3744	3749	3752	rBV	358	450	0.04%	0.005%
100	13.545	3887	3889	3891	rBV	403	157	0.01%	0.002%




Sum of corrected areas: 9567284

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022235.D
Acq On : 20 Sep 2021 16:15
Operator : SY/MD
Sample : M3788-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0CJ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

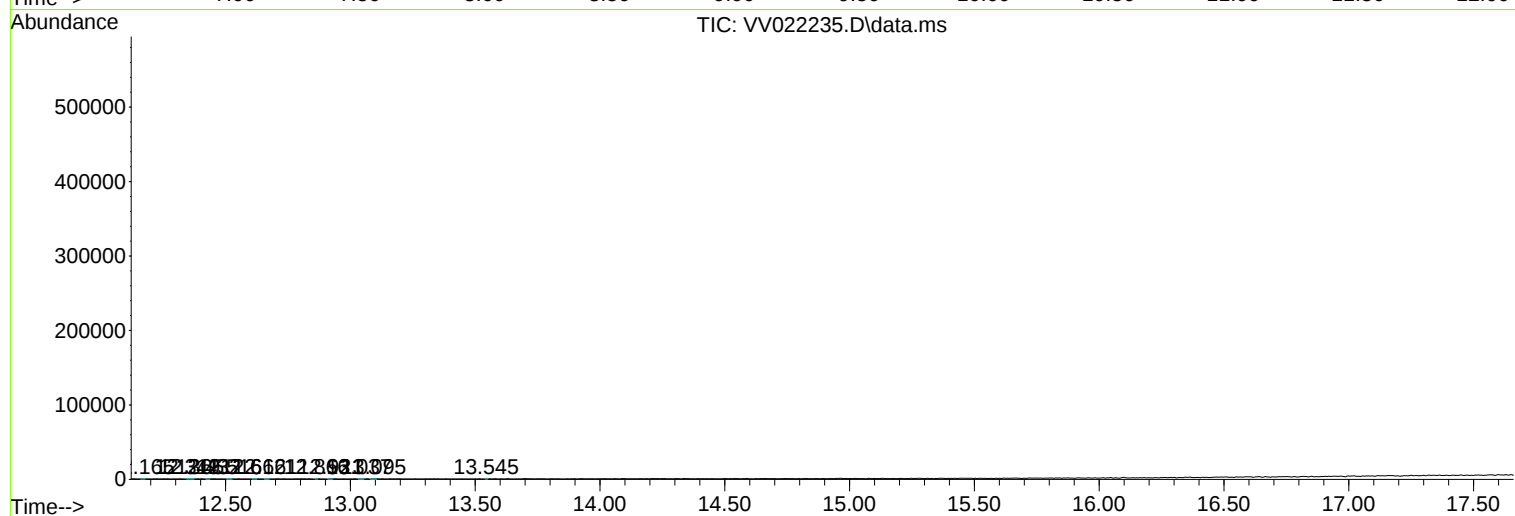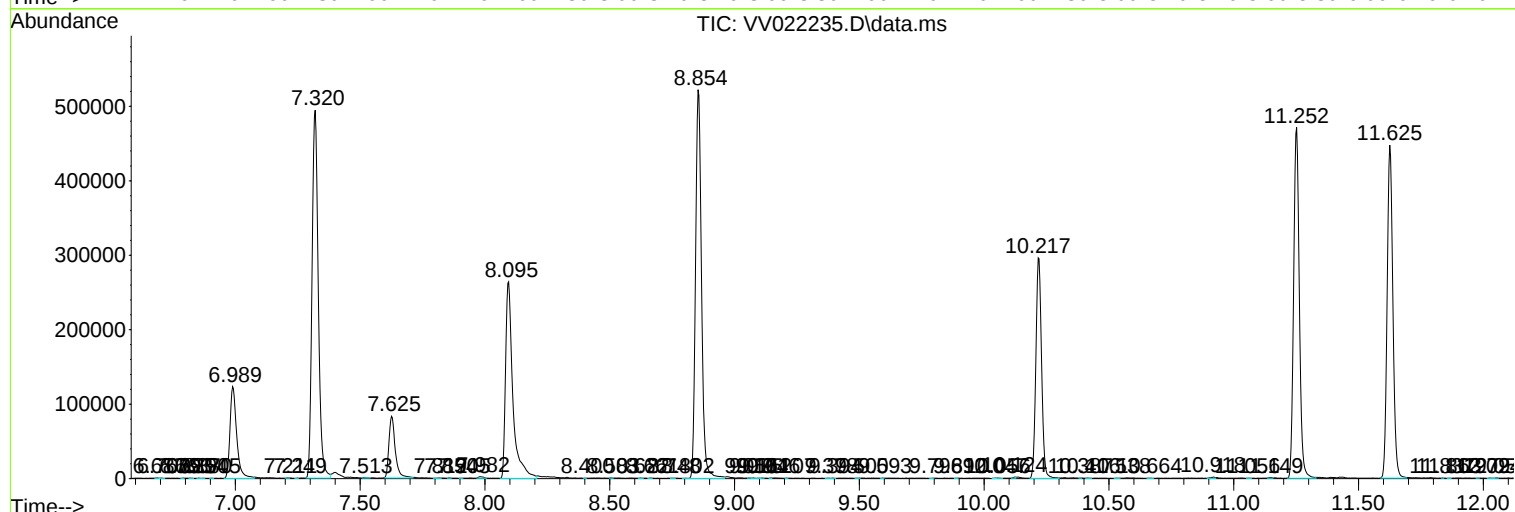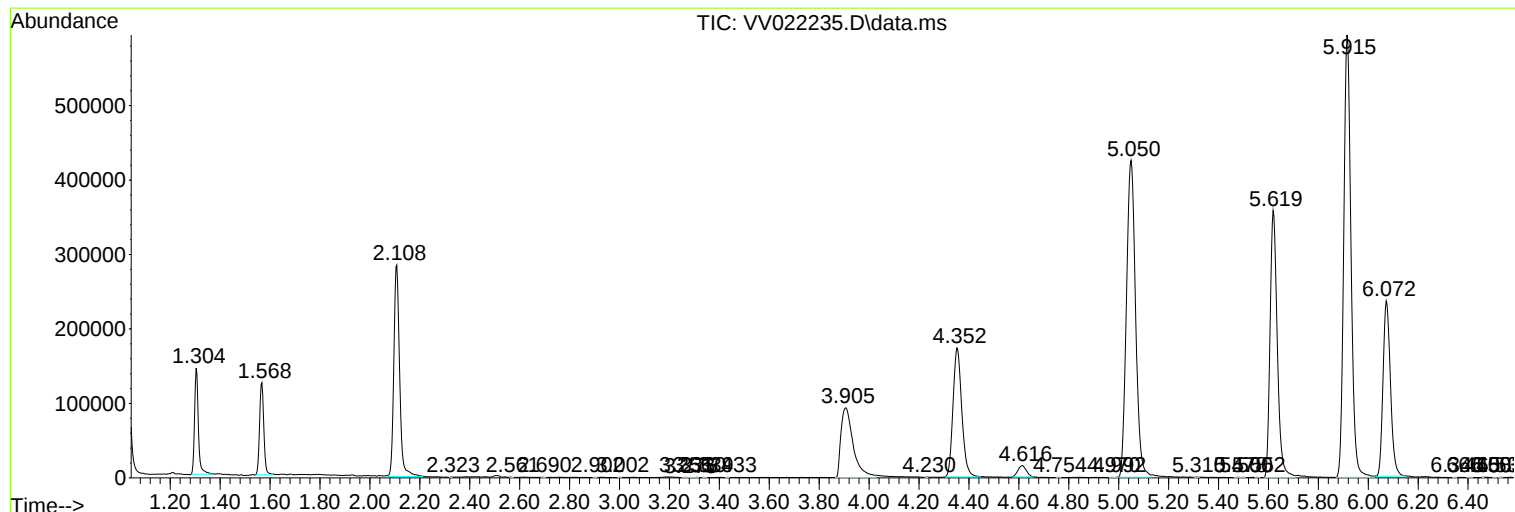

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022235.D
Acq On : 20 Sep 2021 16:15
Operator : SY/MD
Sample : M3788-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022235.D
Acq On : 20 Sep 2021 16:15
Operator : SY/MD
Sample : M3788-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
