

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022239.D
 Acq On : 20 Sep 2021 17:50
 Operator : SY/MD
 Sample : M3788-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022239.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rBV	142417	147930	13.62%	1.792%
2	1.568	156	164	175	rBV	124321	140798	12.96%	1.705%
3	2.105	322	331	353	rBV	261744	377002	34.71%	4.566%
4	2.635	493	496	498	rBV2	246	164	0.02%	0.002%
5	2.667	504	506	510	rVB	434	208	0.02%	0.003%
6	2.876	569	571	574	rVB3	495	257	0.02%	0.003%
7	2.950	587	594	596	rBV2	400	401	0.04%	0.005%
8	3.256	686	689	693	rVB2	201	119	0.01%	0.001%
9	3.310	702	706	707	rBV2	300	133	0.01%	0.002%
10	3.339	713	715	717	rBV	285	136	0.01%	0.002%
11	3.365	720	723	724	rVV2	180	107	0.01%	0.001%
12	3.465	751	754	757	rBV	181	110	0.01%	0.001%
13	3.564	782	785	787	rBV	178	131	0.01%	0.002%
14	3.590	791	793	797	rVB2	228	126	0.01%	0.002%
15	3.616	798	801	804	rBV2	214	148	0.01%	0.002%
16	3.664	814	816	819	rVB2	436	177	0.02%	0.002%
17	3.683	819	822	826	rBV	306	288	0.03%	0.003%
18	3.719	830	833	835	rBV	190	117	0.01%	0.001%
19	3.767	846	848	853	rVB2	320	181	0.02%	0.002%
20	3.899	879	889	925	rBV	71241	243745	22.44%	2.952%
21	4.352	1015	1030	1054	rBV2	170072	421882	38.84%	5.110%
22	4.683	1131	1133	1135	rBV3	227	104	0.01%	0.001%
23	4.812	1169	1173	1175	rBV	404	313	0.03%	0.004%
24	4.841	1179	1182	1185	rVB2	406	217	0.02%	0.003%
25	4.889	1193	1197	1199	rBV3	169	123	0.01%	0.001%
26	4.950	1214	1216	1218	rVB	385	166	0.02%	0.002%
27	5.050	1226	1247	1277	rBV2	431803	1086165	100.00%	13.156%
28	5.349	1336	1340	1342	rBV2	528	326	0.03%	0.004%
29	5.397	1353	1355	1356	rVB2	331	109	0.01%	0.001%
30	5.407	1356	1358	1362	rBV	300	247	0.02%	0.003%
31	5.465	1373	1376	1378	rBV	318	219	0.02%	0.003%
32	5.500	1385	1387	1390	rVB2	387	148	0.01%	0.002%
33	5.619	1412	1424	1469	rBV	349592	719324	66.23%	8.713%
34	5.908	1502	1514	1534	rBV5	35290	84566	7.79%	1.024%
35	6.072	1551	1565	1595	rBV	238154	489774	45.09%	5.932%
36	6.294	1632	1634	1637	rBV3	380	194	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022239.D
 Acq On : 20 Sep 2021 17:50
 Operator : SY/MD
 Sample : M3788-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.513	1697	1702	1703	rBV2	287	254	0.02%	0.003%
38	6.564	1714	1718	1721	rBV2	249	231	0.02%	0.003%
39	6.603	1728	1730	1734	rBV2	333	269	0.02%	0.003%
40	6.677	1749	1753	1754	rBV	373	270	0.02%	0.003%
41	6.793	1785	1789	1792	rBV	330	255	0.02%	0.003%
42	6.879	1812	1816	1818	rBV2	177	148	0.01%	0.002%
43	6.928	1828	1831	1834	rVB	391	195	0.02%	0.002%
44	6.950	1834	1838	1839	rBV2	272	187	0.02%	0.002%
45	6.989	1839	1850	1876	rBV	119001	222717	20.50%	2.698%
46	7.201	1914	1916	1919	rBV2	256	161	0.01%	0.002%
47	7.214	1919	1920	1930	rVB3	592	540	0.05%	0.007%
48	7.262	1930	1935	1936	rBV3	483	313	0.03%	0.004%
49	7.320	1941	1953	1970	rBV	493639	852542	78.49%	10.326%
50	7.625	2036	2048	2075	rBV	82357	149304	13.75%	1.808%
51	7.815	2105	2107	2109	rBV2	351	152	0.01%	0.002%
52	7.838	2112	2114	2116	rBV	229	132	0.01%	0.002%
53	7.870	2119	2124	2126	rBV2	393	330	0.03%	0.004%
54	7.976	2155	2157	2165	rVB4	948	938	0.09%	0.011%
55	8.034	2172	2175	2176	rBV	334	179	0.02%	0.002%
56	8.092	2183	2193	2227	rBV2	257785	525533	48.38%	6.365%
57	8.532	2329	2330	2336	rVB3	264	131	0.01%	0.002%
58	8.635	2359	2362	2367	rVB2	450	407	0.04%	0.005%
59	8.693	2377	2380	2384	rBV3	356	286	0.03%	0.003%
60	8.735	2390	2393	2396	rBV3	284	212	0.02%	0.003%
61	8.783	2404	2408	2410	rBV3	316	159	0.01%	0.002%
62	8.799	2410	2413	2416	rVB2	422	228	0.02%	0.003%
63	8.854	2418	2430	2451	rBV	527379	857127	78.91%	10.382%
64	9.101	2505	2507	2508	rBV	351	181	0.02%	0.002%
65	9.230	2543	2547	2550	rVB3	254	218	0.02%	0.003%
66	9.294	2563	2567	2570	rBV2	461	240	0.02%	0.003%
67	9.313	2571	2573	2576	rVB2	270	165	0.02%	0.002%
68	9.375	2588	2592	2594	rBV3	280	183	0.02%	0.002%
69	9.538	2639	2643	2646	rBV	224	201	0.02%	0.002%
70	9.558	2646	2649	2651	rBV3	423	221	0.02%	0.003%
71	9.603	2661	2663	2667	rVB	247	163	0.02%	0.002%
72	9.709	2692	2696	2698	rBV	160	142	0.01%	0.002%
73	9.735	2702	2704	2707	rVB	415	191	0.02%	0.002%
74	9.834	2732	2735	2737	rBV	317	186	0.02%	0.002%
75	9.966	2774	2776	2779	rVB	218	110	0.01%	0.001%
76	9.982	2779	2781	2786	rBV	218	128	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022239.D
 Acq On : 20 Sep 2021 17:50
 Operator : SY/MD
 Sample : M3788-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.027	2793	2795	2798	rBV2	259	187	0.02%	0.002%
78	10.088	2809	2814	2817	rBV	317	302	0.03%	0.004%
79	10.133	2821	2828	2837	rVB4	1780	2696	0.25%	0.033%
80	10.217	2843	2854	2875	rBV	287127	463483	42.67%	5.614%
81	10.355	2895	2897	2898	rBV2	338	121	0.01%	0.001%
82	10.365	2898	2900	2903	rVV2	206	142	0.01%	0.002%
83	10.522	2948	2949	2954	rVB2	257	135	0.01%	0.002%
84	10.571	2959	2964	2966	rBV3	361	306	0.03%	0.004%
85	10.606	2973	2975	2979	rVB2	296	161	0.01%	0.002%
86	10.670	2993	2995	2997	rBV	241	126	0.01%	0.002%
87	10.706	3002	3006	3008	rBV2	192	163	0.02%	0.002%
88	10.760	3021	3023	3026	rBV2	209	136	0.01%	0.002%
89	10.879	3057	3060	3063	rVB2	436	323	0.03%	0.004%
90	10.915	3063	3071	3073	rBV3	1443	1706	0.16%	0.021%
91	11.034	3106	3108	3110	rBV3	413	209	0.02%	0.003%
92	11.143	3140	3142	3144	rBV2	707	458	0.04%	0.006%
93	11.252	3164	3176	3199	rBV	474738	740853	68.21%	8.973%
94	11.487	3246	3249	3251	rBV	277	140	0.01%	0.002%
95	11.625	3281	3292	3314	rBV	451965	711645	65.52%	8.620%
96	11.825	3352	3354	3357	rBV2	390	272	0.03%	0.003%
97	11.992	3405	3406	3410	rBV2	240	128	0.01%	0.002%
98	12.371	3521	3524	3527	rBV2	342	218	0.02%	0.003%
99	13.333	3819	3823	3827	rVB	414	347	0.03%	0.004%
100	13.828	3974	3977	3979	rBV2	319	212	0.02%	0.003%




Sum of corrected areas: 8256153

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022239.D
Acq On : 20 Sep 2021 17:50
Operator : SY/MD
Sample : M3788-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

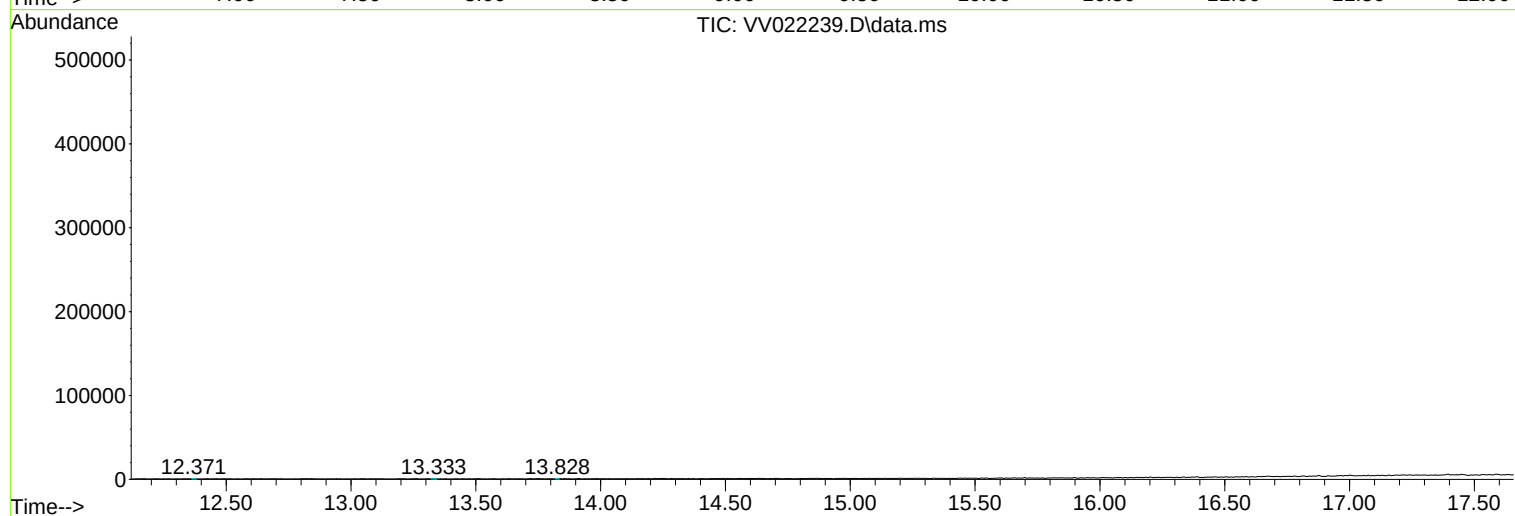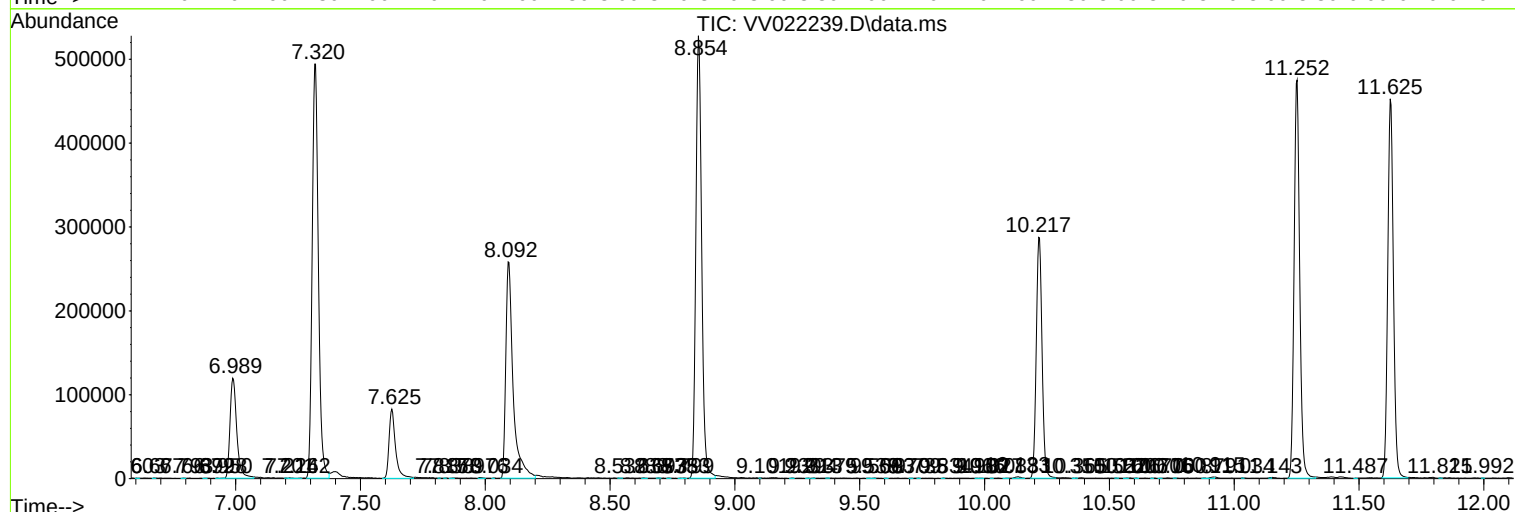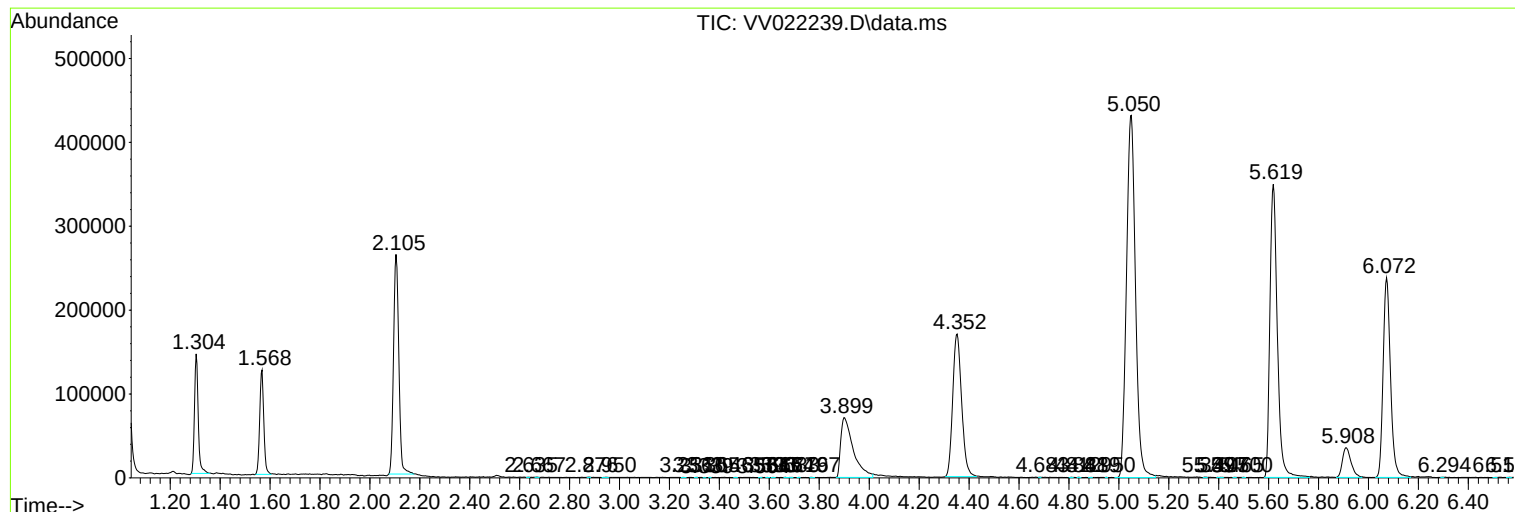

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022239.D
Acq On : 20 Sep 2021 17:50
Operator : SY/MD
Sample : M3788-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022239.D
Acq On : 20 Sep 2021 17:50
Operator : SY/MD
Sample : M3788-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
