

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022241.D
 Acq On : 20 Sep 2021 18:39
 Operator : SY/MD
 Sample : M3788-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022241.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rBV	139866	147458	13.69%	1.794%
2	1.564	156	163	177	rBV	122021	141138	13.11%	1.718%
3	2.105	321	331	361	rBV	261398	380365	35.32%	4.629%
4	2.719	518	522	527	rBV2	282	322	0.03%	0.004%
5	3.053	624	626	630	rVB	404	186	0.02%	0.002%
6	3.082	632	635	638	rBV2	243	158	0.01%	0.002%
7	3.185	663	667	670	rBV2	198	176	0.02%	0.002%
8	3.227	677	680	682	rBV2	204	138	0.01%	0.002%
9	3.420	737	740	744	rBV	181	159	0.01%	0.002%
10	3.574	783	788	790	rBV2	287	208	0.02%	0.003%
11	3.587	790	792	794	rVB2	274	131	0.01%	0.002%
12	3.606	794	798	801	rBV2	173	126	0.01%	0.002%
13	3.760	843	846	849	rBV2	241	182	0.02%	0.002%
14	3.844	869	872	876	rVB2	342	155	0.01%	0.002%
15	3.899	879	889	927	rBV2	75445	273034	25.35%	3.323%
16	4.349	1014	1029	1054	rBV	167981	417993	38.81%	5.087%
17	4.542	1085	1089	1093	rVB4	693	636	0.06%	0.008%
18	4.564	1093	1096	1099	rBV3	532	410	0.04%	0.005%
19	4.600	1104	1107	1109	rBV2	466	266	0.02%	0.003%
20	4.622	1111	1114	1116	rBV2	392	252	0.02%	0.003%
21	4.667	1125	1128	1131	rBV2	421	290	0.03%	0.004%
22	4.683	1131	1133	1136	rVB2	304	131	0.01%	0.002%
23	4.735	1146	1149	1156	rVB3	421	397	0.04%	0.005%
24	4.953	1213	1217	1220	rBV2	283	262	0.02%	0.003%
25	5.047	1229	1246	1279	rBV2	428029	1076978	100.00%	13.106%
26	5.265	1312	1314	1320	rVB2	621	505	0.05%	0.006%
27	5.400	1352	1356	1358	rVB2	204	157	0.01%	0.002%
28	5.413	1358	1360	1362	rBV2	298	143	0.01%	0.002%
29	5.452	1368	1372	1374	rBV2	263	197	0.02%	0.002%
30	5.490	1380	1384	1387	rBV3	371	326	0.03%	0.004%
31	5.538	1395	1399	1401	rBV3	346	232	0.02%	0.003%
32	5.619	1411	1424	1453	rBV	346768	701240	65.11%	8.534%
33	5.809	1481	1483	1486	rVB	678	322	0.03%	0.004%
34	5.828	1486	1489	1490	rBV	268	140	0.01%	0.002%
35	5.911	1502	1515	1542	rVB5	39580	94849	8.81%	1.154%
36	6.001	1542	1543	1546	rBV2	280	186	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022241.D
 Acq On : 20 Sep 2021 18:39
 Operator : SY/MD
 Sample : M3788-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.072	1551	1565	1588	rBV	236887	487430	45.26%	5.932%
38	6.333	1643	1646	1650	rBV	420	226	0.02%	0.003%
39	6.513	1700	1702	1705	rBV	228	139	0.01%	0.002%
40	6.529	1705	1707	1711	rVB2	373	219	0.02%	0.003%
41	6.577	1719	1722	1725	rVB2	423	277	0.03%	0.003%
42	6.606	1725	1731	1735	rBV	227	241	0.02%	0.003%
43	6.667	1746	1750	1753	rBV2	557	476	0.04%	0.006%
44	6.709	1759	1763	1767	rVB2	463	343	0.03%	0.004%
45	6.770	1779	1782	1786	rBV3	208	152	0.01%	0.002%
46	6.805	1791	1793	1797	rVB	360	204	0.02%	0.002%
47	6.989	1839	1850	1866	rBV	117921	214995	19.96%	2.616%
48	7.230	1921	1925	1931	rVB4	581	613	0.06%	0.007%
49	7.259	1932	1934	1937	rBV	285	133	0.01%	0.002%
50	7.317	1940	1952	1972	rBV	483207	843147	78.29%	10.261%
51	7.625	2036	2048	2069	rBV	80772	145091	13.47%	1.766%
52	7.847	2115	2117	2120	rBV	373	196	0.02%	0.002%
53	7.866	2120	2123	2125	rVV	269	138	0.01%	0.002%
54	7.972	2152	2156	2157	rBV2	166	126	0.01%	0.002%
55	8.011	2166	2168	2172	rVB	290	145	0.01%	0.002%
56	8.050	2176	2180	2181	rBV	273	161	0.01%	0.002%
57	8.095	2184	2194	2231	rBV2	258812	530940	49.30%	6.461%
58	8.371	2277	2280	2285	rBV3	513	460	0.04%	0.006%
59	8.574	2339	2343	2344	rBV	250	178	0.02%	0.002%
60	8.664	2368	2371	2375	rVB3	367	252	0.02%	0.003%
61	8.683	2375	2377	2381	rBV2	266	162	0.02%	0.002%
62	8.741	2393	2395	2401	rVB2	407	341	0.03%	0.004%
63	8.773	2402	2405	2409	rBV2	339	232	0.02%	0.003%
64	8.853	2417	2430	2458	rBV	515762	847758	78.72%	10.317%
65	9.027	2479	2484	2486	rBV2	677	631	0.06%	0.008%
66	9.062	2492	2495	2496	rBV	352	182	0.02%	0.002%
67	9.214	2536	2542	2547	rBV2	313	318	0.03%	0.004%
68	9.352	2578	2585	2586	rBV	328	275	0.03%	0.003%
69	9.381	2592	2594	2597	rVB	349	147	0.01%	0.002%
70	9.554	2646	2648	2653	rVV2	315	218	0.02%	0.003%
71	9.580	2654	2656	2660	rVB2	328	160	0.01%	0.002%
72	9.657	2677	2680	2683	rVB2	246	131	0.01%	0.002%
73	9.847	2737	2739	2741	rBV2	225	137	0.01%	0.002%
74	9.860	2741	2743	2746	rVB	345	169	0.02%	0.002%
75	9.915	2756	2760	2762	rBV	187	141	0.01%	0.002%
76	10.127	2820	2826	2835	rBV5	1495	2125	0.20%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022241.D
 Acq On : 20 Sep 2021 18:39
 Operator : SY/MD
 Sample : M3788-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.217	2843	2854	2873	rBV	289613	462736	42.97%	5.631%
78	10.339	2891	2892	2895	rBV2	281	136	0.01%	0.002%
79	10.355	2895	2897	2899	rBV	400	188	0.02%	0.002%
80	10.455	2926	2928	2932	rVB3	249	191	0.02%	0.002%
81	10.484	2932	2937	2939	rBV3	226	198	0.02%	0.002%
82	10.580	2964	2967	2968	rBV2	353	202	0.02%	0.002%
83	10.876	3055	3059	3062	rBV	209	193	0.02%	0.002%
84	10.921	3065	3073	3081	rVB6	1200	2174	0.20%	0.026%
85	11.252	3164	3176	3196	rBV	461004	721307	66.98%	8.778%
86	11.525	3259	3261	3264	rBV3	233	134	0.01%	0.002%
87	11.545	3264	3267	3272	rBV3	610	508	0.05%	0.006%
88	11.625	3281	3292	3318	rBV	440508	706601	65.61%	8.599%
89	11.869	3365	3368	3370	rBV	371	280	0.03%	0.003%
90	11.953	3392	3394	3398	rBV3	345	221	0.02%	0.003%
91	12.098	3436	3439	3445	rVB2	654	546	0.05%	0.007%
92	12.246	3479	3485	3488	rBV2	273	263	0.02%	0.003%
93	12.262	3488	3490	3495	rVV3	314	234	0.02%	0.003%
94	12.583	3584	3590	3594	rBV3	274	408	0.04%	0.005%
95	13.011	3719	3723	3727	rVB3	349	275	0.03%	0.003%
96	13.033	3727	3730	3736	rBV3	341	260	0.02%	0.003%
97	13.416	3846	3849	3852	rBV2	437	295	0.03%	0.004%
98	13.680	3926	3931	3933	rBV2	350	327	0.03%	0.004%
99	14.229	4099	4102	4105	rBV	505	280	0.03%	0.003%
100	14.512	4188	4190	4192	rBV3	388	151	0.01%	0.002%




Sum of corrected areas: 8217365

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022241.D
Acq On : 20 Sep 2021 18:39
Operator : SY/MD
Sample : M3788-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

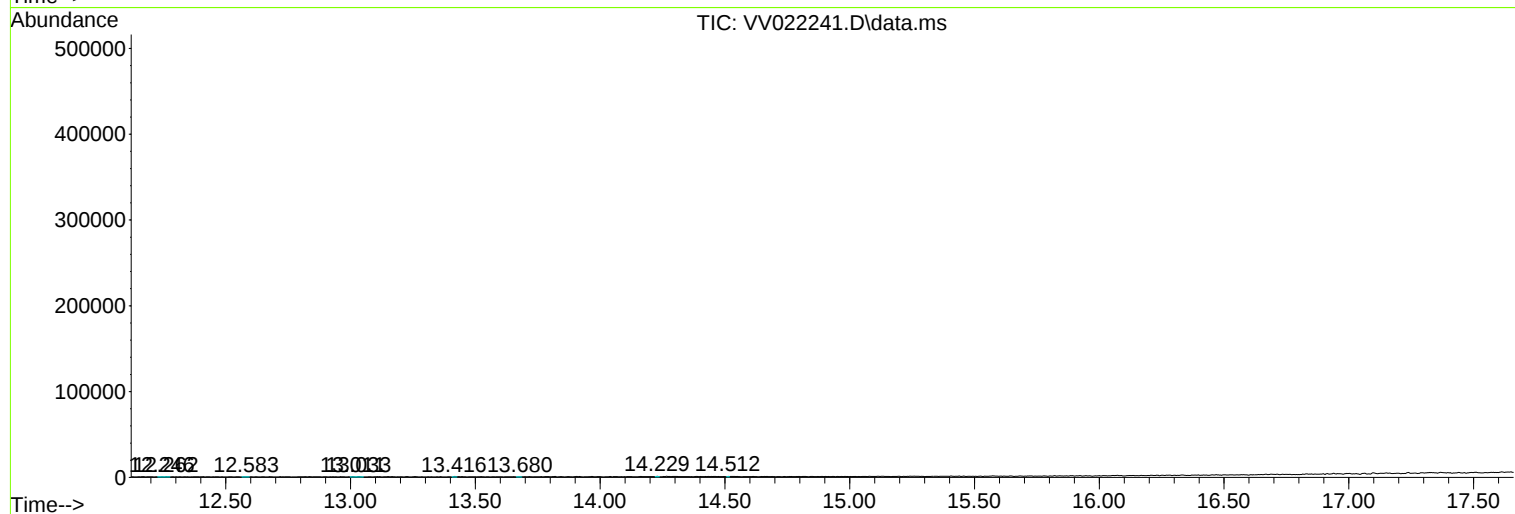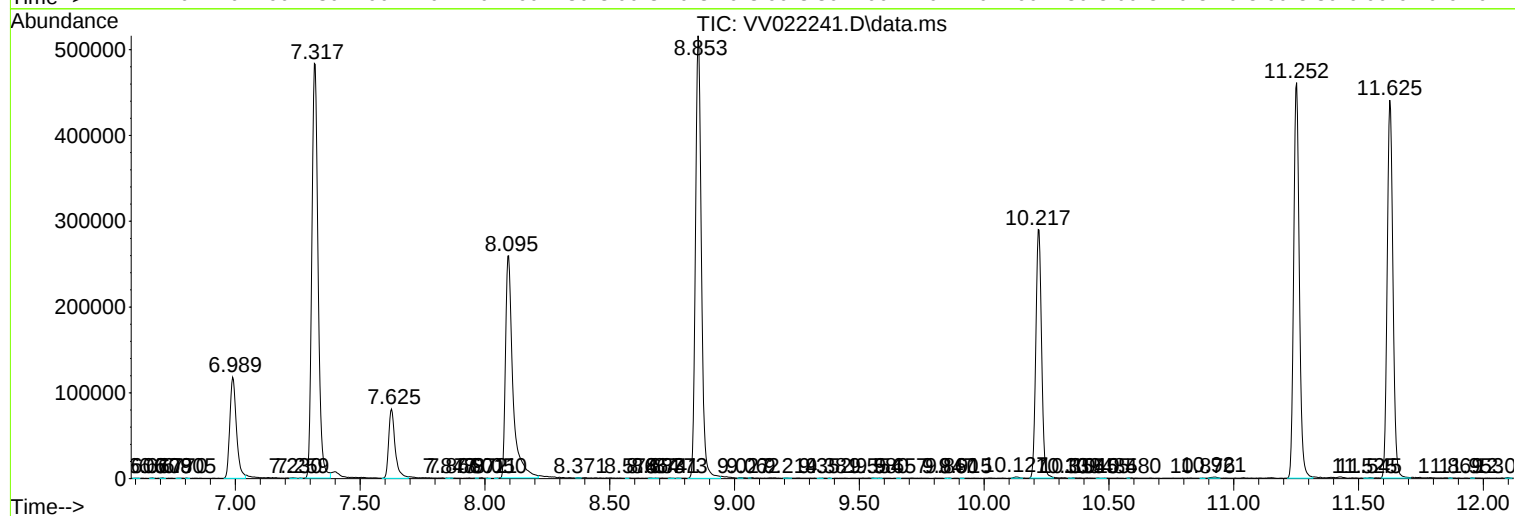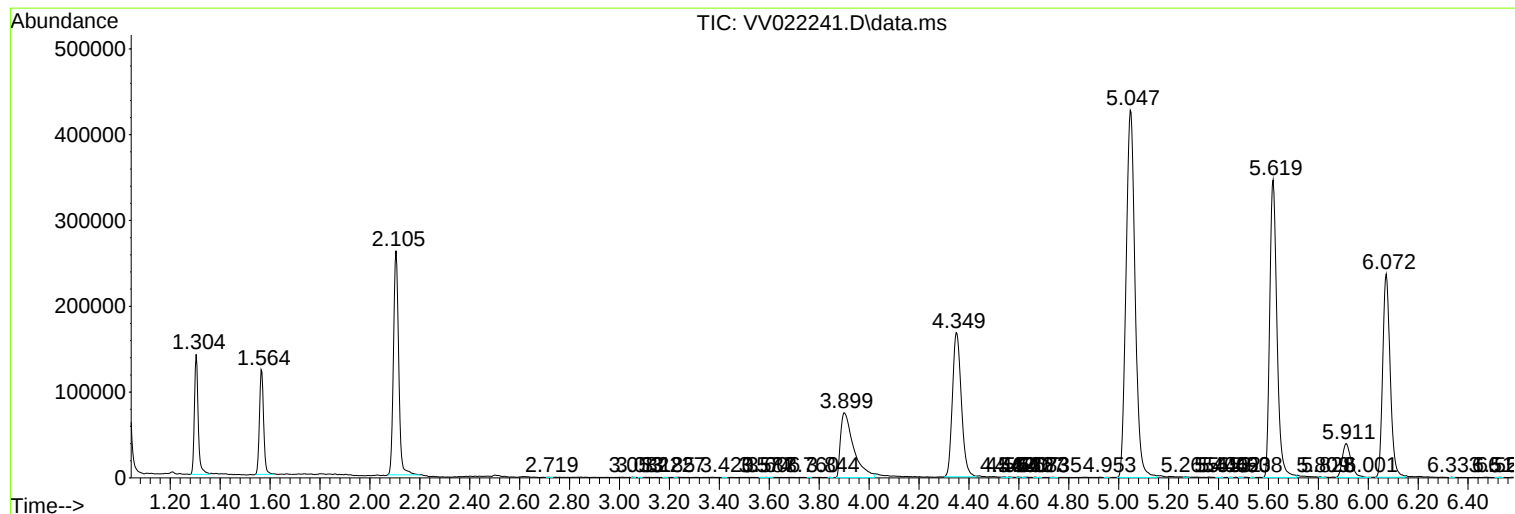

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022241.D
Acq On : 20 Sep 2021 18:39
Operator : SY/MD
Sample : M3788-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022241.D
Acq On : 20 Sep 2021 18:39
Operator : SY/MD
Sample : M3788-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------