

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022242.D
 Acq On : 20 Sep 2021 19:03
 Operator : SY/MD
 Sample : M3788-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CLO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022242.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	102	rVB	139131	148067	14.12%	1.835%
2	1.564	157	163	175	rVB	119498	138100	13.17%	1.712%
3	2.105	322	331	361	rVB	258362	384485	36.67%	4.766%
4	2.394	419	421	422	rBV	295	120	0.01%	0.001%
5	2.574	473	477	480	rBV2	305	189	0.02%	0.002%
6	2.635	493	496	500	rVB2	316	234	0.02%	0.003%
7	2.664	503	505	509	rVB	421	223	0.02%	0.003%
8	2.941	588	591	595	rBV2	438	241	0.02%	0.003%
9	3.034	618	620	622	rBV	319	157	0.01%	0.002%
10	3.085	633	636	639	rBV2	359	258	0.02%	0.003%
11	3.137	651	652	653	rBV	314	110	0.01%	0.001%
12	3.185	665	667	668	rBV	336	152	0.01%	0.002%
13	3.240	681	684	692	rVB2	292	333	0.03%	0.004%
14	3.378	723	727	732	rBV2	621	470	0.04%	0.006%
15	3.526	770	773	775	rBV2	274	166	0.02%	0.002%
16	3.622	799	803	805	rBV	278	186	0.02%	0.002%
17	3.658	811	814	817	rVB	211	146	0.01%	0.002%
18	3.725	832	835	837	rBV	228	134	0.01%	0.002%
19	3.770	847	849	853	rVB2	196	104	0.01%	0.001%
20	3.902	879	890	936	rBV2	73108	260152	24.81%	3.224%
21	4.349	1015	1029	1062	rBV	167436	410293	39.13%	5.085%
22	4.725	1141	1146	1150	rBV3	278	307	0.03%	0.004%
23	4.767	1154	1159	1161	rBV3	383	294	0.03%	0.004%
24	4.851	1179	1185	1188	rBV3	779	646	0.06%	0.008%
25	4.992	1226	1229	1230	rBV3	288	146	0.01%	0.002%
26	5.050	1230	1247	1278	rBV2	415770	1048611	100.00%	12.997%
27	5.297	1322	1324	1325	rBV2	436	198	0.02%	0.002%
28	5.410	1356	1359	1362	rVB3	340	154	0.01%	0.002%
29	5.506	1387	1389	1392	rVB2	343	187	0.02%	0.002%
30	5.529	1392	1396	1401	rBV2	467	382	0.04%	0.005%
31	5.619	1411	1424	1452	rBV	338873	689465	65.75%	8.546%
32	5.912	1503	1515	1534	rBV5	46550	112076	10.69%	1.389%
33	6.072	1550	1565	1591	rBV	226897	471151	44.93%	5.840%
34	6.243	1616	1618	1619	rBV	392	163	0.02%	0.002%
35	6.313	1636	1640	1642	rBV	360	246	0.02%	0.003%
36	6.333	1644	1646	1647	rVV	393	154	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022242.D
 Acq On : 20 Sep 2021 19:03
 Operator : SY/MD
 Sample : M3788-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CLO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.371	1656	1658	1660	rBV3	301	150	0.01%	0.002%
38	6.494	1693	1696	1699	rBV	154	111	0.01%	0.001%
39	6.535	1704	1709	1712	rVB	414	319	0.03%	0.004%
40	6.686	1753	1756	1758	rBV	385	216	0.02%	0.003%
41	6.719	1764	1766	1771	rVB2	405	167	0.02%	0.002%
42	6.908	1823	1825	1831	rVB	204	130	0.01%	0.002%
43	6.940	1831	1835	1837	rBV2	247	207	0.02%	0.003%
44	6.989	1839	1850	1875	rBV	115125	213348	20.35%	2.644%
45	7.217	1920	1921	1923	rVB	530	152	0.01%	0.002%
46	7.268	1935	1937	1939	rBV	310	155	0.01%	0.002%
47	7.317	1940	1952	1972	rBV	472896	823313	78.51%	10.205%
48	7.625	2038	2048	2072	rBV	78662	142060	13.55%	1.761%
49	7.863	2120	2122	2124	rVB2	394	154	0.01%	0.002%
50	7.876	2124	2126	2131	rVB3	451	307	0.03%	0.004%
51	7.905	2131	2135	2140	rBV2	397	293	0.03%	0.004%
52	7.937	2143	2145	2148	rBV2	328	176	0.02%	0.002%
53	7.985	2158	2160	2166	rVB3	672	536	0.05%	0.007%
54	8.011	2166	2168	2170	rVB	312	131	0.01%	0.002%
55	8.030	2170	2174	2177	rBV3	457	329	0.03%	0.004%
56	8.095	2183	2194	2232	rBV2	252353	516076	49.22%	6.397%
57	8.342	2268	2271	2274	rBV3	598	425	0.04%	0.005%
58	8.625	2357	2359	2361	rBV	292	109	0.01%	0.001%
59	8.683	2374	2377	2379	rBV	276	151	0.01%	0.002%
60	8.696	2379	2381	2383	rVB	258	112	0.01%	0.001%
61	8.789	2407	2410	2413	rBV2	282	166	0.02%	0.002%
62	8.854	2418	2430	2454	rBV	516530	832146	79.36%	10.314%
63	9.037	2483	2487	2491	rVB3	800	522	0.05%	0.006%
64	9.217	2539	2543	2549	rVB4	576	575	0.05%	0.007%
65	9.349	2582	2584	2587	rBV2	244	109	0.01%	0.001%
66	9.378	2590	2593	2596	rVB3	400	287	0.03%	0.004%
67	9.426	2605	2608	2611	rBV	264	207	0.02%	0.003%
68	9.468	2616	2621	2624	rBV2	408	308	0.03%	0.004%
69	9.715	2695	2698	2701	rBV2	361	203	0.02%	0.003%
70	9.847	2736	2739	2740	rBV2	209	127	0.01%	0.002%
71	9.921	2760	2762	2764	rBV	211	104	0.01%	0.001%
72	10.034	2795	2797	2801	rBV2	182	115	0.01%	0.001%
73	10.069	2806	2808	2812	rBV2	176	105	0.01%	0.001%
74	10.127	2819	2826	2838	rBV4	1294	2472	0.24%	0.031%
75	10.217	2843	2854	2873	rBV	282547	453011	43.20%	5.615%
76	10.342	2891	2893	2898	rVB3	489	362	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022242.D
 Acq On : 20 Sep 2021 19:03
 Operator : SY/MD
 Sample : M3788-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CLO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.416	2912	2916	2917	rBV2	344	277	0.03%	0.003%
78	10.513	2944	2946	2950	rBV2	194	107	0.01%	0.001%
79	10.542	2954	2955	2959	rVB2	336	192	0.02%	0.002%
80	10.564	2959	2962	2963	rBV	259	142	0.01%	0.002%
81	10.577	2963	2966	2967	rBV	426	186	0.02%	0.002%
82	10.648	2987	2988	2991	rBV2	279	159	0.02%	0.002%
83	10.693	2999	3002	3004	rBV	265	159	0.02%	0.002%
84	10.706	3004	3006	3009	rVB	247	112	0.01%	0.001%
85	10.754	3019	3021	3024	rBV2	258	151	0.01%	0.002%
86	10.818	3037	3041	3045	rVB2	422	301	0.03%	0.004%
87	10.921	3067	3073	3082	rVB5	1262	2003	0.19%	0.025%
88	11.043	3109	3111	3114	rVB2	504	202	0.02%	0.003%
89	11.210	3160	3163	3164	rBV2	444	179	0.02%	0.002%
90	11.252	3164	3176	3196	rVV	461247	711811	67.88%	8.823%
91	11.564	3271	3273	3277	rVB2	492	242	0.02%	0.003%
92	11.583	3277	3279	3280	rBV	270	148	0.01%	0.002%
93	11.625	3280	3292	3317	rVV	434895	691503	65.94%	8.571%
94	11.844	3358	3360	3367	rVB3	320	323	0.03%	0.004%
95	11.927	3384	3386	3388	rBV	237	130	0.01%	0.002%
96	12.172	3460	3462	3466	rBV2	322	193	0.02%	0.002%
97	12.622	3600	3602	3604	rBV2	246	131	0.01%	0.002%
98	12.834	3666	3668	3671	rBV2	408	225	0.02%	0.003%
99	13.140	3760	3763	3767	rBV2	302	258	0.02%	0.003%
100	13.365	3829	3833	3839	rBV	565	478	0.05%	0.006%




Sum of corrected areas: 8068058

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022242.D
Acq On : 20 Sep 2021 19:03
Operator : SY/MD
Sample : M3788-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CLO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

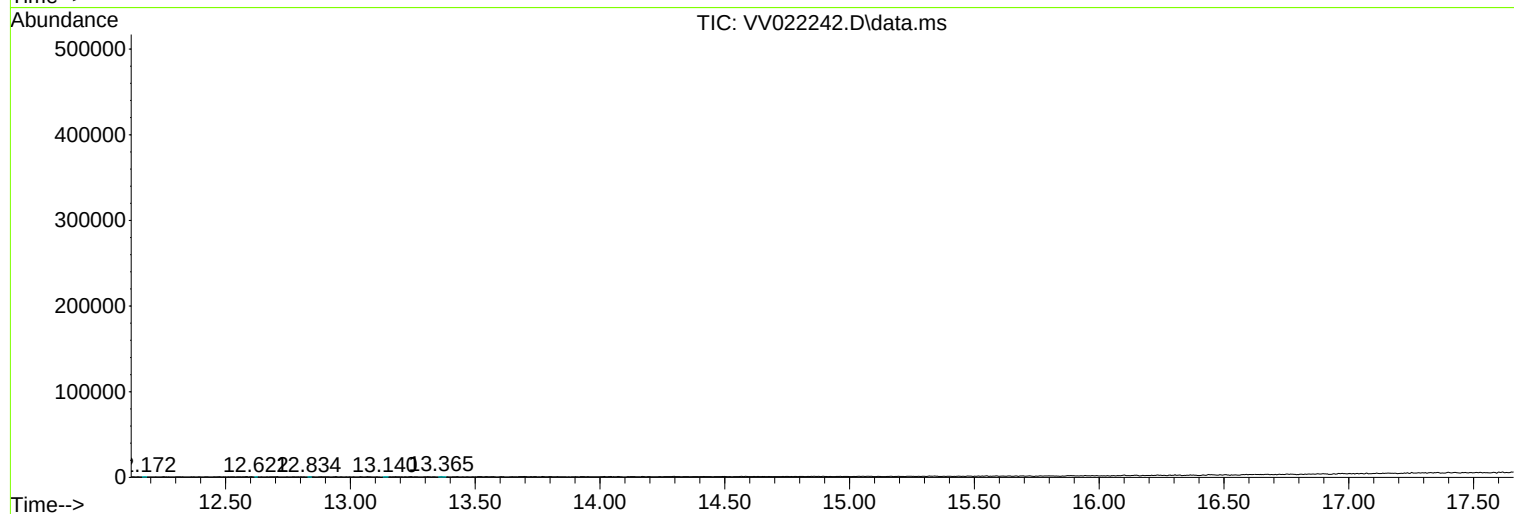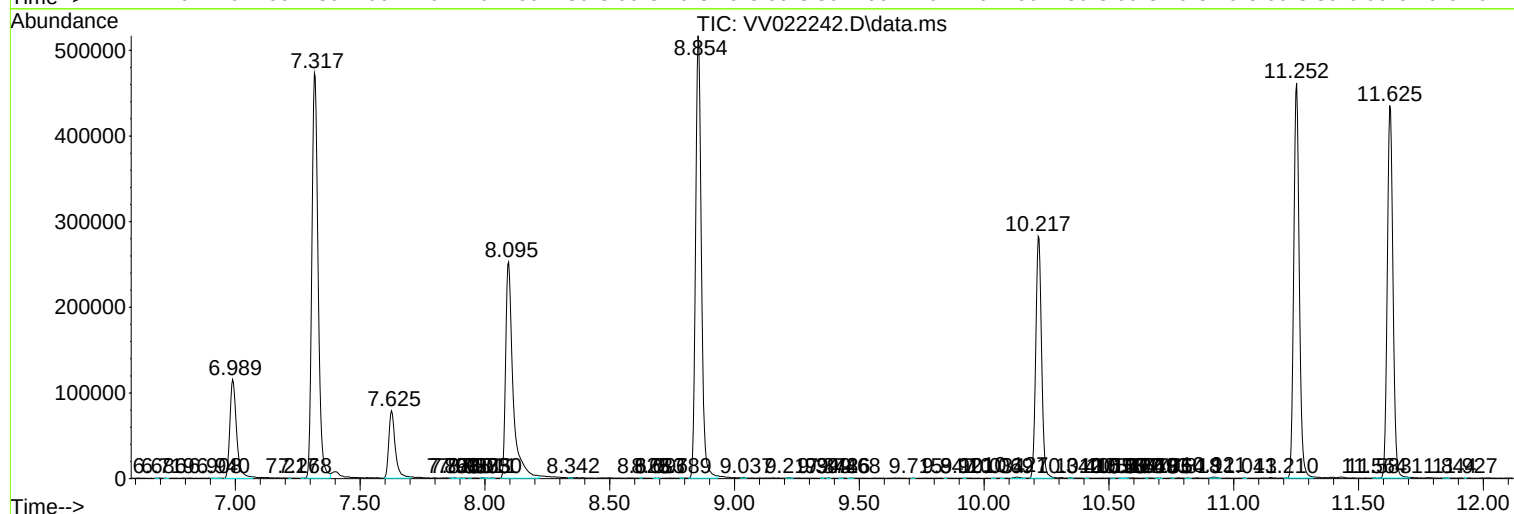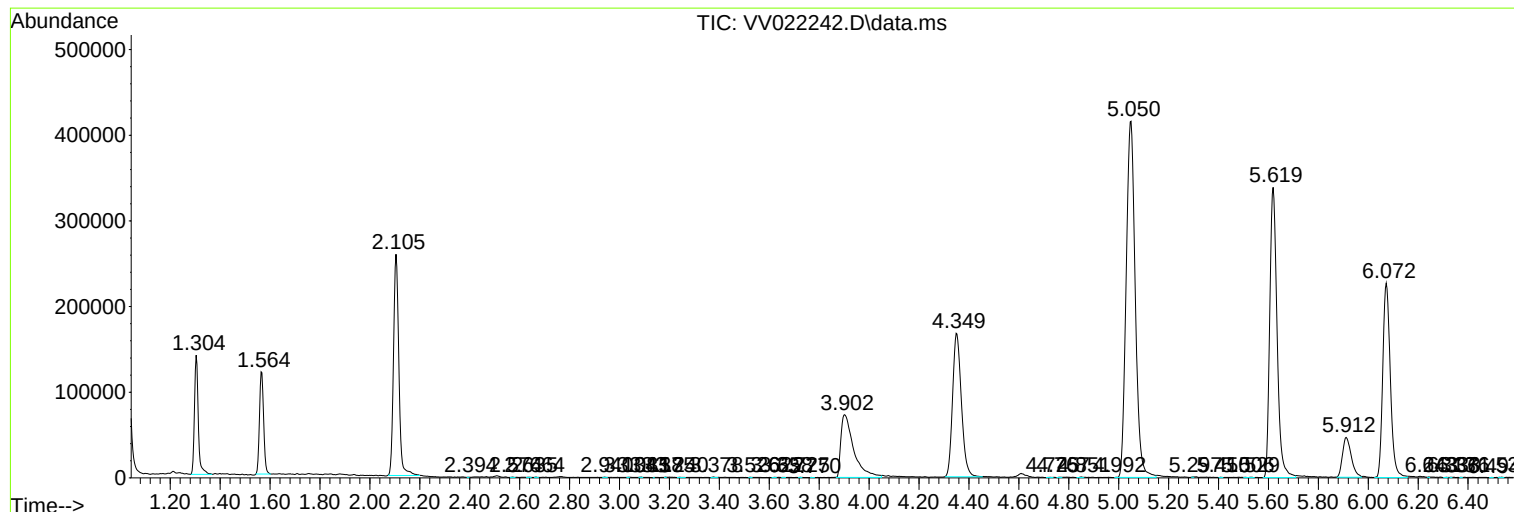

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022242.D
Acq On : 20 Sep 2021 19:03
Operator : SY/MD
Sample : M3788-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CLO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022242.D
Acq On : 20 Sep 2021 19:03
Operator : SY/MD
Sample : M3788-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CLO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------