

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022250.D
 Acq On : 20 Sep 2021 22:39
 Operator : SY/MD
 Sample : M3788-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022250.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	103	rVB	143853	148002	7.06%	1.512%
2	1.568	156	164	178	rVB	113560	131032	6.25%	1.339%
3	2.108	322	332	345	rBV3	281362	442628	21.12%	4.523%
4	2.651	498	501	505	rBV3	388	310	0.01%	0.003%
5	2.912	578	582	583	rBV	218	145	0.01%	0.001%
6	2.944	589	592	593	rBV	283	167	0.01%	0.002%
7	3.066	626	630	631	rBV2	322	192	0.01%	0.002%
8	3.105	640	642	645	rBV	187	121	0.01%	0.001%
9	3.124	645	648	653	rVB3	270	203	0.01%	0.002%
10	3.198	662	671	684	rVB9	2055	3889	0.19%	0.040%
11	3.265	684	692	697	rBV4	356	485	0.02%	0.005%
12	3.323	708	710	714	rBV2	287	196	0.01%	0.002%
13	3.474	754	757	759	rBV2	148	100	0.00%	0.001%
14	3.494	759	763	765	rVV3	440	274	0.01%	0.003%
15	3.506	765	767	771	rVB2	211	128	0.01%	0.001%
16	3.561	782	784	787	rBV	272	129	0.01%	0.001%
17	3.577	787	789	793	rVV2	344	167	0.01%	0.002%
18	3.658	812	814	819	rBV	282	203	0.01%	0.002%
19	3.683	819	822	826	rVV3	198	164	0.01%	0.002%
20	3.841	864	871	872	rBB3	281	237	0.01%	0.002%
21	3.912	880	893	926	rBV3	99828	334019	15.94%	3.413%
22	4.352	1013	1030	1061	rBV	151671	384673	18.36%	3.931%
23	4.555	1090	1093	1094	rBV	357	215	0.01%	0.002%
24	4.712	1139	1142	1144	rVV2	471	234	0.01%	0.002%
25	4.738	1148	1150	1153	rVB2	443	187	0.01%	0.002%
26	4.767	1157	1159	1163	rVB	167	89	0.00%	0.001%
27	4.895	1196	1199	1201	rBV2	285	183	0.01%	0.002%
28	4.986	1223	1227	1229	rBV2	205	162	0.01%	0.002%
29	5.050	1229	1247	1274	rBV2	379303	959249	45.78%	9.802%
30	5.342	1333	1338	1341	rBV2	393	416	0.02%	0.004%
31	5.355	1341	1342	1346	rBV2	366	224	0.01%	0.002%
32	5.394	1351	1354	1355	rBV	324	206	0.01%	0.002%
33	5.500	1384	1387	1392	rVB3	655	615	0.03%	0.006%
34	5.555	1398	1404	1406	rBV2	352	322	0.02%	0.003%
35	5.619	1411	1424	1451	rBV	340743	693708	33.11%	7.089%
36	5.821	1484	1487	1489	rBV3	436	287	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022250.D
 Acq On : 20 Sep 2021 22:39
 Operator : SY/MD
 Sample : M3788-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	5.915	1501	1516	1545	rBV	1068265	2095374	100.00%	21.412%
38	6.072	1554	1565	1587	rVB	212047	427146	20.39%	4.365%
39	6.275	1626	1628	1632	rBV3	556	325	0.02%	0.003%
40	6.400	1664	1667	1669	rBV3	355	189	0.01%	0.002%
41	6.432	1674	1677	1679	rBV	241	203	0.01%	0.002%
42	6.481	1690	1692	1694	rBV	244	129	0.01%	0.001%
43	6.654	1743	1746	1748	rVV3	575	303	0.01%	0.003%
44	6.754	1774	1777	1783	rBV3	335	264	0.01%	0.003%
45	6.809	1791	1794	1795	rBV	254	133	0.01%	0.001%
46	6.944	1834	1836	1837	rBV	257	94	0.00%	0.001%
47	6.989	1840	1850	1880	rVV	103088	193502	9.23%	1.977%
48	7.265	1934	1936	1939	rVB3	196	107	0.01%	0.001%
49	7.320	1941	1953	1970	rBV	434909	763347	36.43%	7.800%
50	7.625	2038	2048	2072	rBV	70918	126416	6.03%	1.292%
51	7.776	2093	2095	2096	rBV	569	273	0.01%	0.003%
52	7.854	2112	2119	2130	rVB8	1178	2033	0.10%	0.021%
53	7.989	2155	2161	2169	rBV6	892	1263	0.06%	0.013%
54	8.095	2184	2194	2232	rBV2	222426	462489	22.07%	4.726%
55	8.545	2331	2334	2335	rBV	255	140	0.01%	0.001%
56	8.667	2370	2372	2377	rBV3	325	244	0.01%	0.002%
57	8.693	2377	2380	2383	rBV2	389	255	0.01%	0.003%
58	8.731	2388	2392	2393	rBV2	381	210	0.01%	0.002%
59	8.783	2405	2408	2411	rBB	252	126	0.01%	0.001%
60	8.799	2411	2413	2414	rBV	246	104	0.00%	0.001%
61	8.854	2419	2430	2455	rBV	520328	834588	39.83%	8.528%
62	9.088	2497	2503	2504	rBV3	496	477	0.02%	0.005%
63	9.281	2560	2563	2566	rVB	315	225	0.01%	0.002%
64	9.307	2566	2571	2576	rVB4	428	495	0.02%	0.005%
65	9.342	2580	2582	2584	rVB2	292	116	0.01%	0.001%
66	9.362	2586	2588	2591	rVB	354	144	0.01%	0.001%
67	9.413	2602	2604	2609	rBV2	219	116	0.01%	0.001%
68	9.439	2609	2612	2614	rBV2	185	130	0.01%	0.001%
69	9.484	2625	2626	2628	rBV2	224	125	0.01%	0.001%
70	9.850	2737	2740	2745	rVB	281	197	0.01%	0.002%
71	9.972	2775	2778	2784	rVB2	320	299	0.01%	0.003%
72	10.001	2784	2787	2789	rBV	205	150	0.01%	0.002%
73	10.050	2798	2802	2804	rBV2	277	196	0.01%	0.002%
74	10.127	2818	2826	2832	rBV5	1688	2135	0.10%	0.022%
75	10.217	2842	2854	2872	rBV	250388	404859	19.32%	4.137%
76	10.435	2919	2922	2924	rVB2	235	107	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022250.D
 Acq On : 20 Sep 2021 22:39
 Operator : SY/MD
 Sample : M3788-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.452	2925	2927	2931	rVB2	269	150	0.01%	0.002%
78	10.477	2931	2935	2937	rBV2	306	211	0.01%	0.002%
79	10.542	2953	2955	2957	rVB	318	127	0.01%	0.001%
80	10.580	2963	2967	2971	rVB3	340	331	0.02%	0.003%
81	10.603	2971	2974	2979	rBV3	341	342	0.02%	0.003%
82	10.628	2979	2982	2985	rBV2	350	246	0.01%	0.003%
83	10.815	3038	3040	3044	rVB2	382	191	0.01%	0.002%
84	10.844	3046	3049	3050	rBV	382	166	0.01%	0.002%
85	10.882	3056	3061	3064	rBV3	344	198	0.01%	0.002%
86	10.924	3065	3074	3080	rVV5	1671	2330	0.11%	0.024%
87	11.075	3119	3121	3124	rBV2	343	145	0.01%	0.001%
88	11.191	3154	3157	3162	rVB	365	256	0.01%	0.003%
89	11.252	3164	3176	3199	rBV	463795	723598	34.53%	7.394%
90	11.574	3272	3276	3279	rBV3	637	441	0.02%	0.005%
91	11.625	3281	3292	3317	rVV	393446	632065	30.16%	6.459%
92	11.789	3339	3343	3346	rBV3	660	470	0.02%	0.005%
93	11.834	3354	3357	3358	rBV	276	161	0.01%	0.002%
94	11.844	3358	3360	3364	rVV3	475	305	0.01%	0.003%
95	12.056	3424	3426	3429	rVB2	352	156	0.01%	0.002%
96	12.458	3547	3551	3558	rBV3	294	458	0.02%	0.005%
97	12.969	3708	3710	3713	rBV	404	239	0.01%	0.002%
98	13.558	3890	3893	3896	rVB	563	330	0.02%	0.003%
99	14.101	4060	4062	4064	rBV	369	204	0.01%	0.002%
100	14.149	4074	4077	4079	rBV2	417	300	0.01%	0.003%




Sum of corrected areas: 9786009

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022250.D
Acq On : 20 Sep 2021 22:39
Operator : SY/MD
Sample : M3788-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

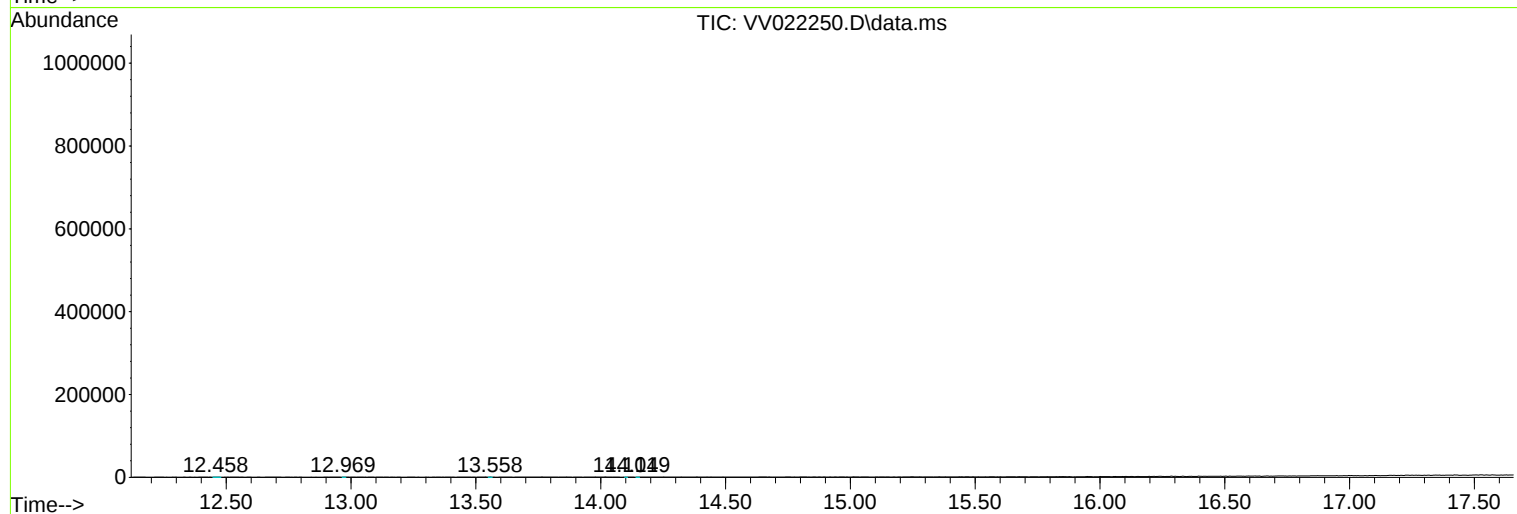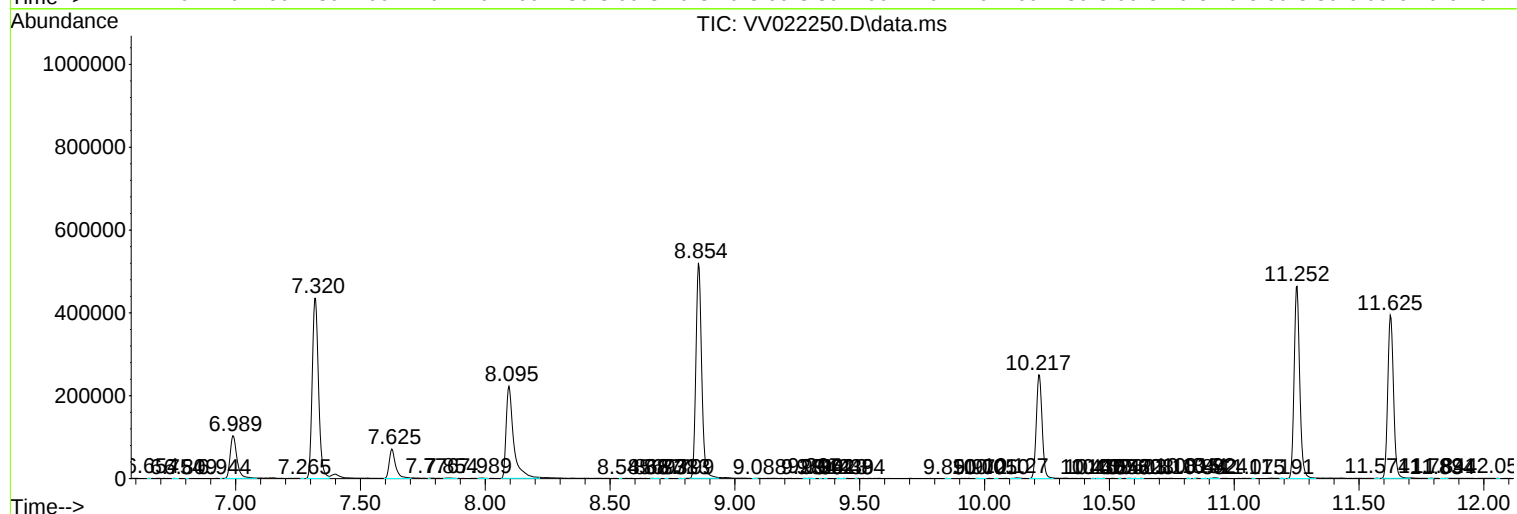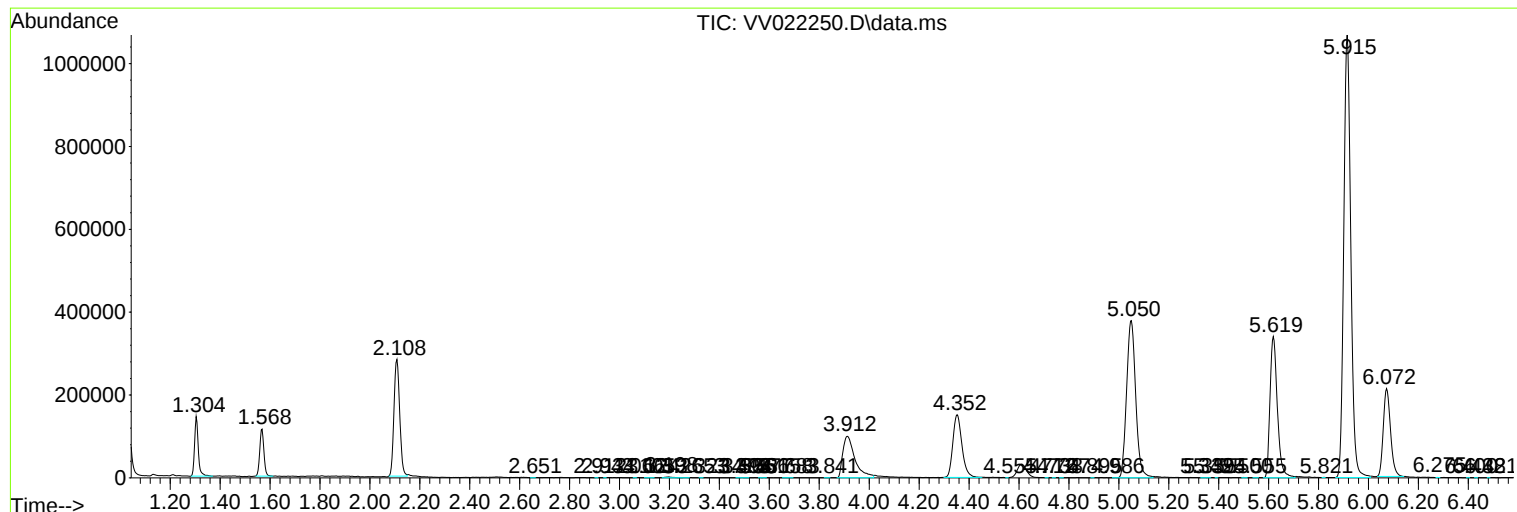

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022250.D
Acq On : 20 Sep 2021 22:39
Operator : SY/MD
Sample : M3788-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022250.D
Acq On : 20 Sep 2021 22:39
Operator : SY/MD
Sample : M3788-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
