

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022263.D
 Acq On : 21 Sep 2021 03:50
 Operator : SY/MD
 Sample : M3778-01DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E4585DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022263.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	141812	149365	10.79%	1.514%
2	1.565	157	163	176	rVB	121448	142119	10.27%	1.441%
3	2.101	321	330	351	rVB	269328	379060	27.38%	3.843%
4	2.503	446	455	472	rVB2	29461	50746	3.67%	0.514%
5	2.677	508	509	514	rBV2	461	251	0.02%	0.003%
6	2.757	530	534	535	rBV4	972	644	0.05%	0.007%
7	2.867	564	568	571	rBV2	276	269	0.02%	0.003%
8	2.973	597	601	602	rBV2	281	174	0.01%	0.002%
9	3.011	611	613	616	rVB	336	166	0.01%	0.002%
10	3.063	625	629	635	rVB2	427	399	0.03%	0.004%
11	3.146	651	655	658	rBV	239	153	0.01%	0.002%
12	3.172	661	663	667	rVB	334	177	0.01%	0.002%
13	3.191	667	669	670	rBV	349	143	0.01%	0.001%
14	3.288	696	699	703	rBV2	160	165	0.01%	0.002%
15	3.323	707	710	713	rVV2	251	171	0.01%	0.002%
16	3.368	719	724	726	rBV3	296	253	0.02%	0.003%
17	3.439	743	746	748	rBV2	402	274	0.02%	0.003%
18	3.471	753	756	760	rVB3	224	151	0.01%	0.002%
19	3.539	772	777	780	rBV2	266	259	0.02%	0.003%
20	3.638	807	808	813	rVB	428	171	0.01%	0.002%
21	3.912	882	893	940	rBV2	55840	248654	17.96%	2.521%
22	4.349	1015	1029	1066	rVB	173167	431305	31.16%	4.373%
23	4.597	1103	1106	1108	rBV2	296	206	0.01%	0.002%
24	4.680	1127	1132	1136	rBV3	558	639	0.05%	0.006%
25	4.815	1172	1174	1177	rBV	337	178	0.01%	0.002%
26	4.976	1220	1224	1225	rBV2	296	197	0.01%	0.002%
27	5.047	1230	1246	1275	rBV2	445305	1116401	80.65%	11.319%
28	5.346	1337	1339	1341	rBV2	312	143	0.01%	0.001%
29	5.442	1366	1369	1371	rVB2	361	214	0.02%	0.002%
30	5.461	1371	1375	1376	rBV	303	184	0.01%	0.002%
31	5.484	1379	1382	1386	rBV3	422	356	0.03%	0.004%
32	5.513	1387	1391	1392	rVV	319	196	0.01%	0.002%
33	5.616	1411	1423	1451	rBV	360237	739724	53.44%	7.500%
34	5.908	1502	1514	1537	rVV4	38371	92251	6.66%	0.935%
35	5.992	1537	1540	1543	rVB	606	317	0.02%	0.003%
36	6.072	1551	1565	1593	rBV	242805	503109	36.35%	5.101%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022263.D
 Acq On : 21 Sep 2021 03:50
 Operator : SY/MD
 Sample : M3778-01DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E4585DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.333	1641	1646	1648	rBV3	295	230	0.02%	0.002%
38	6.365	1652	1656	1659	rVB	374	276	0.02%	0.003%
39	6.391	1659	1664	1670	rBV2	319	242	0.02%	0.002%
40	6.461	1681	1686	1692	rBV2	254	280	0.02%	0.003%
41	6.548	1711	1713	1718	rBV2	334	287	0.02%	0.003%
42	6.580	1721	1723	1729	rVB2	432	252	0.02%	0.003%
43	6.651	1740	1745	1750	rBV2	293	286	0.02%	0.003%
44	6.812	1791	1795	1798	rVB2	372	226	0.02%	0.002%
45	6.876	1812	1815	1820	rBV2	245	271	0.02%	0.003%
46	6.934	1830	1833	1837	rBV3	163	148	0.01%	0.002%
47	6.989	1839	1850	1870	rBV2	114625	210608	15.21%	2.135%
48	7.317	1940	1952	1971	rBV	511733	878974	63.50%	8.912%
49	7.625	2038	2048	2071	rBV	75674	140174	10.13%	1.421%
50	7.783	2095	2097	2099	rVB2	485	190	0.01%	0.002%
51	7.850	2113	2118	2124	rVB4	595	684	0.05%	0.007%
52	7.892	2128	2131	2133	rBV	252	150	0.01%	0.002%
53	7.976	2144	2157	2184	rVV	829645	1384229	100.00%	14.034%
54	8.095	2184	2194	2237	rVV	243626	518773	37.48%	5.260%
55	8.558	2335	2338	2340	rBV3	479	239	0.02%	0.002%
56	8.603	2346	2352	2355	rBV3	373	433	0.03%	0.004%
57	8.645	2363	2365	2368	rBV2	308	201	0.01%	0.002%
58	8.690	2375	2379	2383	rVB2	370	298	0.02%	0.003%
59	8.712	2383	2386	2390	rVB3	381	207	0.01%	0.002%
60	8.760	2397	2401	2404	rBV2	297	253	0.02%	0.003%
61	8.854	2418	2430	2466	rBV	533730	886520	64.04%	8.988%
62	9.082	2497	2501	2503	rBV2	255	157	0.01%	0.002%
63	9.111	2506	2510	2514	rBV3	354	309	0.02%	0.003%
64	9.230	2544	2547	2549	rVB	343	176	0.01%	0.002%
65	9.259	2551	2556	2559	rBV	280	249	0.02%	0.003%
66	9.439	2601	2612	2615	rBV3	588	749	0.05%	0.008%
67	9.747	2705	2708	2710	rBV3	270	199	0.01%	0.002%
68	9.802	2723	2725	2729	rBV2	243	218	0.02%	0.002%
69	9.934	2762	2766	2767	rBV2	457	272	0.02%	0.003%
70	10.066	2802	2807	2808	rBV	188	157	0.01%	0.002%
71	10.130	2820	2827	2834	rVB4	1369	1955	0.14%	0.020%
72	10.217	2843	2854	2876	rBV	289087	463674	33.50%	4.701%
73	10.384	2901	2906	2911	rBV2	438	521	0.04%	0.005%
74	10.407	2911	2913	2916	rVB2	445	268	0.02%	0.003%
75	10.429	2916	2920	2926	rBV3	417	446	0.03%	0.005%
76	10.465	2926	2931	2935	rBV4	295	319	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022263.D
 Acq On : 21 Sep 2021 03:50
 Operator : SY/MD
 Sample : M3778-01DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E4585DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.545	2952	2956	2962	rVB3	640	632	0.05%	0.006%
78	10.680	2995	2998	3001	rBV2	272	241	0.02%	0.002%
79	10.747	3017	3019	3024	rVB	297	188	0.01%	0.002%
80	10.799	3031	3035	3040	rBV2	287	284	0.02%	0.003%
81	10.921	3066	3073	3082	rVV4	1759	2787	0.20%	0.028%
82	11.040	3107	3110	3114	rBV2	411	319	0.02%	0.003%
83	11.091	3121	3126	3128	rBV	285	218	0.02%	0.002%
84	11.146	3139	3143	3144	rBV3	549	388	0.03%	0.004%
85	11.252	3164	3176	3200	rBV	484192	765091	55.27%	7.757%
86	11.481	3245	3247	3250	rBV2	495	286	0.02%	0.003%
87	11.625	3280	3292	3318	rBV	468591	735925	53.16%	7.461%
88	11.889	3368	3374	3379	rBV3	275	433	0.03%	0.004%
89	12.992	3711	3717	3718	rBV2	391	334	0.02%	0.003%
90	13.046	3732	3734	3736	rVB	324	146	0.01%	0.001%
91	13.072	3740	3742	3745	rBV	279	174	0.01%	0.002%
92	13.390	3838	3841	3844	rBV2	224	156	0.01%	0.002%
93	13.532	3880	3885	3890	rBV2	347	442	0.03%	0.004%
94	13.603	3902	3907	3911	rBV2	421	388	0.03%	0.004%
95	13.648	3919	3921	3924	rBV2	249	185	0.01%	0.002%
96	13.947	4011	4014	4015	rBV2	268	151	0.01%	0.002%
97	14.033	4038	4041	4044	rBV3	431	342	0.02%	0.003%
98	14.233	4101	4103	4106	rBV2	283	157	0.01%	0.002%
99	14.259	4109	4111	4114	rVB	486	271	0.02%	0.003%
100	14.542	4194	4199	4202	rBV2	380	434	0.03%	0.004%




Sum of corrected areas: 9863256

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022263.D
Acq On : 21 Sep 2021 03:50
Operator : SY/MD
Sample : M3778-01DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
E4585DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

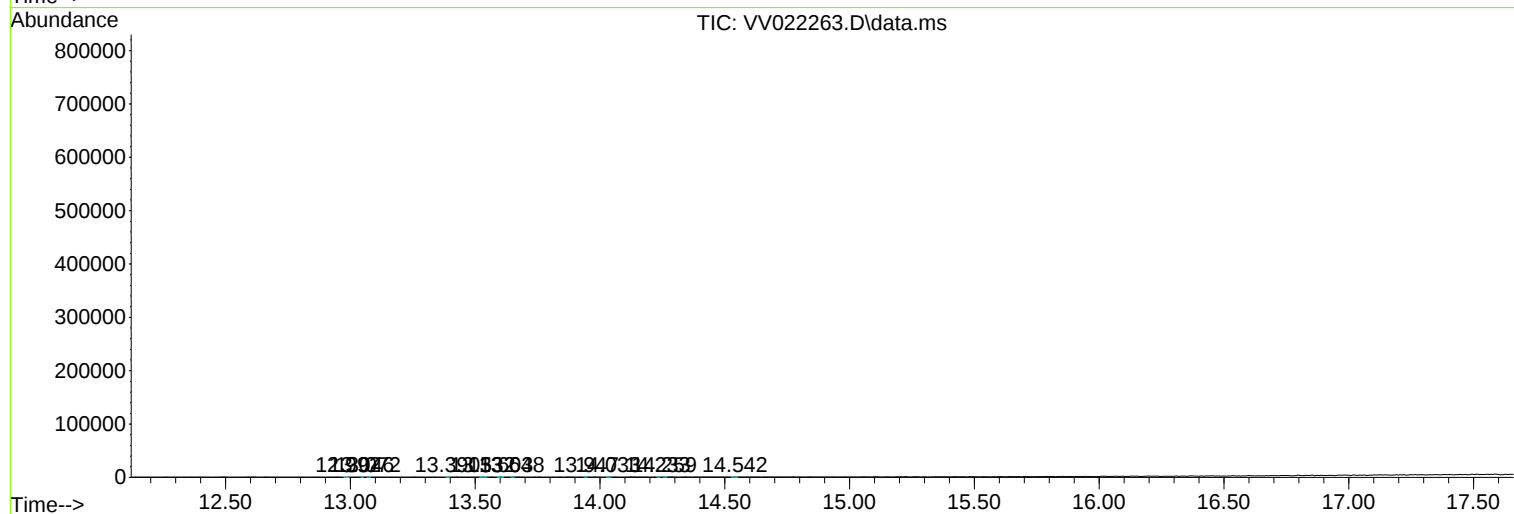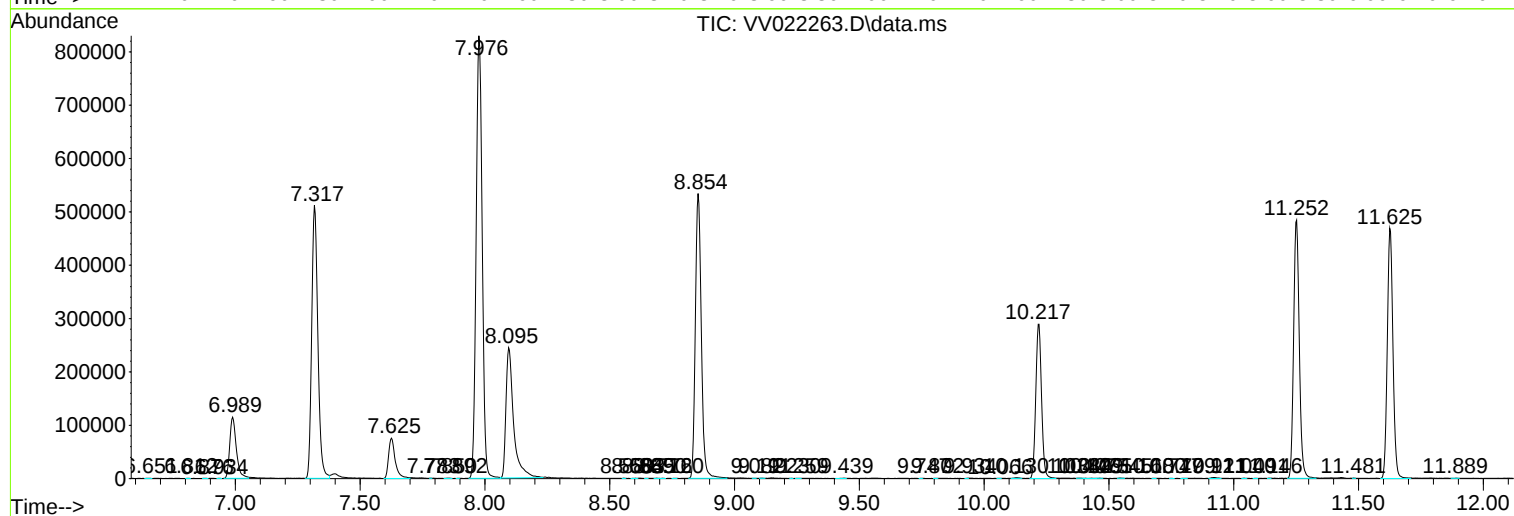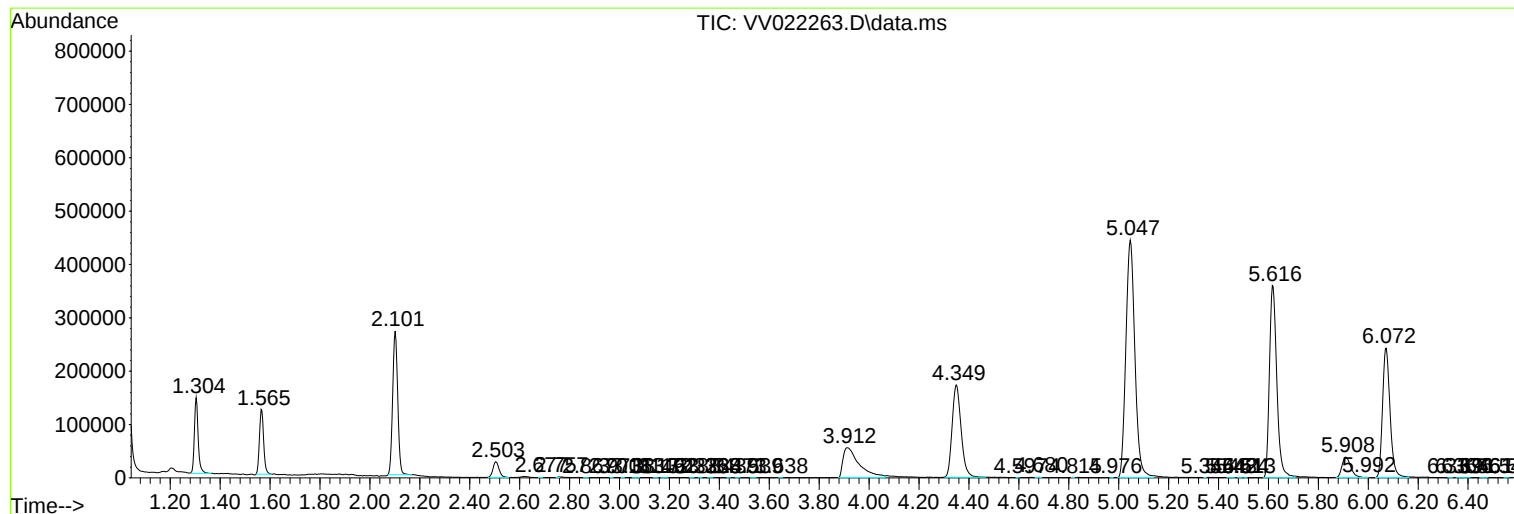

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022263.D
Acq On : 21 Sep 2021 03:50
Operator : SY/MD
Sample : M3778-01DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E4585DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022263.D
Acq On : 21 Sep 2021 03:50
Operator : SY/MD
Sample : M3778-01DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E4585DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
