

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022264.D
 Acq On : 21 Sep 2021 04:14
 Operator : SY/MD
 Sample : M3778-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E4586

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022264.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	127211	139251	1.97%	0.875%
2	1.564	157	163	176	rVB	115901	133073	1.88%	0.836%
3	2.098	319	329	341	rBV	259721	367256	5.18%	2.307%
4	2.384	416	418	421	rBV2	410	239	0.00%	0.002%
5	2.558	470	472	474	rVB	461	155	0.00%	0.001%
6	2.574	474	477	479	rBV3	407	265	0.00%	0.002%
7	2.760	526	535	541	rBV4	5125	8966	0.13%	0.056%
8	3.124	645	648	651	rVB3	481	261	0.00%	0.002%
9	3.156	651	658	660	rBV3	342	351	0.00%	0.002%
10	3.198	670	671	675	rBV2	299	176	0.00%	0.001%
11	3.217	675	677	684	rVB	239	239	0.00%	0.002%
12	3.291	697	700	705	rVB2	244	199	0.00%	0.001%
13	3.423	734	741	743	rBV2	387	389	0.01%	0.002%
14	3.539	773	777	781	rVB2	320	282	0.00%	0.002%
15	3.912	879	893	924	rBV2	96963	320751	4.53%	2.015%
16	4.272	1003	1005	1007	rBV2	515	299	0.00%	0.002%
17	4.349	1014	1029	1060	rBV	167764	418549	5.91%	2.630%
18	4.600	1102	1107	1113	rBV3	571	593	0.01%	0.004%
19	4.728	1144	1147	1152	rBV4	263	251	0.00%	0.002%
20	4.780	1158	1163	1164	rBV2	460	327	0.00%	0.002%
21	4.838	1178	1181	1184	rBV	364	169	0.00%	0.001%
22	4.854	1184	1186	1189	rBV3	303	197	0.00%	0.001%
23	5.047	1229	1246	1275	rBV2	441282	1093735	15.44%	6.872%
24	5.275	1312	1317	1324	rBV6	525	612	0.01%	0.004%
25	5.436	1363	1367	1369	rBV	497	329	0.00%	0.002%
26	5.455	1371	1373	1377	rVB2	387	235	0.00%	0.001%
27	5.516	1388	1392	1393	rVV2	390	176	0.00%	0.001%
28	5.616	1410	1423	1446	rBV	349803	706840	9.98%	4.441%
29	5.850	1494	1496	1499	rVB4	431	200	0.00%	0.001%
30	5.915	1502	1516	1545	rBV2	303741	626021	8.84%	3.933%
31	6.069	1552	1564	1591	rVB	232484	482858	6.82%	3.034%
32	6.391	1661	1664	1665	rVV	301	162	0.00%	0.001%
33	6.477	1689	1691	1692	rBV2	409	153	0.00%	0.001%
34	6.535	1703	1709	1711	rBV2	201	192	0.00%	0.001%
35	6.580	1719	1723	1726	rBV2	210	191	0.00%	0.001%
36	6.628	1732	1738	1741	rVB3	389	259	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022264.D
 Acq On : 21 Sep 2021 04:14
 Operator : SY/MD
 Sample : M3778-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E4586

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.654	1741	1746	1749	rBV	319	306	0.00%	0.002%
38	6.796	1788	1790	1795	rVB2	233	179	0.00%	0.001%
39	6.854	1804	1808	1812	rVB3	266	205	0.00%	0.001%
40	6.911	1823	1826	1828	rBV2	364	178	0.00%	0.001%
41	6.950	1833	1838	1839	rBV2	270	190	0.00%	0.001%
42	6.989	1839	1850	1872	rBV2	110858	206554	2.92%	1.298%
43	7.181	1906	1910	1913	rBV3	479	487	0.01%	0.003%
44	7.223	1921	1923	1927	rVB	494	284	0.00%	0.002%
45	7.252	1927	1932	1936	rBV3	377	364	0.01%	0.002%
46	7.278	1936	1940	1941	rBV3	320	188	0.00%	0.001%
47	7.317	1941	1952	1970	rBV	496550	856900	12.10%	5.384%
48	7.625	2036	2048	2070	rBV	75458	136993	1.93%	0.861%
49	7.863	2119	2122	2125	rBV3	370	213	0.00%	0.001%
50	7.911	2134	2137	2141	rVB2	374	305	0.00%	0.002%
51	7.976	2141	2157	2185	rBV	4285163	7084570	100.00%	44.510%
52	8.098	2186	2195	2236	rVB	222163	521597	7.36%	3.277%
53	8.773	2402	2405	2407	rBV3	447	269	0.00%	0.002%
54	8.853	2419	2430	2458	rBV	520134	850287	12.00%	5.342%
55	9.146	2517	2521	2524	rBV3	794	636	0.01%	0.004%
56	9.214	2538	2542	2543	rBV2	333	200	0.00%	0.001%
57	9.249	2550	2553	2556	rBV	368	175	0.00%	0.001%
58	9.284	2561	2564	2567	rBV2	330	180	0.00%	0.001%
59	9.429	2605	2609	2611	rBV	280	180	0.00%	0.001%
60	9.448	2614	2615	2619	rVB	351	163	0.00%	0.001%
61	9.474	2619	2623	2627	rBV2	333	262	0.00%	0.002%
62	9.548	2643	2646	2649	rBV2	257	226	0.00%	0.001%
63	9.593	2655	2660	2663	rBV2	468	397	0.01%	0.002%
64	9.612	2664	2666	2670	rVV3	395	308	0.00%	0.002%
65	9.718	2694	2699	2704	rBV3	246	293	0.00%	0.002%
66	9.805	2724	2726	2732	rVB2	263	163	0.00%	0.001%
67	9.834	2732	2735	2738	rBV2	219	189	0.00%	0.001%
68	9.953	2769	2772	2775	rBV3	385	257	0.00%	0.002%
69	10.127	2820	2826	2828	rBV2	525	556	0.01%	0.003%
70	10.220	2842	2855	2881	rBV	298789	478947	6.76%	3.009%
71	10.365	2897	2900	2902	rBV2	346	211	0.00%	0.001%
72	10.548	2954	2957	2958	rBV2	470	205	0.00%	0.001%
73	10.628	2977	2982	2984	rBV2	282	251	0.00%	0.002%
74	10.683	2995	2999	3003	rBV2	410	336	0.00%	0.002%
75	10.734	3010	3015	3017	rBV	213	156	0.00%	0.001%
76	10.757	3017	3022	3025	rBV2	228	242	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
 Data File : VV022264.D
 Acq On : 21 Sep 2021 04:14
 Operator : SY/MD
 Sample : M3778-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E4586

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

77	10.914	3069	3071	3073	rBV2	617	339	0.00%	0.002%
78	10.976	3086	3090	3093	rBV2	214	190	0.00%	0.001%
79	11.011	3098	3101	3103	rBV	309	218	0.00%	0.001%
80	11.056	3111	3115	3119	rBV3	422	417	0.01%	0.003%
81	11.117	3130	3134	3138	rVB2	302	238	0.00%	0.001%
82	11.143	3138	3142	3143	rBV	529	305	0.00%	0.002%
83	11.252	3165	3176	3200	rBV	472928	730226	10.31%	4.588%
84	11.461	3239	3241	3245	rBV2	347	242	0.00%	0.002%
85	11.538	3257	3265	3276	rBV2	5758	9751	0.14%	0.061%
86	11.628	3281	3293	3312	rVV	454807	718046	10.14%	4.511%
87	11.873	3365	3369	3372	rBV2	294	268	0.00%	0.002%
88	11.937	3385	3389	3390	rBV	355	163	0.00%	0.001%
89	12.316	3503	3507	3508	rBV	267	173	0.00%	0.001%
90	12.352	3512	3518	3526	rVV6	3177	4484	0.06%	0.028%
91	12.390	3526	3530	3534	rVB2	418	431	0.01%	0.003%
92	12.763	3643	3646	3648	rVB2	390	170	0.00%	0.001%
93	13.262	3799	3801	3804	rBV	410	242	0.00%	0.002%
94	13.474	3863	3867	3868	rBV2	308	228	0.00%	0.001%
95	13.577	3894	3899	3906	rVB2	488	610	0.01%	0.004%
96	13.686	3929	3933	3937	rBV3	369	311	0.00%	0.002%
97	13.943	4009	4013	4015	rBV2	474	374	0.01%	0.002%
98	14.027	4037	4039	4042	rBV2	235	160	0.00%	0.001%
99	14.098	4059	4061	4064	rVB	328	196	0.00%	0.001%
100	14.217	4096	4098	4103	rVB2	455	206	0.00%	0.001%




Sum of corrected areas: 15916791

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022264.D
Acq On : 21 Sep 2021 04:14
Operator : SY/MD
Sample : M3778-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E4586

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

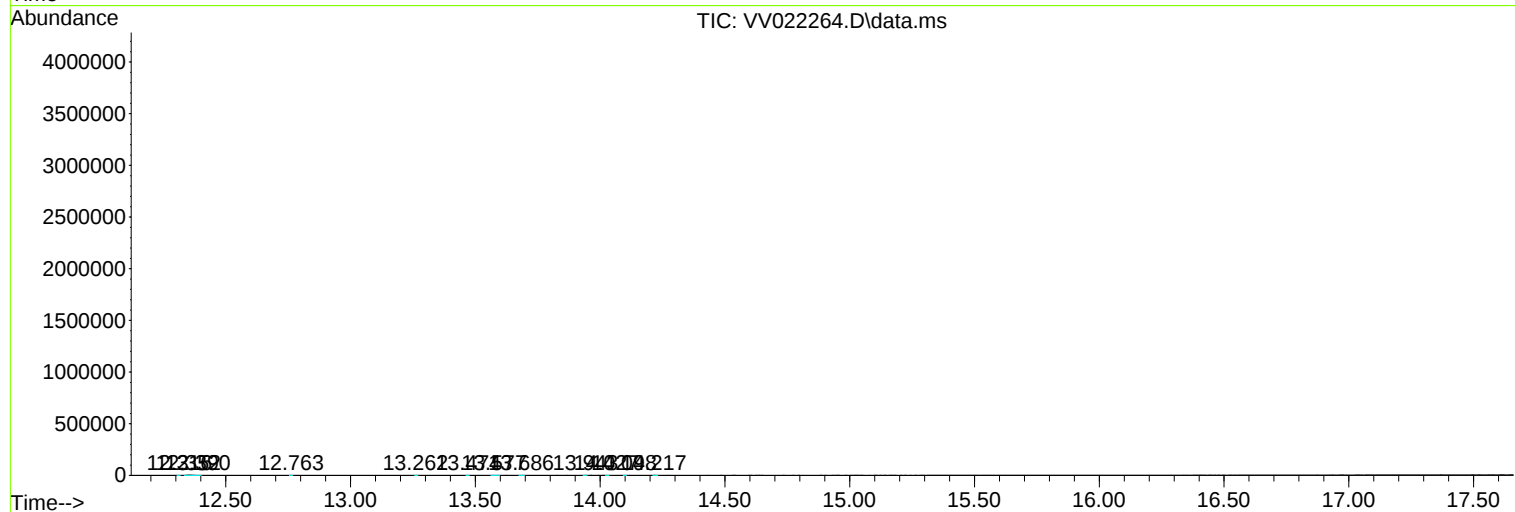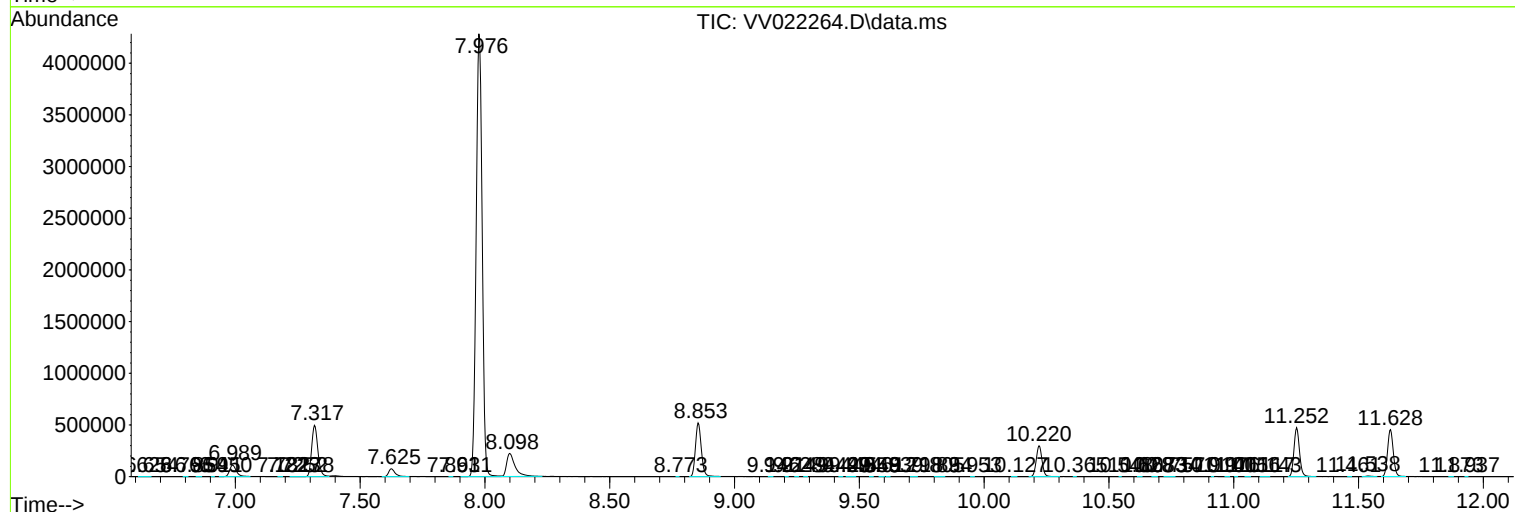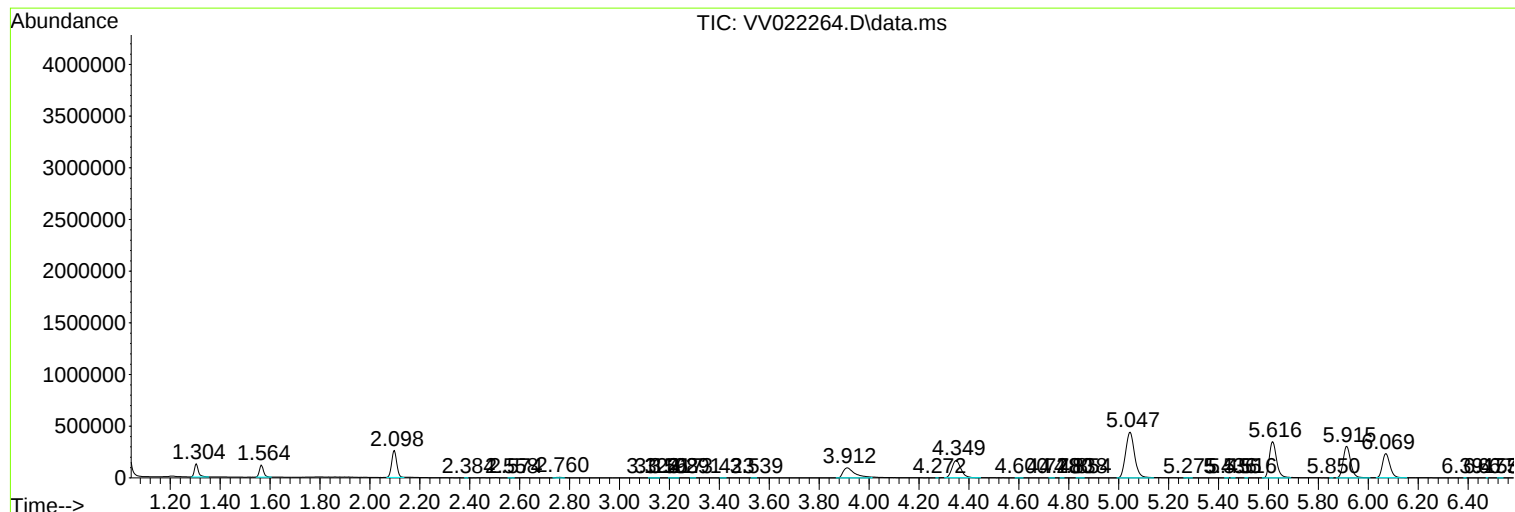

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022264.D
Acq On : 21 Sep 2021 04:14
Operator : SY/MD
Sample : M3778-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E4586

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022264.D
Acq On : 21 Sep 2021 04:14
Operator : SY/MD
Sample : M3778-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E4586

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
