
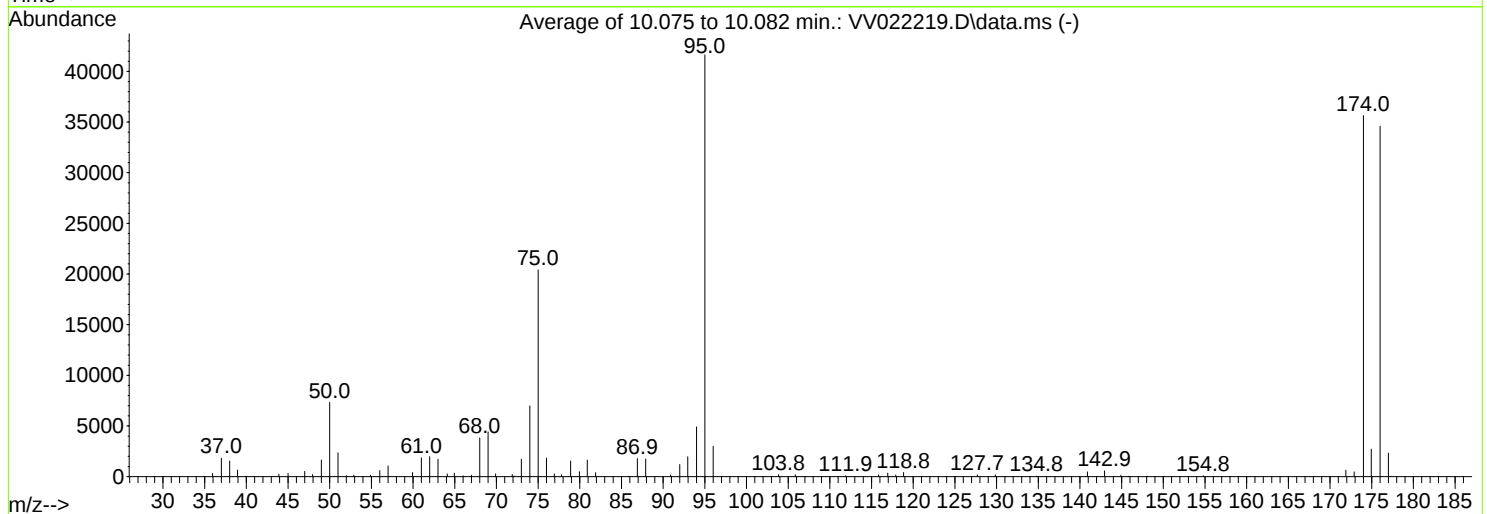


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092021\
Data File : VV022219.D
Acq On : 20 Sep 2021 09:02
Operator : SY/MD
Sample : BFB233
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB233

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Title : VOC Analysis
Last Update : Wed Sep 22 01:12:58 2021

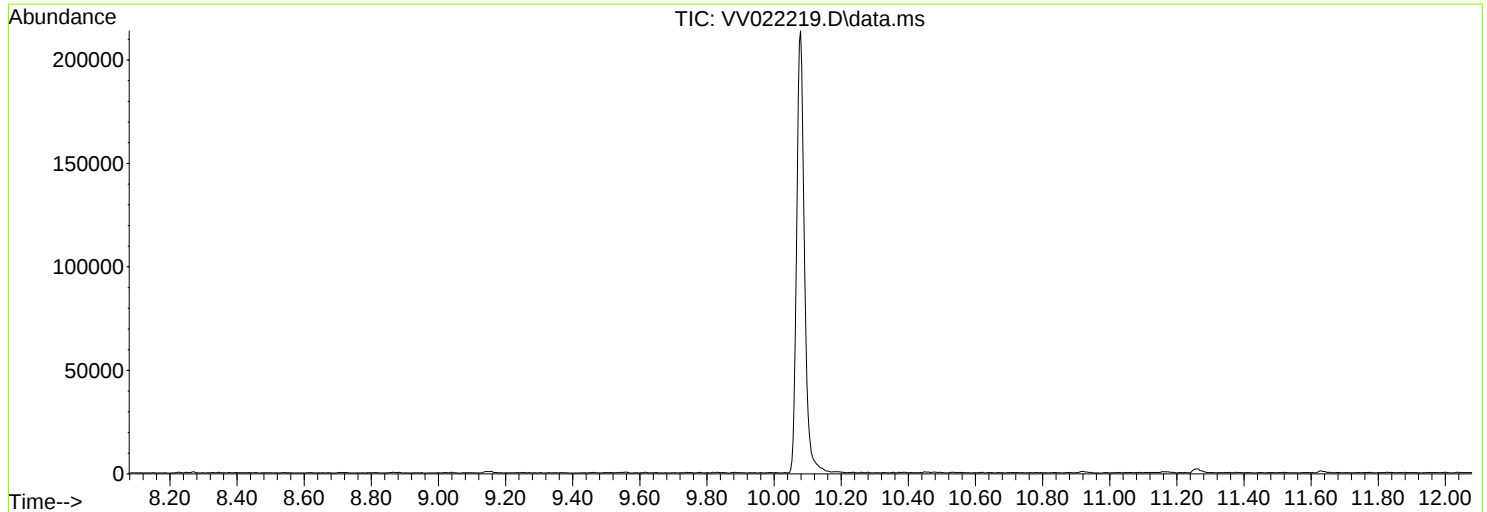

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	7322	PASS
75	95	30	80	49.0	20413	PASS
95	95	100	100	100.0	41632	PASS
96	95	5	9	7.2	3009	PASS
173	174	0.00	2	1.3	470	PASS
174	95	50	120	85.6	35648	PASS
175	174	5	9	7.6	2713	PASS
176	174	95	105	97.0	34581	PASS
177	176	5	10	6.7	2319	PASS

Scan 2799 (10.040 min): VV022219.D\data.ms
BFB233

m/z	Abundance
39.90	164.0
43.90	343.0

Instrument :
MSVOA_V
ClientSampleId :
BFB233

m/z	Abundance
36.00	324.0
37.00	1850.0
38.00	1562.0
38.90	644.0
39.90	180.0
44.00	558.0
45.00	330.0
47.00	470.0
47.90	222.0
49.00	1678.0
50.00	7686.0
51.00	2454.0
52.00	154.0
52.90	132.0
54.90	139.0
56.00	638.0
57.00	1094.0
60.00	407.0
61.00	1922.0
62.00	1958.0
63.00	1822.0
64.10	298.0
64.90	355.0
66.00	107.0
67.00	154.0
68.00	3817.0
69.00	4543.0
69.90	260.0
71.90	242.0
73.00	1868.0
74.00	7060.0
75.00	20600.0
76.00	1841.0
76.90	216.0
77.80	185.0
78.90	1635.0
79.90	529.0
80.90	1674.0
81.90	416.0
85.80	115.0
86.90	1971.0
87.90	1987.0
90.90	204.0
92.00	1302.0
92.90	1979.0
94.00	5100.0
95.00	42248.0
96.00	2970.0
103.90	219.0
105.80	193.0
111.90	114.0
115.80	170.0
117.00	320.0
117.90	155.0
118.80	394.0
127.70	203.0
129.80	202.0
134.80	120.0
140.90	500.0
143.00	530.0
144.90	129.0
148.10	126.0
171.90	632.0
172.90	471.0
174.00	35456.0
175.00	2768.0
176.00	33760.0
177.00	2482.0

Instrument :
MSVOA_V
ClientSampleId :
BFB233

m/z	Abundance
35.90	326.0
37.00	1867.0
38.00	1598.0
39.00	657.0
39.90	218.0
43.90	581.0
45.00	351.0
47.00	530.0
47.90	204.0
49.00	1737.0
50.00	7605.0
51.00	2455.0
52.00	135.0
52.90	160.0
54.90	147.0
56.00	609.0
57.00	1102.0
59.90	409.0
61.00	1923.0
62.00	2066.0
63.00	1730.0
64.10	297.0
64.90	369.0
66.00	108.0
67.00	164.0
68.00	3946.0
69.00	4624.0
69.90	271.0
71.90	222.0
73.00	1753.0
74.00	7209.0
75.00	21216.0
76.00	1902.0
76.90	289.0
77.80	178.0
78.90	1595.0
80.00	506.0
80.90	1741.0
81.90	429.0
86.90	1863.0
87.90	1747.0
90.90	179.0
92.00	1230.0
92.90	2049.0
94.00	5067.0
95.00	43200.0
96.00	3126.0
103.80	219.0
105.80	202.0
111.90	116.0
115.90	168.0
116.90	364.0
117.90	158.0
118.80	432.0
127.70	200.0
129.80	182.0
140.90	486.0
142.90	586.0
144.90	152.0
154.80	125.0
171.90	658.0
172.90	495.0
174.00	36776.0
175.00	2797.0
176.00	35776.0
177.00	2389.0

Instrument :
MSVOA_V
ClientSampleId :
BFB233

m/z	Abundance
35.90	317.0
37.00	1726.0
38.00	1503.0
39.00	625.0
39.90	211.0
43.90	582.0
45.00	338.0
47.00	561.0
48.00	203.0
49.00	1533.0
50.00	6675.0
51.00	2132.0
52.90	149.0
54.90	162.0
56.00	576.0
57.00	1001.0
59.90	420.0
61.00	1759.0
62.00	1901.0
63.00	1611.0
64.10	226.0
65.00	338.0
67.00	133.0
68.00	3711.0
69.00	4110.0
69.90	262.0
71.90	197.0
72.10	197.0
73.00	1552.0
74.00	6689.0
75.00	19424.0
76.00	1762.0
77.00	313.0
77.80	204.0
78.90	1432.0
79.90	437.0
80.90	1495.0
81.90	364.0
86.90	1499.0
87.90	1492.0
90.90	166.0
92.00	1071.0
93.00	1872.0
94.00	4579.0
95.00	39448.0
96.00	2931.0
103.80	171.0
105.90	185.0
115.90	177.0
116.90	364.0
117.90	147.0
118.90	422.0
127.70	142.0
129.90	142.0
140.90	443.0
142.90	600.0
144.90	134.0
145.80	113.0
154.80	157.0
171.90	587.0
172.90	444.0
174.00	34712.0
174.90	2573.0
176.00	34208.0
177.00	2087.0

Instrument :
MSVOA_V
ClientSampleId :
BFB233